

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041468.D
 Acq On : 24 Aug 2023 16:45
 Operator : MA/JU
 Sample : 04105-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH8X9

Quant Time: Aug 24 18:36:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.118	152	10477	0.400	ng/ul	0.00
4) Naphthalene-d8	10.949	136	30689	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.759	164	14102	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.514	188	24825	0.400	ng/ul	0.00
17) Chrysene-d12	21.705	240	8339	0.400	ng/ul	# 0.00
23) Perylene-d12	24.278	264	9740	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	58948	4.446	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.528	152	10894	0.269	ng/ul	0.00
18) Fluoranthene-d10	19.533	212	13059	0.355	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	1157	0.085	ng/ul#	72
20) Pyrene	19.905	202	3740	0.048	ng/ul#	1
26) Benzo(a)pyrene	24.111	252	6166	0.112	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041468.D
Acq On : 24 Aug 2023 16:45
Operator : MA/JU
Sample : 04105-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH8X9

Quant Time: Aug 24 18:36:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration




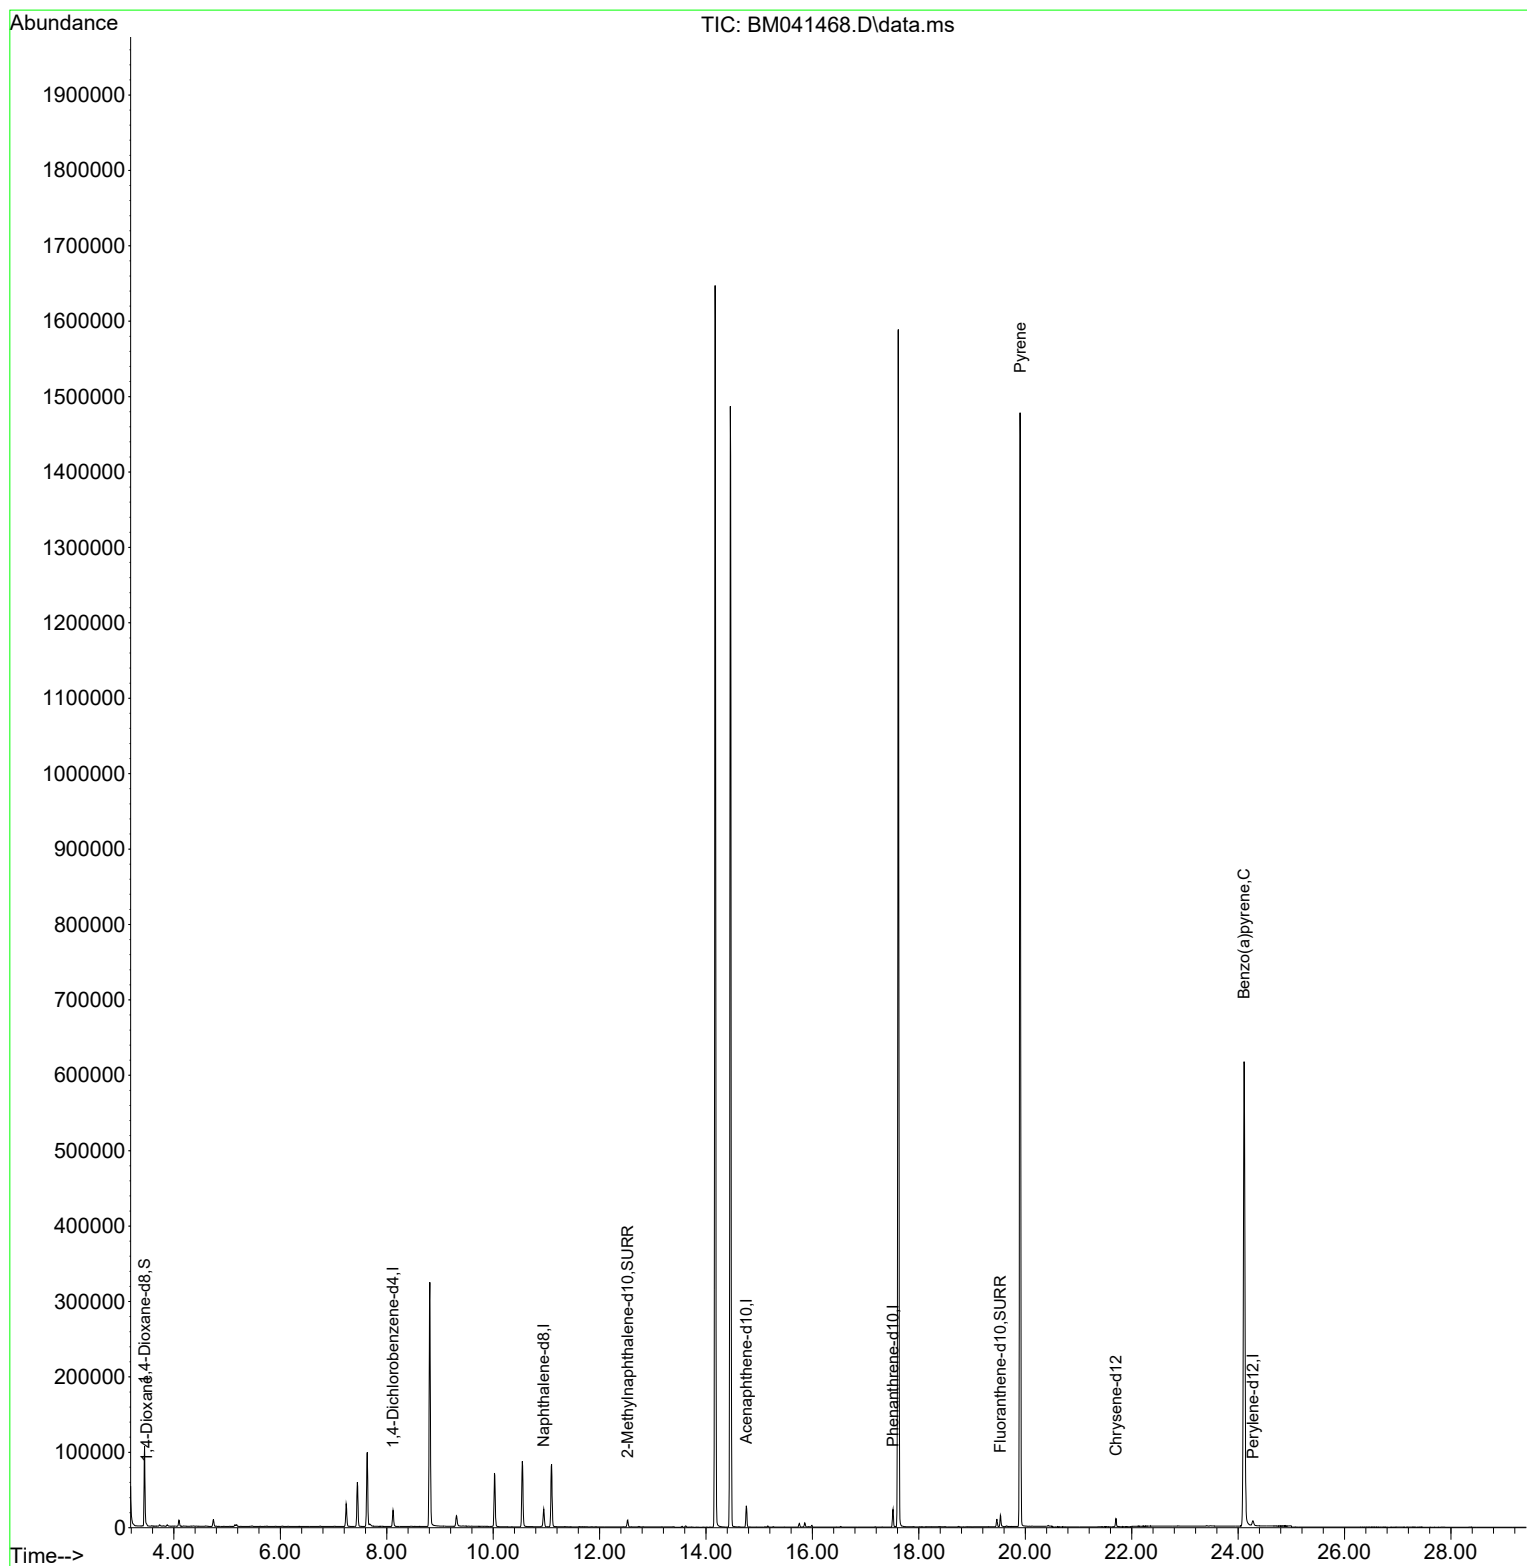


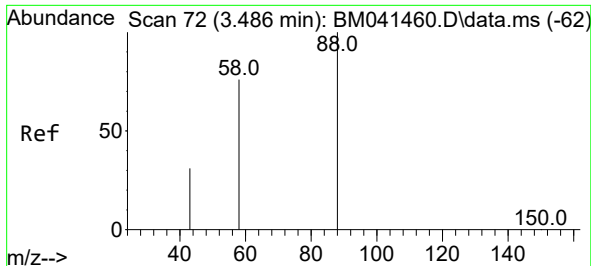

#2
1,4-Dioxane
Concen: 0.085 ng/ul
RT: 3.486 min Scan# 71
Delta R.T. -0.000 min
Lab File: BM041468.D
Acq: 24 Aug 2023 16:45




Instrument :
BNA_M
ClientSampleId :
BH8X9


Tgt Ion: 88 Resp: 1157
Ion Ratio Lower Upper
88 100
43 72.3 35.4 53.2#
58 56.0 57.3 85.9#

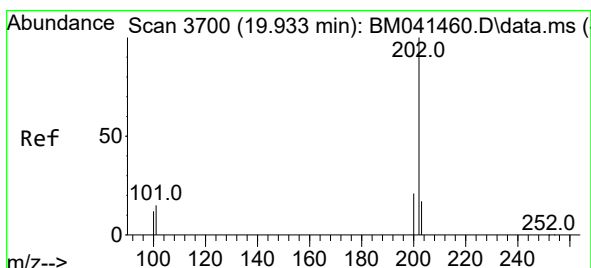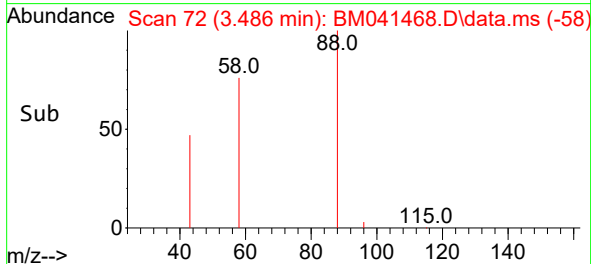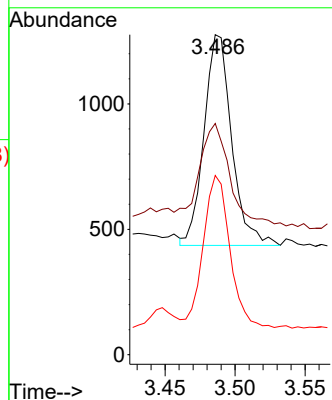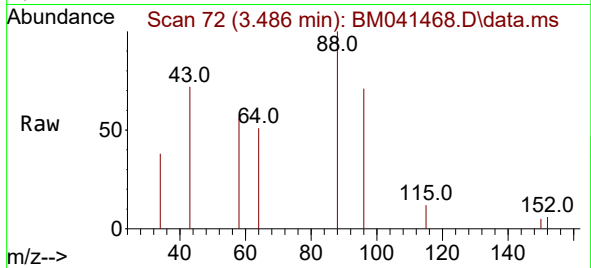

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.905 min Scan# 3694
Delta R.T. -0.028 min
Lab File: BM041468.D
Acq: 24 Aug 2023 16:45


Tgt Ion: 202 Resp: 3740
Ion Ratio Lower Upper
202 100
101 139.0 12.2 18.2#
100 958.1 9.8 14.8#

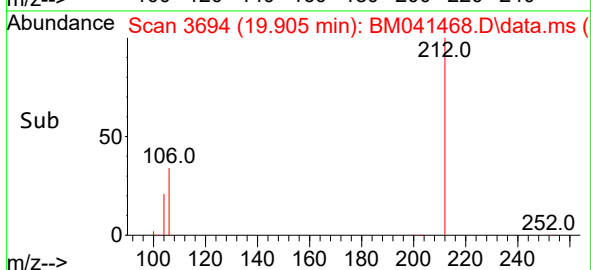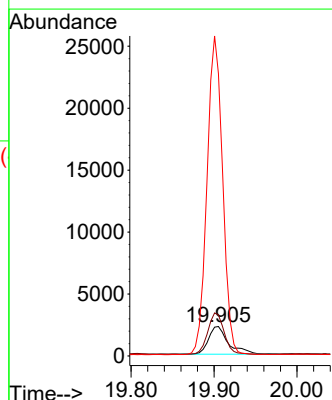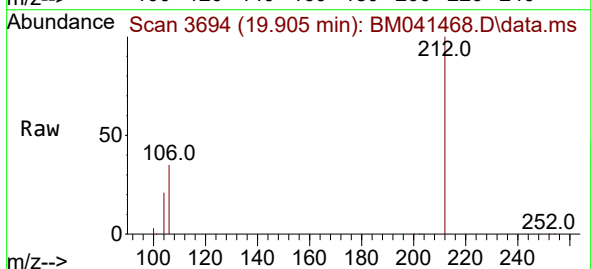

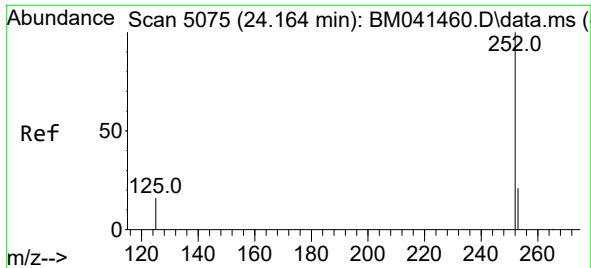

#26
Benzo(a)pyrene
Concen: 0.112 ng/ul
RT: 24.111 min Scan# 50
Delta R.T. -0.053 min
Lab File: BM041468.D
Acq: 24 Aug 2023 16:45

Instrument :
BNA_M
ClientSampleId :
BH8X9

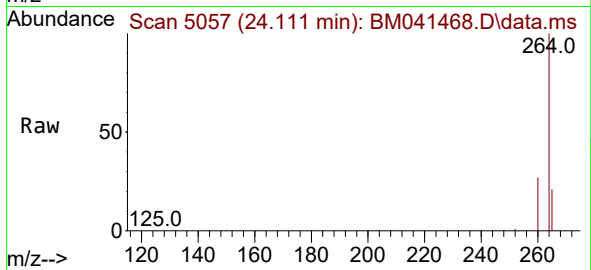

Tgt Ion:252 Resp: 6166
Ion Ratio Lower Upper
252 100
253 37.2 19.5 29.3#
125 32.1 16.0 24.0#

