

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082423\  
 Data File : BM041477.D  
 Acq On : 24 Aug 2023 22:53  
 Operator : MA/JU  
 Sample : 04105-18  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BH8X3

Quant Time: Aug 25 02:33:19 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM082423.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Aug 24 18:34:12 2023  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 8.119  | 152  | 11709    | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.950 | 136  | 35285    | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.754 | 164  | 17550    | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.510 | 188  | 32267    | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.700 | 240  | 9533     | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 24.269 | 264  | 9927     | 0.400 | ng/ul  | -0.01    |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.448  | 96   | 71712    | 4.839 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.523 | 152  | 14803    | 0.318 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.534 | 212  | 18474    | 0.439 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 2) 1,4-Dioxane              | 3.486  | 88   | 1825     | 0.120 | ng/ul# | 80       |
| 12) Fluorene                | 15.749 | 166  | 5926     | 0.072 | ng/ul# | 13       |
| 20) Pyrene                  | 19.901 | 202  | 5153     | 0.058 | ng/ul# | 1        |
| 26) Benzo(a)pyrene          | 24.103 | 252  | 7492     | 0.134 | ng/ul# | 77       |
| -----                       |        |      |          |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082423\  
Data File : BM041477.D  
Acq On : 24 Aug 2023 22:53  
Operator : MA/JU  
Sample : 04105-18  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BH8X3

Quant Time: Aug 25 02:33:19 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM082423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 24 18:34:12 2023  
Response via : Initial Calibration




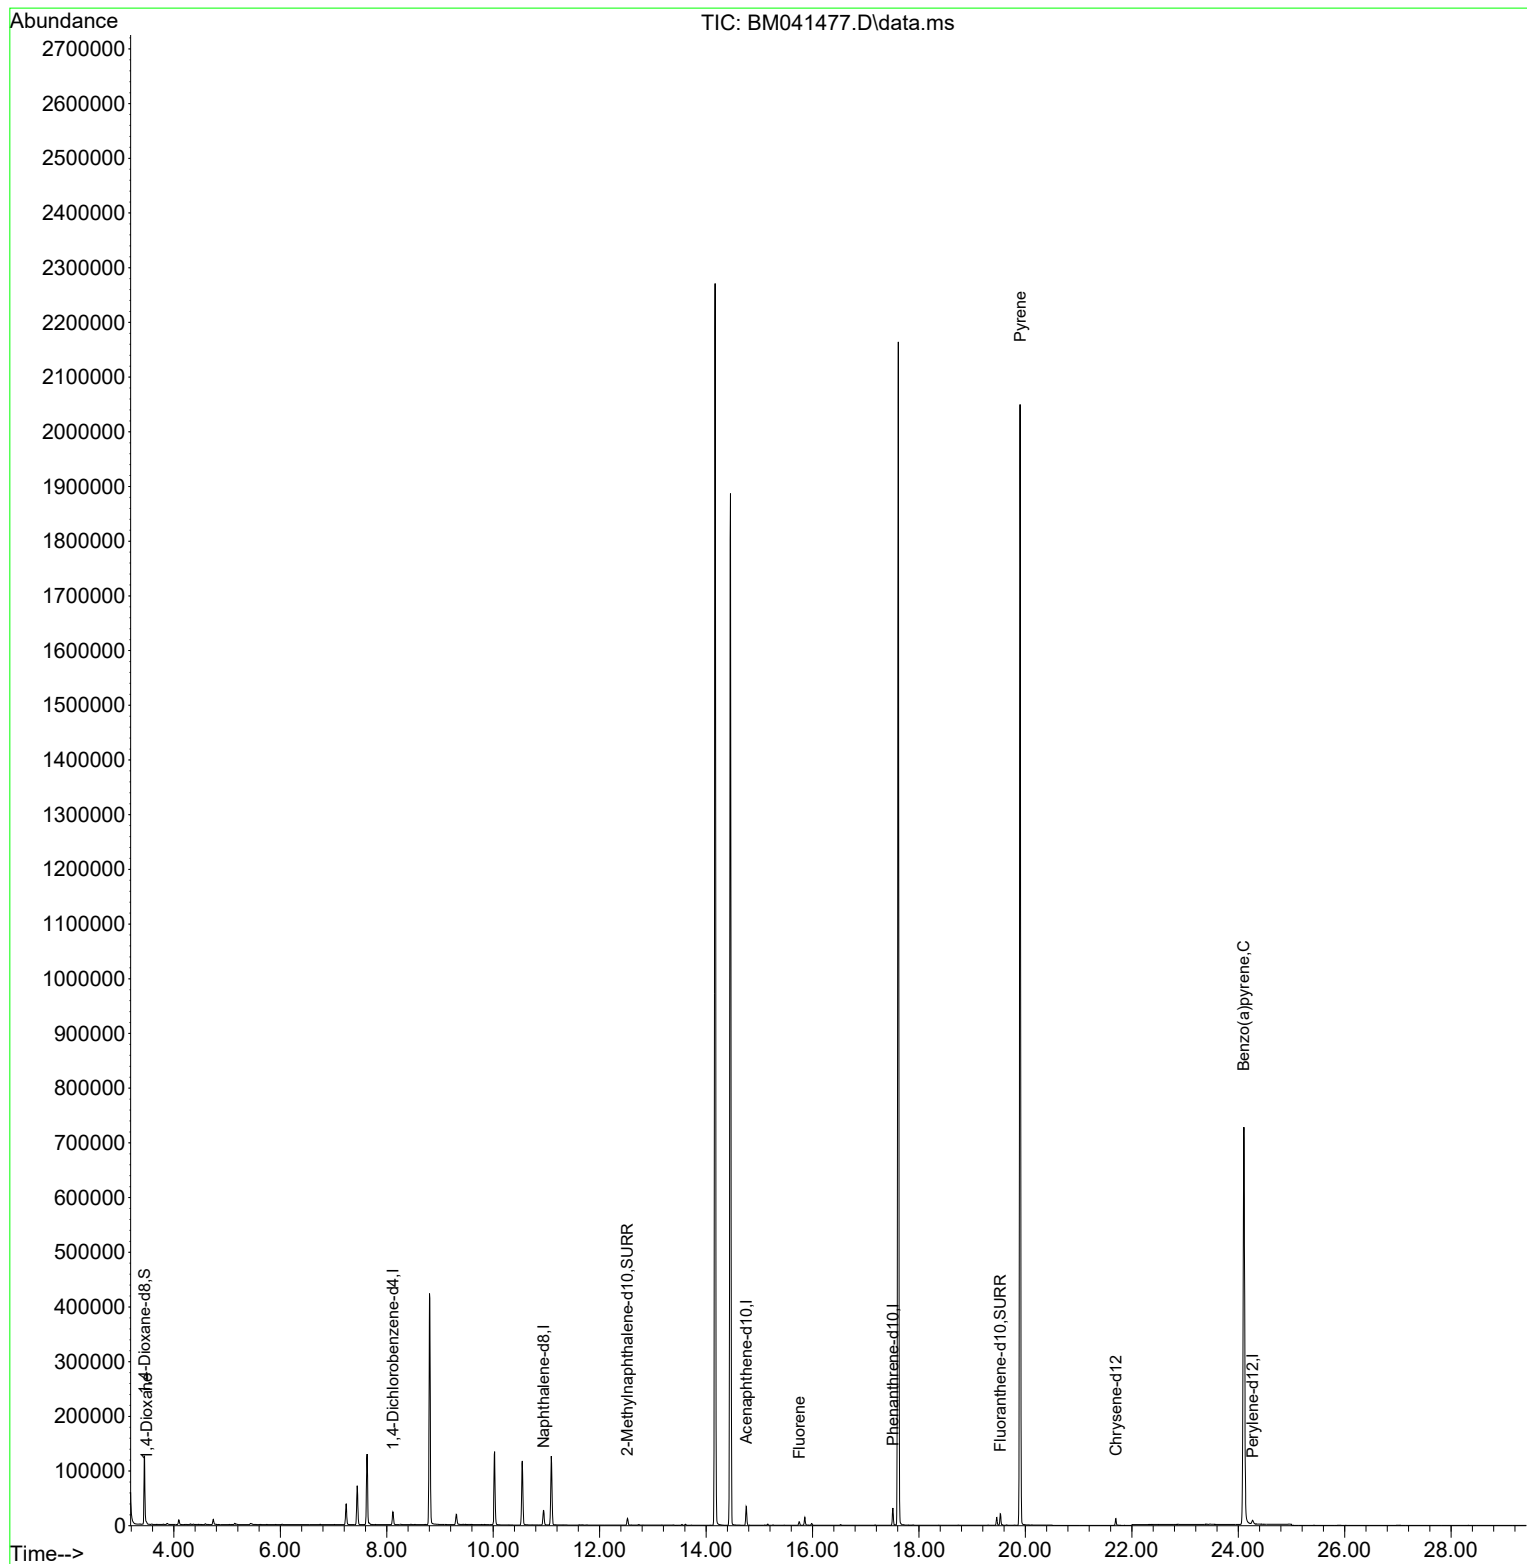


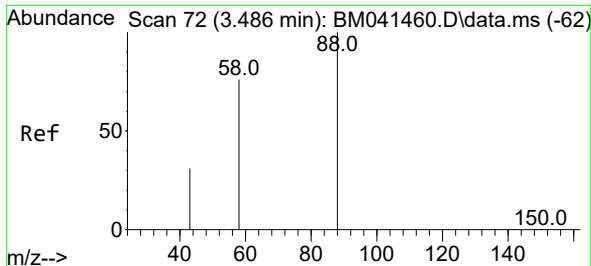

#2  
1,4-Dioxane  
Concen: 0.120 ng/ul  
RT: 3.486 min Scan# 71  
Delta R.T. 0.000 min  
Lab File: BM041477.D  
Acq: 24 Aug 2023 22:53




Instrument :  
BNA\_M  
ClientSampleId :  
BH8X3


Tgt Ion: 88 Resp: 1825  
Ion Ratio Lower Upper  
88 100  
43 67.0 35.4 53.2#  
58 62.0 57.3 85.9

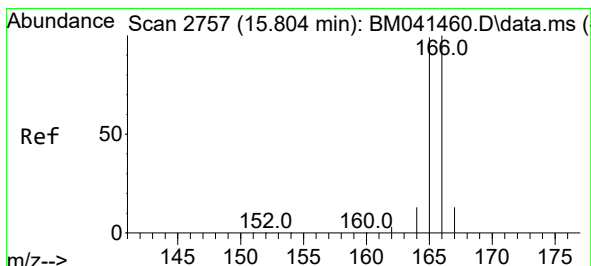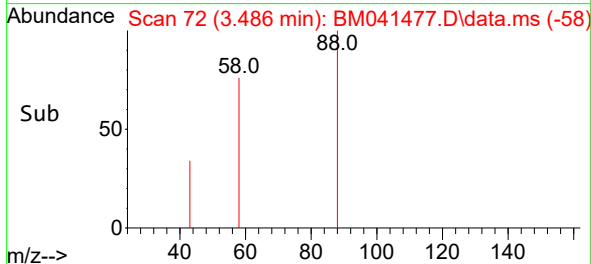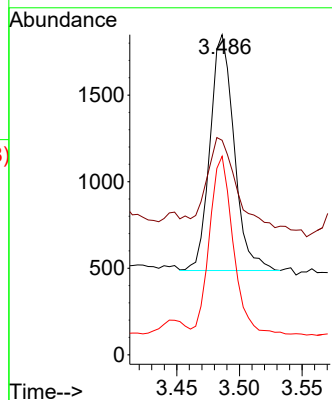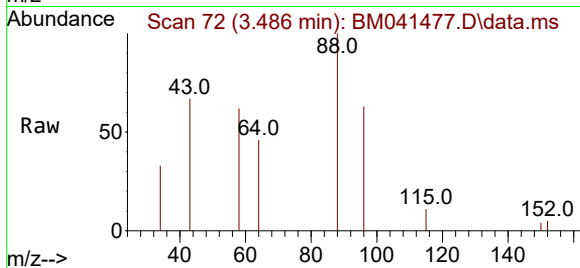

#12  
Fluorene  
Concen: 0.072 ng/ul  
RT: 15.749 min Scan# 2745  
Delta R.T. -0.055 min  
Lab File: BM041477.D  
Acq: 24 Aug 2023 22:53

Tgt Ion: 166 Resp: 5926  
Ion Ratio Lower Upper  
166 100  
165 6.0 79.4 119.2#  
167 31.1 11.0 16.6#


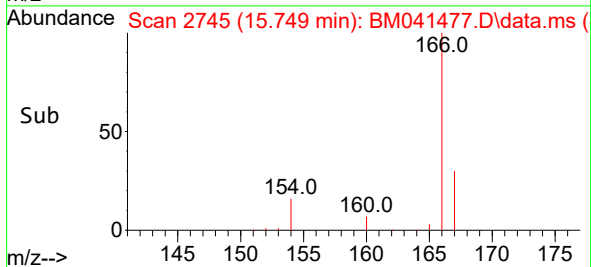
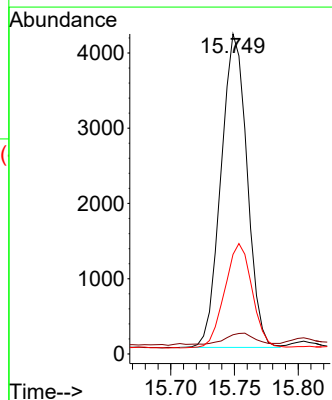
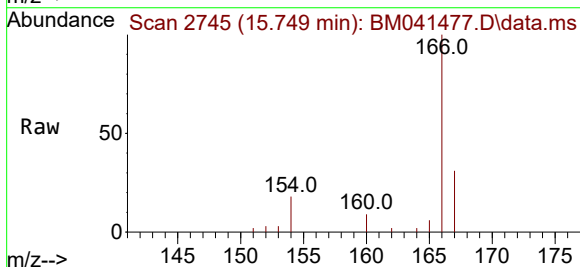


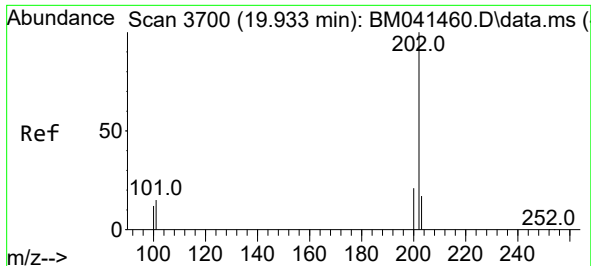

#20  
Pyrene  
Concen: 0.058 ng/ul  
RT: 19.901 min Scan# 3693  
Delta R.T. -0.032 min  
Lab File: BM041477.D  
Acq: 24 Aug 2023 22:53

Instrument :  
BNA\_M  
ClientSampleId :  
BH8X3

Tgt Ion:202 Resp: 5153  
Ion Ratio Lower Upper  
202 100  
101 153.4 12.2 18.2#  
100 1124.2 9.8 14.8#

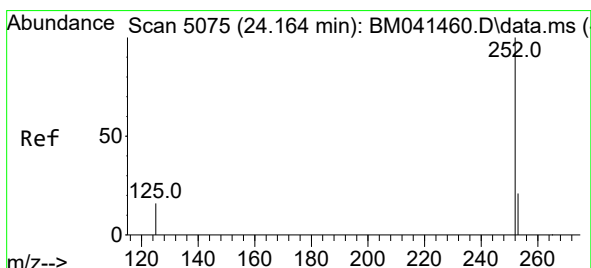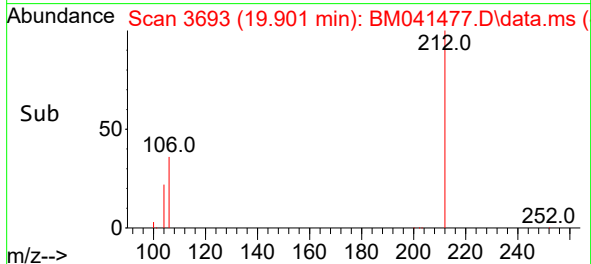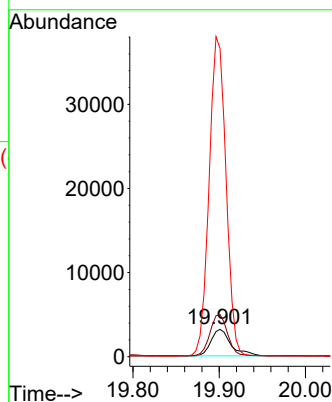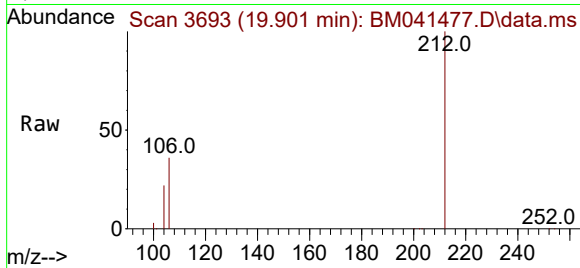

#26  
Benzo(a)pyrene  
Concen: 0.134 ng/ul  
RT: 24.103 min Scan# 5054  
Delta R.T. -0.061 min  
Lab File: BM041477.D  
Acq: 24 Aug 2023 22:53

Tgt Ion:252 Resp: 7492  
Ion Ratio Lower Upper  
252 100  
253 35.1 19.5 29.3#  
125 31.8 16.0 24.0#

