

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041491.D
 Acq On : 25 Aug 2023 10:48
 Operator : MA/JU
 Sample : 04105-15
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH968

Quant Time: Aug 26 00:17:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	14847	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	45103	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.754	164	25316	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	48034	0.400	ng/ul #	0.00
17) Chrysene-d12	21.699	240	16699	0.400	ng/ul	0.00
23) Perylene-d12	24.269	264	16346	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	91908	4.891	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	20258	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.529	212	30976	0.421	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.482	88	505	0.026	ng/ul#	52
20) Pyrene	19.928	202	8907	0.058	ng/ul#	89
26) Benzo(a)pyrene	24.105	252	10787	0.117	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041491.D
Acq On : 25 Aug 2023 10:48
Operator : MA/JU
Sample : 04105-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH968

Quant Time: Aug 26 00:17:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration




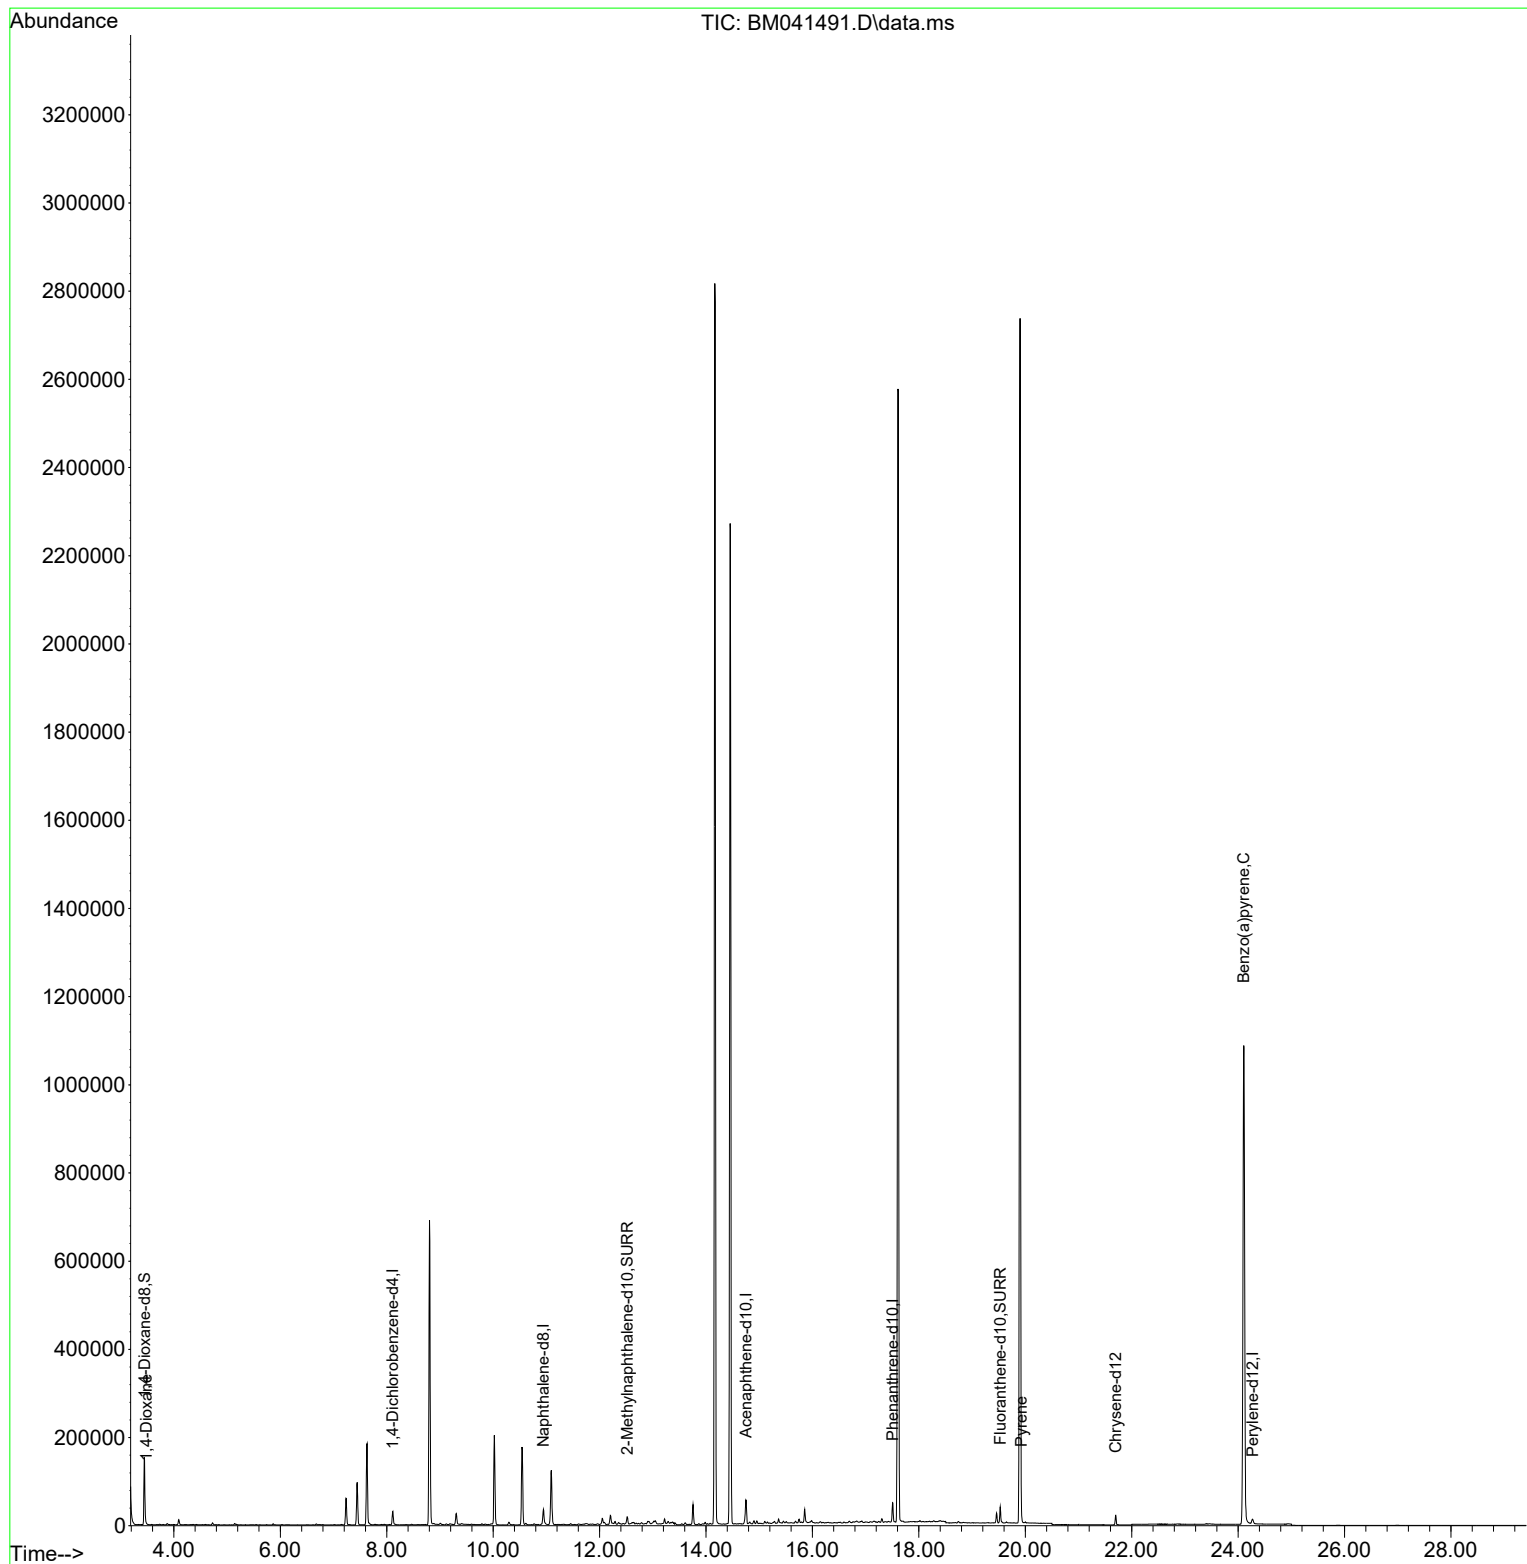


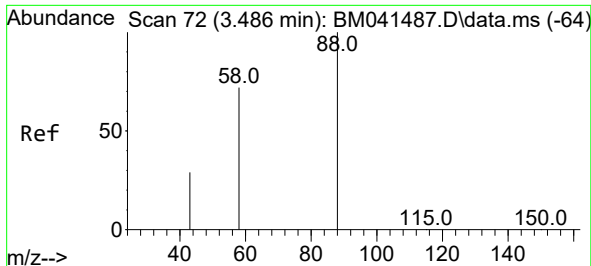

#2
1,4-Dioxane
Concen: 0.026 ng/ul
RT: 3.482 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM041491.D
Acq: 25 Aug 2023 10:48




Instrument :
BNA_M
ClientSampleId :
BH968


Tgt Ion: 88 Resp: 505
Ion Ratio Lower Upper
88 100
43 94.0 35.4 53.2#
58 46.0 57.3 85.9#

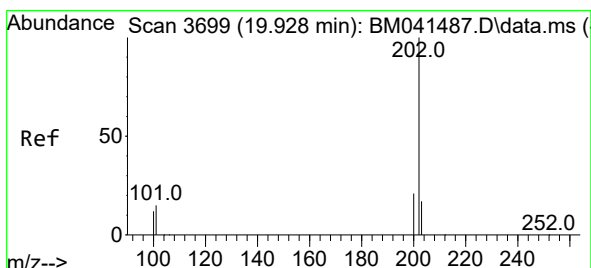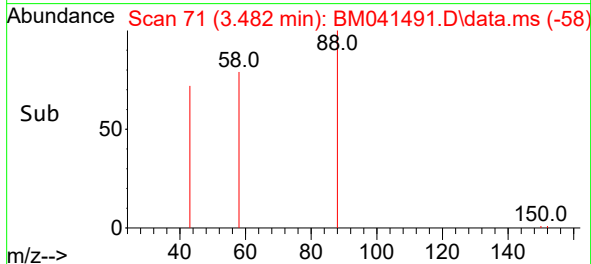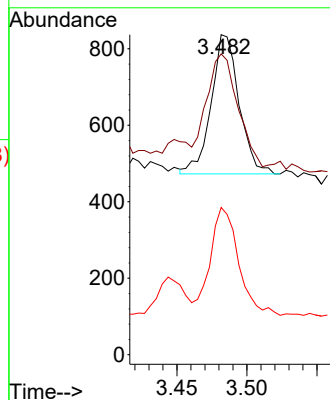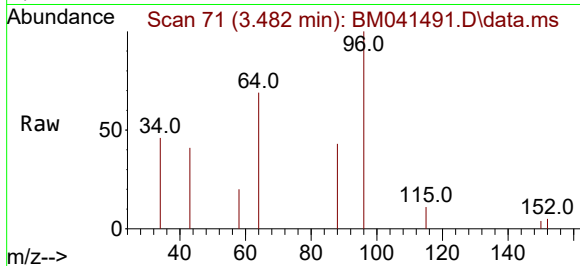

#20
Pyrene
Concen: 0.058 ng/ul
RT: 19.928 min Scan# 3699
Delta R.T. -0.005 min
Lab File: BM041491.D
Acq: 25 Aug 2023 10:48


Tgt Ion: 202 Resp: 8907
Ion Ratio Lower Upper
202 100
101 19.4 12.2 18.2#
100 17.4 9.8 14.8#

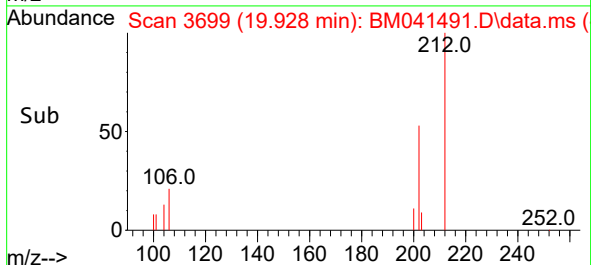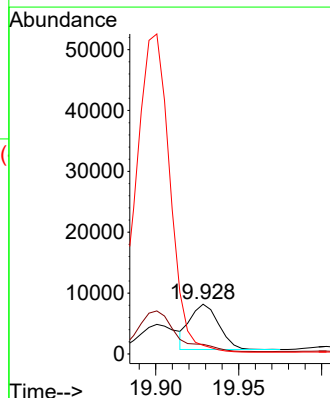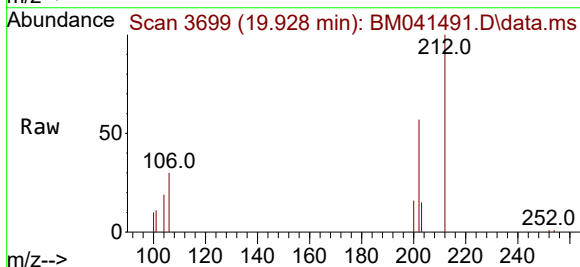

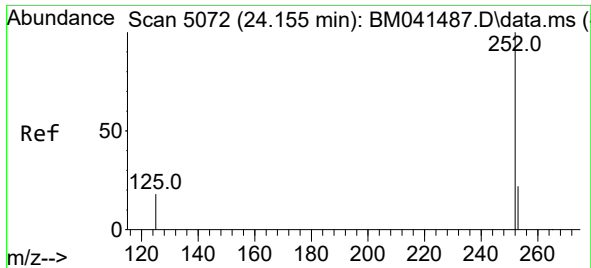

#26
Benzo(a)pyrene
Concen: 0.117 ng/ul
RT: 24.105 min Scan# 50
Delta R.T. -0.059 min
Lab File: BM041491.D
Acq: 25 Aug 2023 10:48

Instrument :
BNA_M
ClientSampleId :
BH968

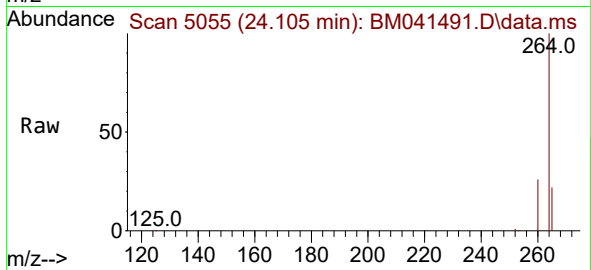

Tgt Ion:252 Resp: 10787
Ion Ratio Lower Upper
252 100
253 35.0 19.5 29.3#
125 31.0 16.0 24.0#

