

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041503.D
 Acq On : 25 Aug 2023 20:59
 Operator : MA/JU
 Sample : 04037-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYH1

Quant Time: Aug 26 00:18:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	11408	0.400	ng/ul	0.00
4) Naphthalene-d8	10.950	136	32156	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	16021	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	30183	0.400	ng/ul	0.00
17) Chrysene-d12	21.697	240	11968	0.400	ng/ul	# 0.00
23) Perylene-d12	24.269	264	12946	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	59992	4.155	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	9336	0.220	ng/ul	0.00
18) Fluoranthene-d10	19.529	212	13550	0.257	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.999	128	3447	0.036	ng/ul#	88
7) 2-Methylnaphthalene	12.594	142	2037	0.035	ng/ul	100
8) 1-Methylnaphthalene	12.814	142	1430	0.024	ng/ul	99
15) Phenanthrene	17.552	178	7104	0.064	ng/ul#	90
19) Fluoranthene	19.561	202	7378	0.067	ng/ul#	91
20) Pyrene	19.929	202	7691	0.069	ng/ul#	92
21) Benzo(a)anthracene	21.682	228	2506	0.032	ng/ul#	40
22) Chrysene	21.734	228	3047	0.036	ng/ul#	54
24) Benzo(b)fluoranthene	23.468	252	5374	0.061	ng/ul#	1
26) Benzo(a)pyrene	24.155	252	2546	0.035	ng/ul#	1
27) Indeno(1,2,3-cd)pyrene	26.988	276	3875	0.043	ng/ul#	100
29) Benzo(g,h,i)perylene	27.833	276	6283	0.078	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041503.D
Acq On : 25 Aug 2023 20:59
Operator : MA/JU
Sample : 04037-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYH1

Quant Time: Aug 26 00:18:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

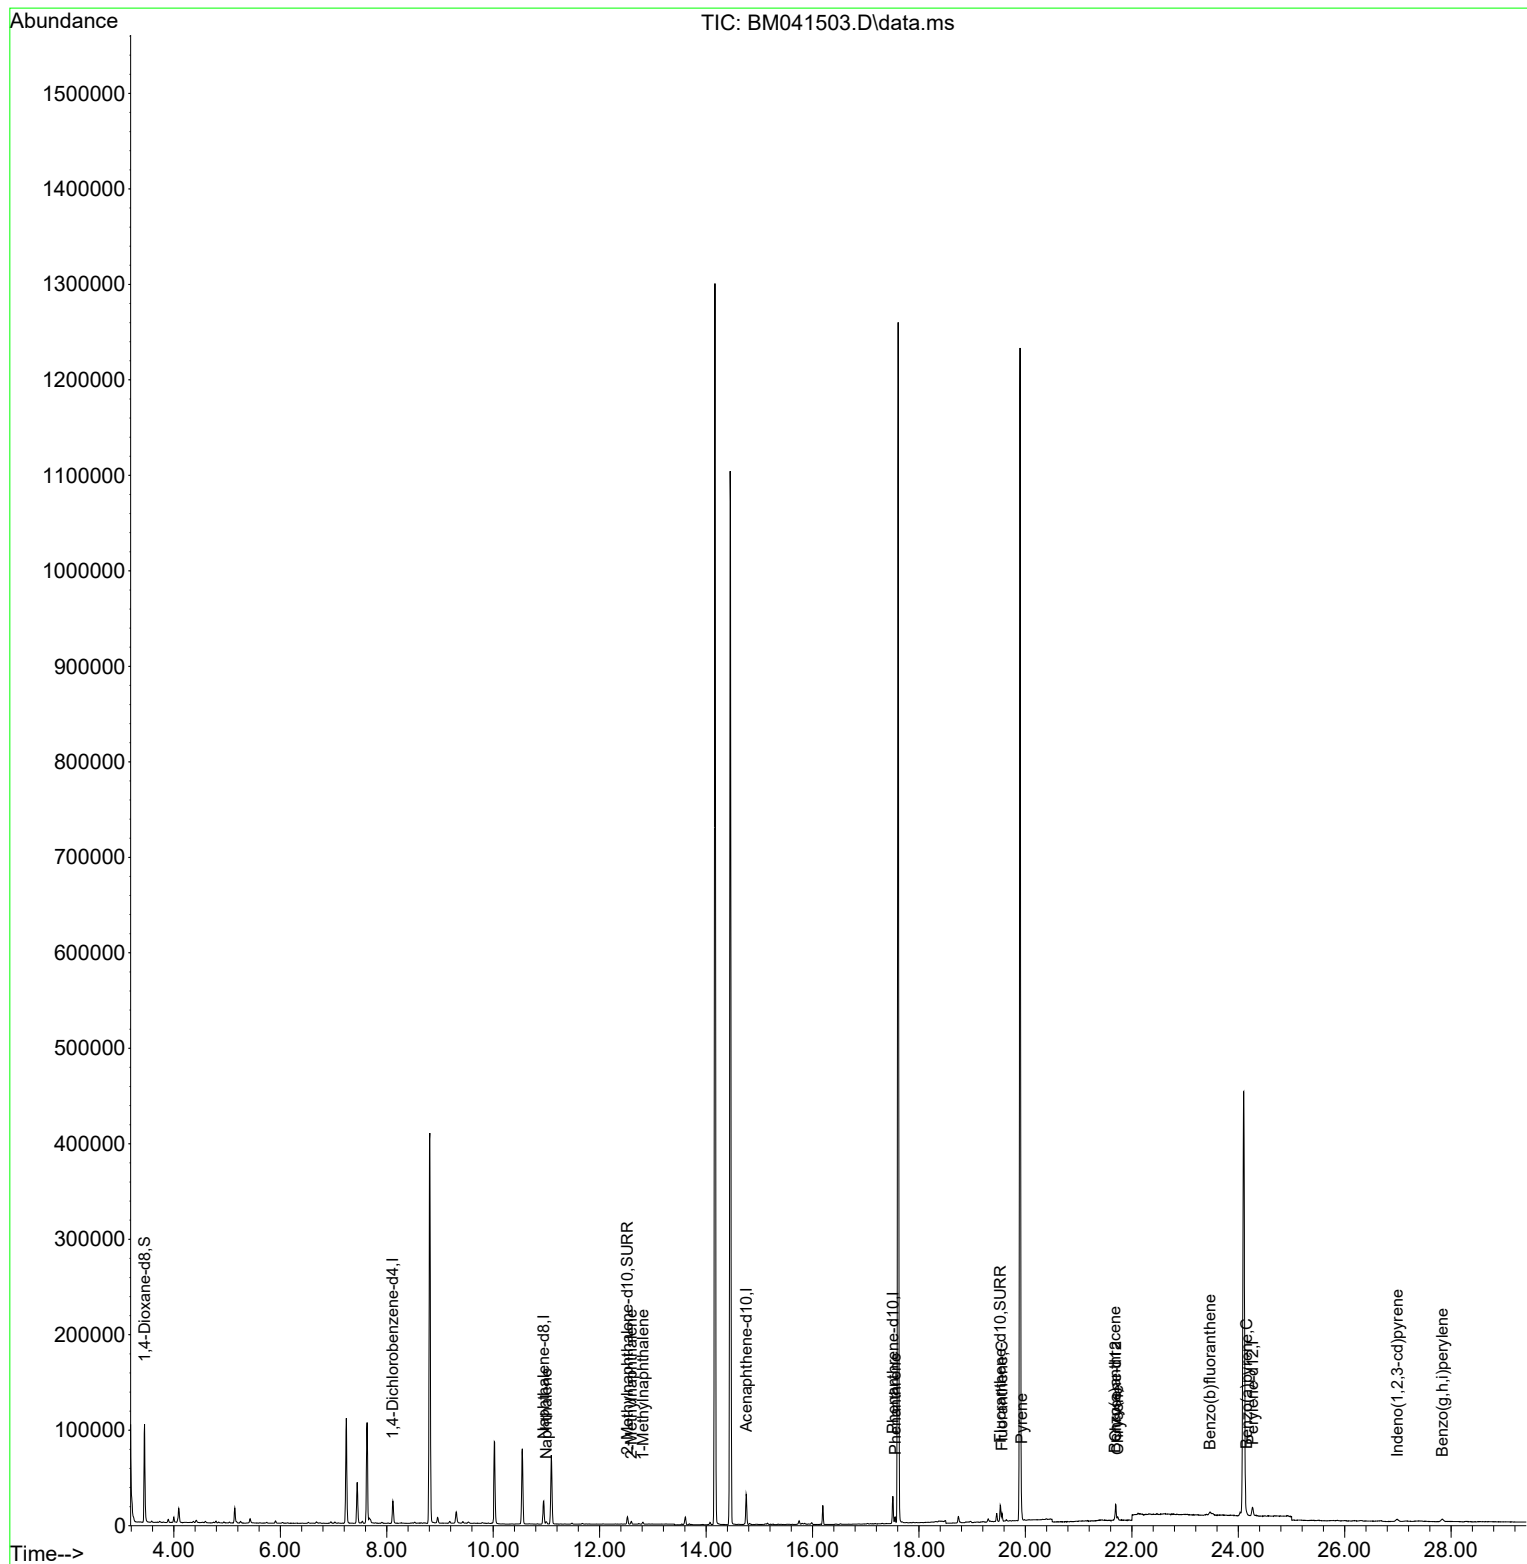



#5

Naphthalene

Concen: 0.036 ng/ul

RT: 10.999 min Scan# 1801

Delta R.T. -0.000 min

Lab File: BM041503.D

Acq: 25 Aug 2023 20:59

Instrument :

BNA_M

ClientSampleId :

EZYH1





Tgt Ion:128 Resp: 3447

Ion Ratio Lower Upper

128 100

129 16.8 8.9 13.3#

127 16.7 10.6 15.8#

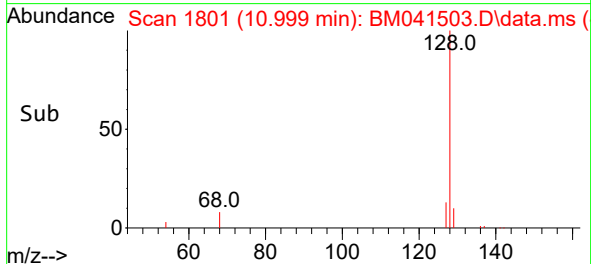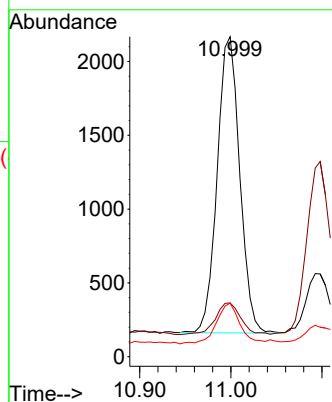

#7

2-Methylnaphthalene

Concen: 0.035 ng/ul

RT: 12.594 min Scan# 2091

Delta R.T. -0.006 min

Lab File: BM041503.D




Acq: 25 Aug 2023 20:59


Tgt Ion:142 Resp: 2037

Ion Ratio Lower Upper

142 100

141 88.9 71.1 106.7

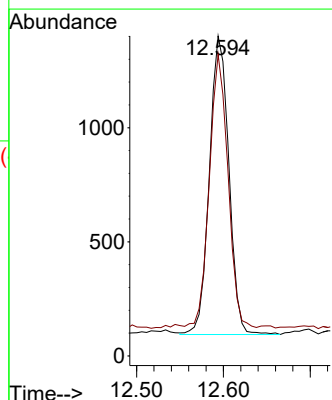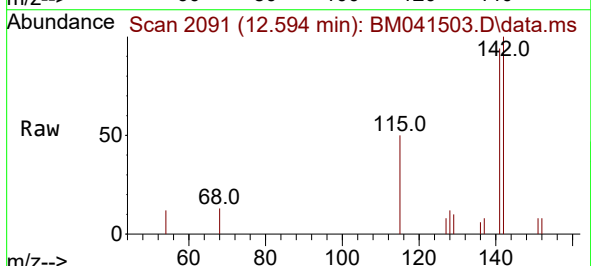



#8

1-Methylnaphthalene

Concen: 0.024 ng/ul

RT: 12.814 min Scan# 2131

Delta R.T. -0.006 min

Lab File: BM041503.D

Acq: 25 Aug 2023 20:59

Instrument :

BNA_M

ClientSampleId :





EZYH1

Tgt Ion:142 Resp: 1430

Ion Ratio Lower Upper

142 100

141 92.8 73.4 110.2

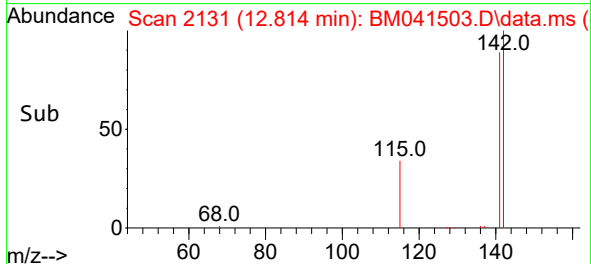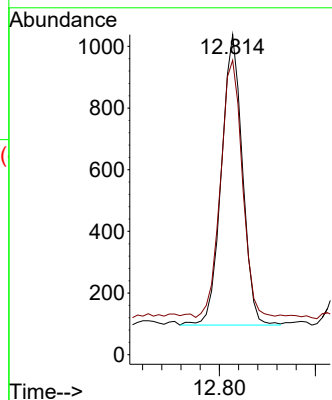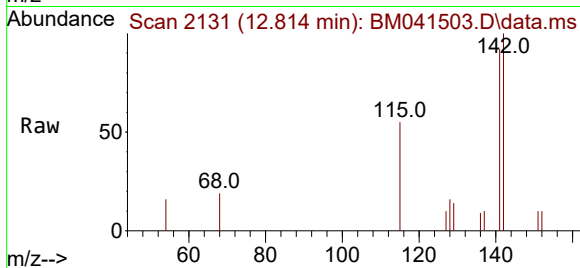

#15

Phenanthrene

Concen: 0.064 ng/ul

RT: 17.552 min Scan# 3167

Delta R.T. -0.004 min

Lab File: BM041503.D

Acq: 25 Aug 2023 20:59




Tgt Ion:178 Resp: 7104


Ion Ratio Lower Upper

178 100

179 20.9 12.5 18.7#

176 23.7 15.8 23.8


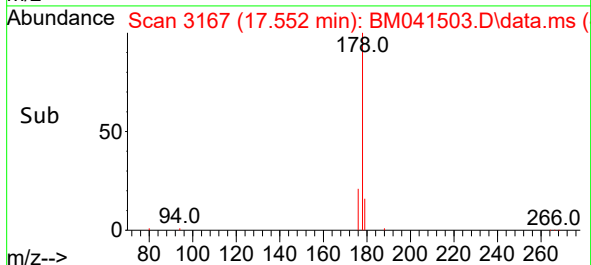
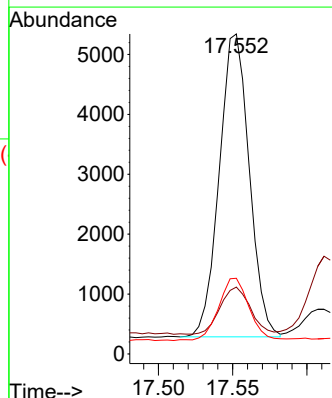
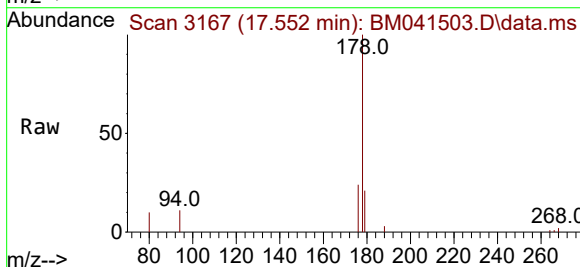


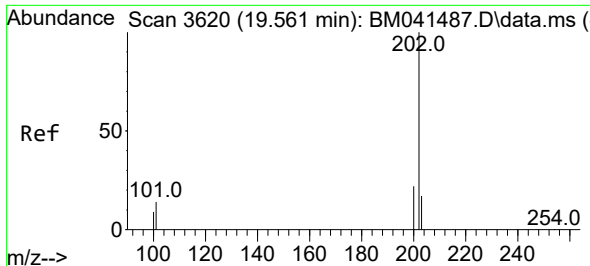

#19
Fluoranthene
Concen: 0.067 ng/ul
RT: 19.561 min Scan# 3620
Delta R.T. -0.005 min
Lab File: BM041503.D
Acq: 25 Aug 2023 20:59




Instrument :
BNA_M
ClientSampleId :
EZYH1


Tgt Ion:202 Resp: 7378
Ion Ratio Lower Upper
202 100
101 17.5 11.0 16.6#
100 13.4 7.9 11.9#

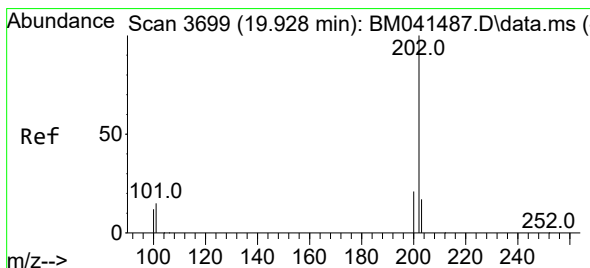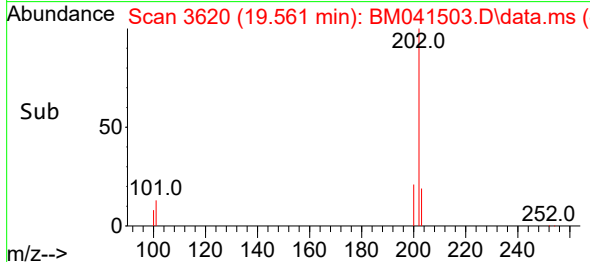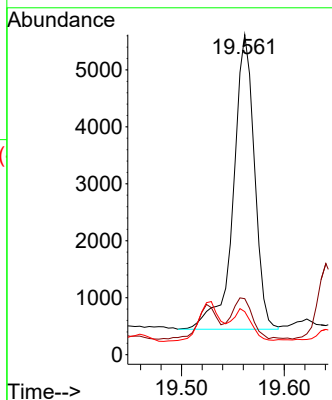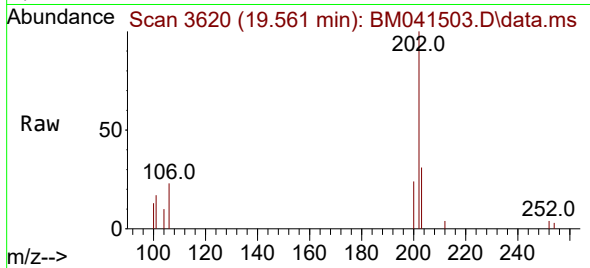

#20
Pyrene
Concen: 0.069 ng/ul
RT: 19.929 min Scan# 3699
Delta R.T. -0.005 min
Lab File: BM041503.D
Acq: 25 Aug 2023 20:59

Tgt Ion:202 Resp: 7691
Ion Ratio Lower Upper
202 100
101 18.5 12.2 18.2#
100 15.1 9.8 14.8#

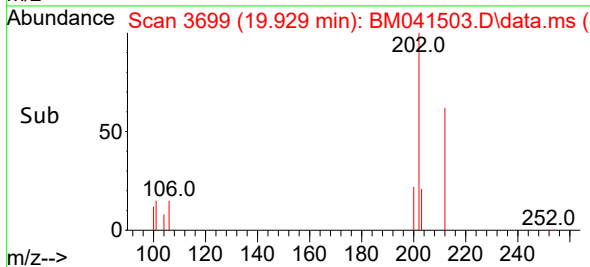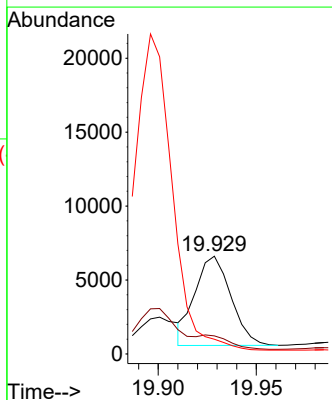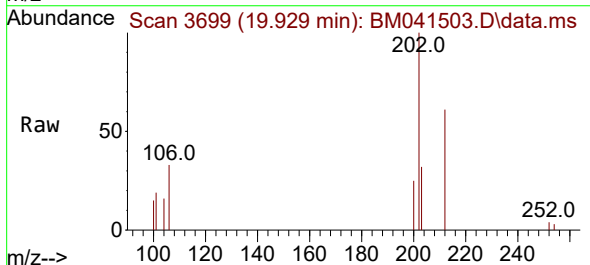



#21

Benzo(a)anthracene

Concen: 0.032 ng/ul

RT: 21.682 min Scan# 4226

Delta R.T. -0.006 min

Lab File: BM041503.D

Acq: 25 Aug 2023 20:59

Instrument :

BNA_M

ClientSampleId :

EZYH1





Tgt Ion:228 Resp: 2506

Ion Ratio Lower Upper

228 100

229 55.4 15.3 22.9#

226 52.9 22.7 34.1#

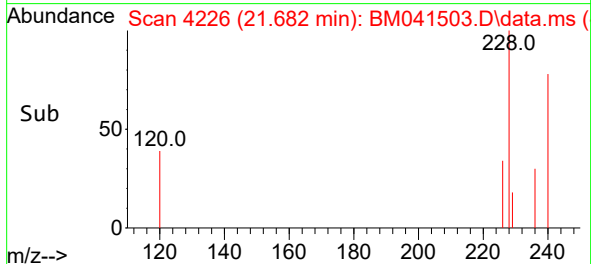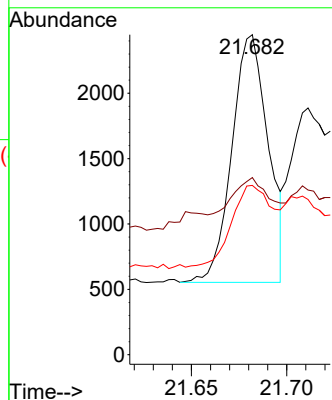

#22

Chrysene

Concen: 0.036 ng/ul

RT: 21.734 min Scan# 4244

Delta R.T. -0.009 min

Lab File: BM041503.D

Acq: 25 Aug 2023 20:59




Tgt Ion:228 Resp: 3047


Ion Ratio Lower Upper

228 100

226 50.2 25.6 38.4#

229 51.0 15.7 23.5#


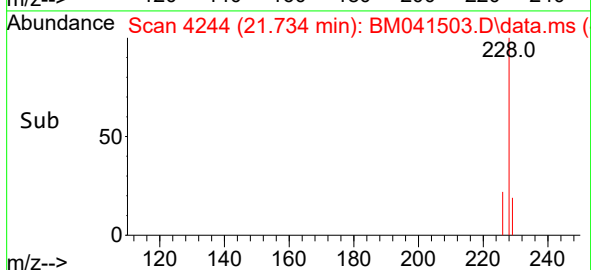
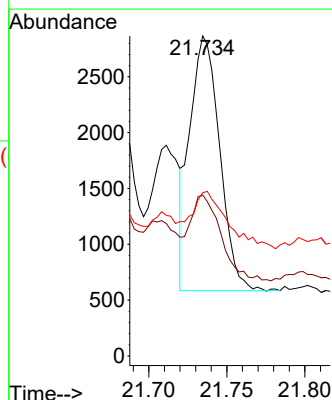
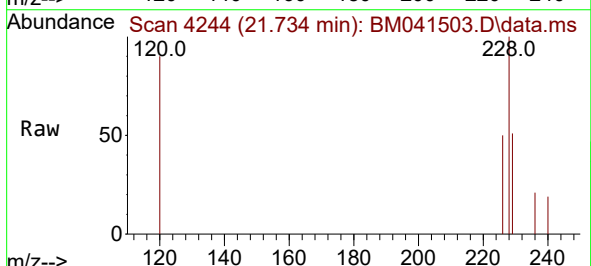


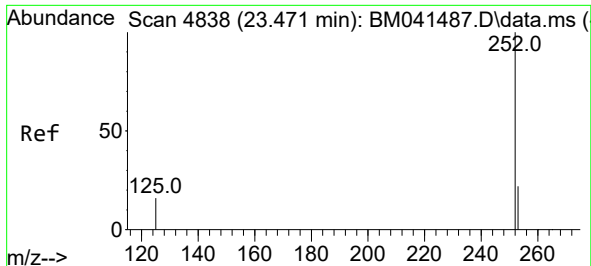

#24
Benzo(b)fluoranthene
Concen: 0.061 ng/ul
RT: 23.468 min Scan# 4837
Delta R.T. -0.015 min
Lab File: BM041503.D
Acq: 25 Aug 2023 20:59




Instrument :
BNA_M
ClientSampleId :
EZYH1


Tgt Ion:252 Resp: 5374
Ion Ratio Lower Upper
252 100
253 56.8 0.0 46.8#
125 207.5 0.0 32.8#

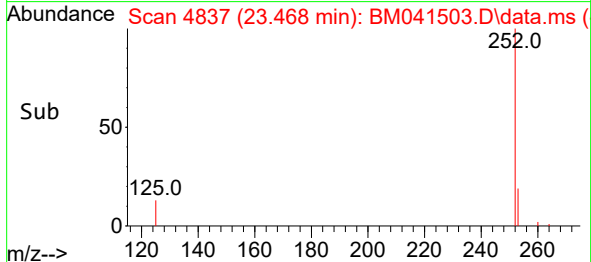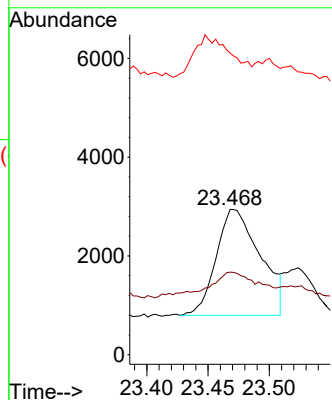

#26
Benzo(a)pyrene
Concen: 0.035 ng/ul
RT: 24.155 min Scan# 5072
Delta R.T. -0.009 min
Lab File: BM041503.D
Acq: 25 Aug 2023 20:59


Tgt Ion:252 Resp: 2546
Ion Ratio Lower Upper
252 100
253 67.0 19.5 29.3#
125 262.1 16.0 24.0#

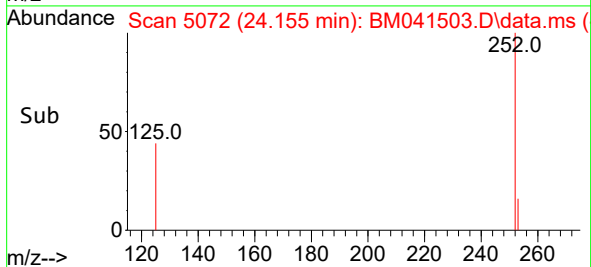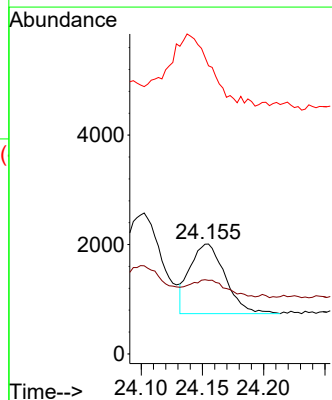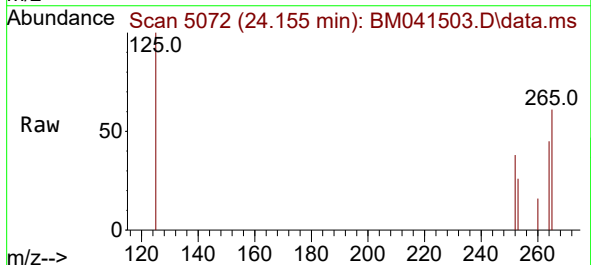



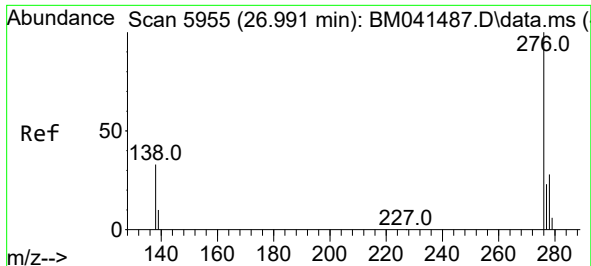


#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.043 ng/ul
 RT: 26.988 min Scan# 5954
 Delta R.T. -0.017 min
 Lab File: BM041503.D
 Acq: 25 Aug 2023 20:59


Instrument :
 BNA_M
 ClientSampleId :
 EZYH1



Tgt Ion:276 Resp: 3875
 Ion Ratio Lower Upper
 276 100
 138 34.9 27.8 41.6
 227 1.1 0.0 0.0#

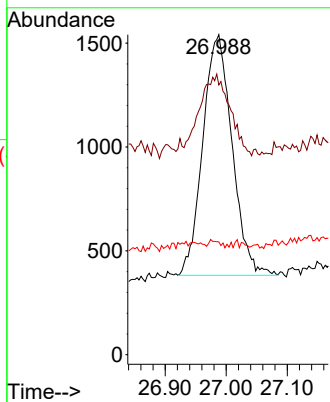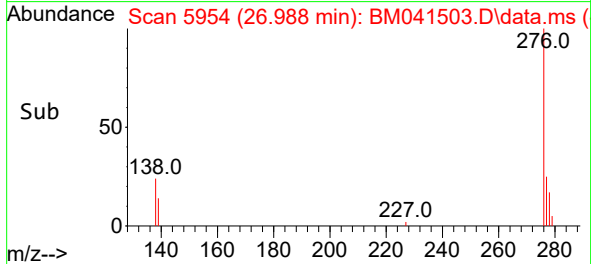

#29
 Benzo(g,h,i)perylene
 Concen: 0.078 ng/ul
 RT: 27.833 min Scan# 6206
 Delta R.T. -0.020 min
 Lab File: BM041503.D
 Acq: 25 Aug 2023 20:59

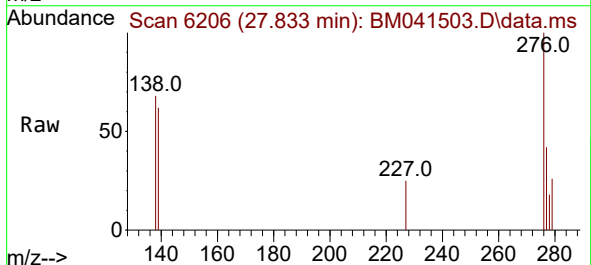

Tgt Ion:276 Resp: 6283
 Ion Ratio Lower Upper
 276 100
 138 68.1 25.9 38.9#
 277 42.0 19.4 29.2#

