

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041467.D
 Acq On : 24 Aug 2023 16:08
 Operator : MA/JU
 Sample : 04105-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHAR9

Quant Time: Aug 24 18:36:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.118	152	10537	0.400	ng/ul	0.00
4) Naphthalene-d8	10.950	136	30709	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.759	164	14974	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	26435	0.400	ng/ul	0.00
17) Chrysene-d12	21.705	240	7742	0.400	ng/ul	0.00
23) Perylene-d12	24.281	264	8834	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	68704	5.152	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.528	152	11357	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.534	212	13214	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	24946	1.818	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041467.D
Acq On : 24 Aug 2023 16:08
Operator : MA/JU
Sample : 04105-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHAR9


Quant Time: Aug 24 18:36:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

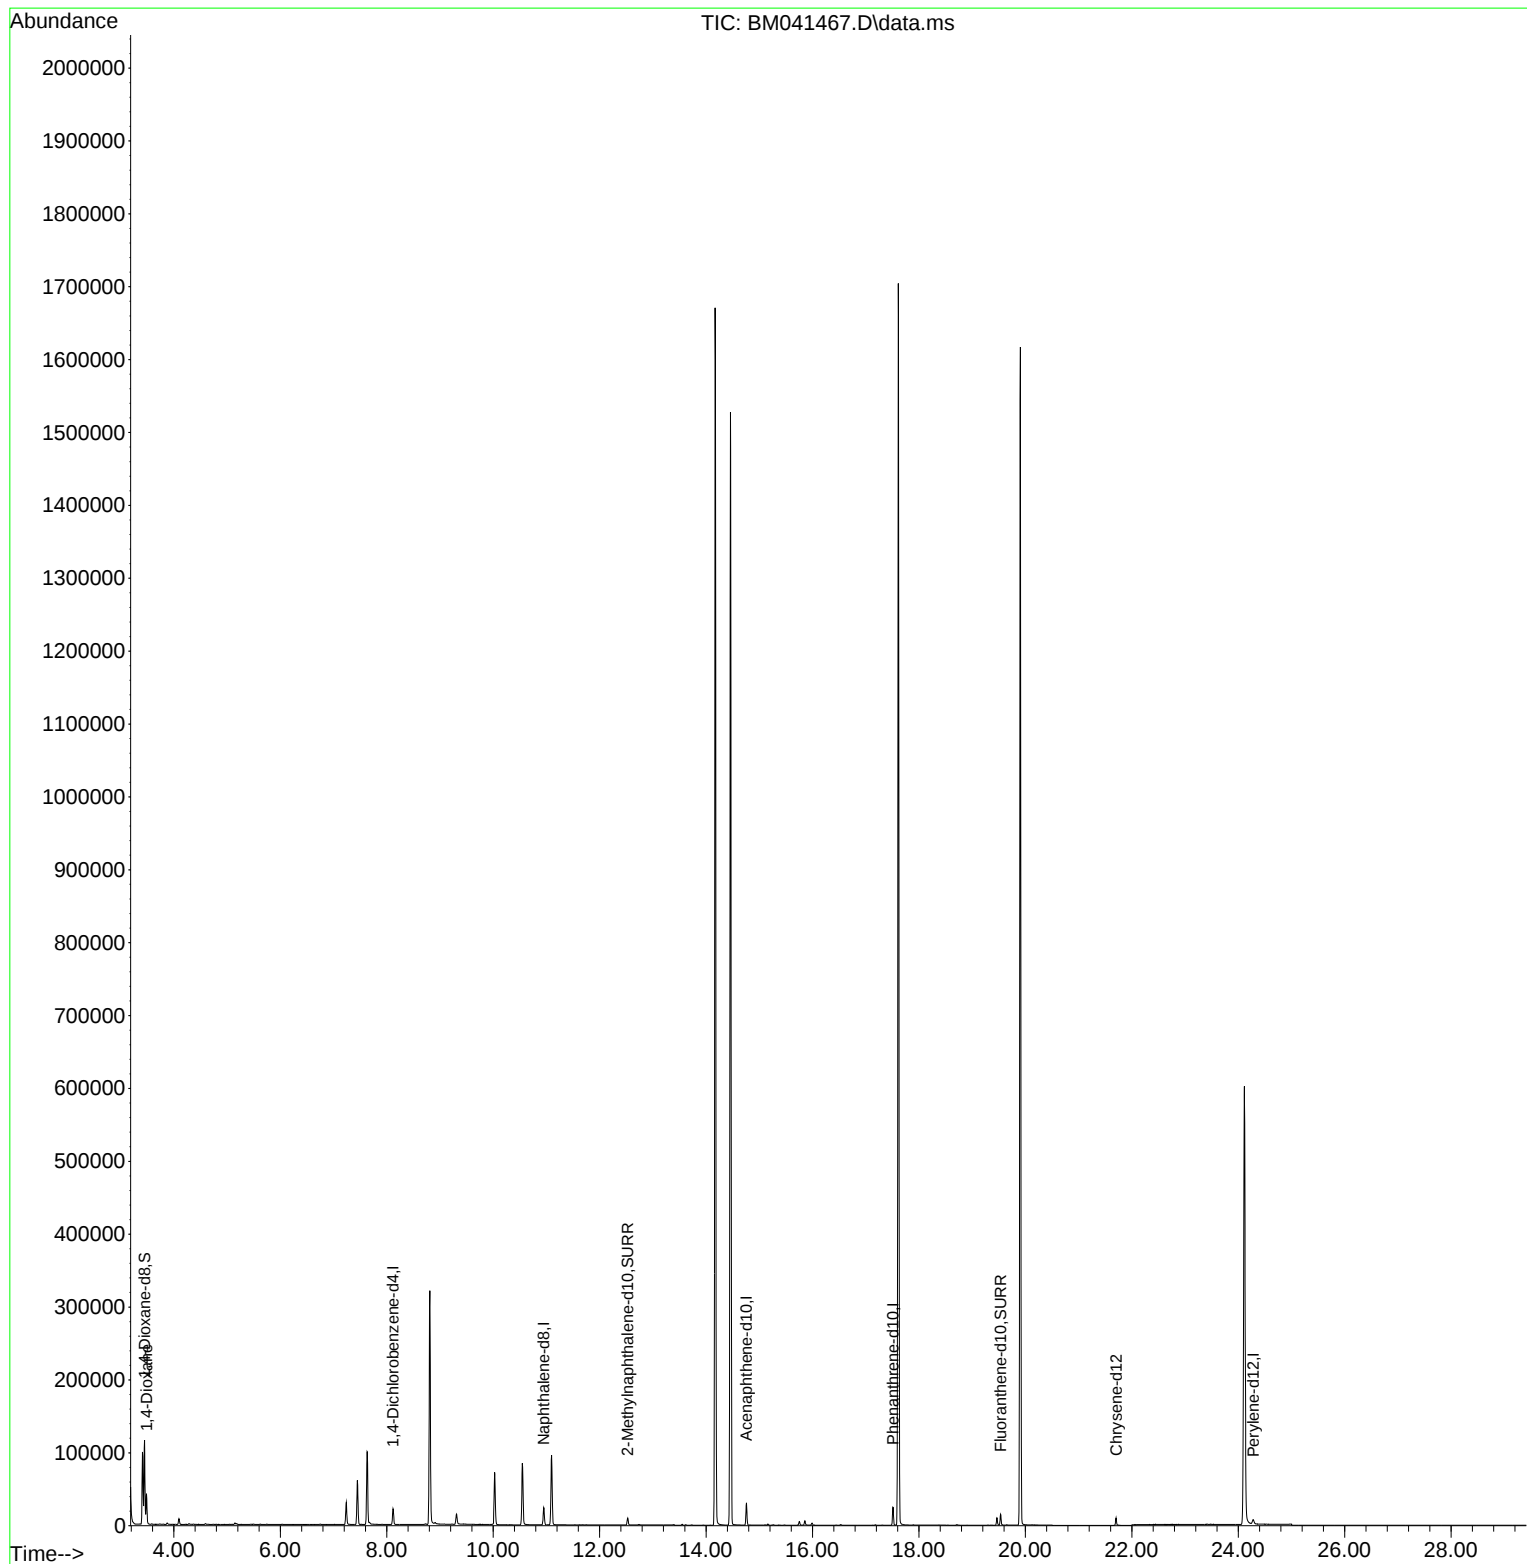

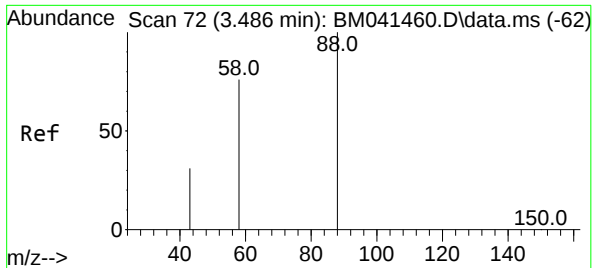

#2
 1,4-Dioxane
 Concen: 1.818 ng/ul
 RT: 3.486 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM041467.D
 Acq: 24 Aug 2023 16:08

Instrument :
 BNA_M
 ClientSampleId :
 BHAR9

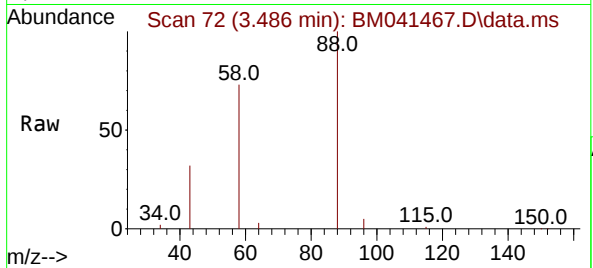

Tgt Ion: 88 Resp: 24946
 Ion Ratio Lower Upper
 88 100
 43 32.0 35.4 53.2#
 58 72.9 57.3 85.9

