

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041468.D
 Acq On : 24 Aug 2023 16:45
 Operator : MA/JU
 Sample : 04105-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH8X9

Quant Time: Aug 24 18:36:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.118	152	10477	0.400	ng/ul	0.00
4) Naphthalene-d8	10.949	136	30689	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.759	164	14102	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.514	188	24825	0.400	ng/ul	0.00
17) Chrysene-d12	21.705	240	8339	0.400	ng/ul	# 0.00
23) Perylene-d12	24.278	264	9740	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	58948	4.446	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.528	152	10894	0.269	ng/ul	0.00
18) Fluoranthene-d10	19.533	212	13059	0.355	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	1157	0.085	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041468.D
Acq On : 24 Aug 2023 16:45
Operator : MA/JU
Sample : 04105-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH8X9


Quant Time: Aug 24 18:36:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

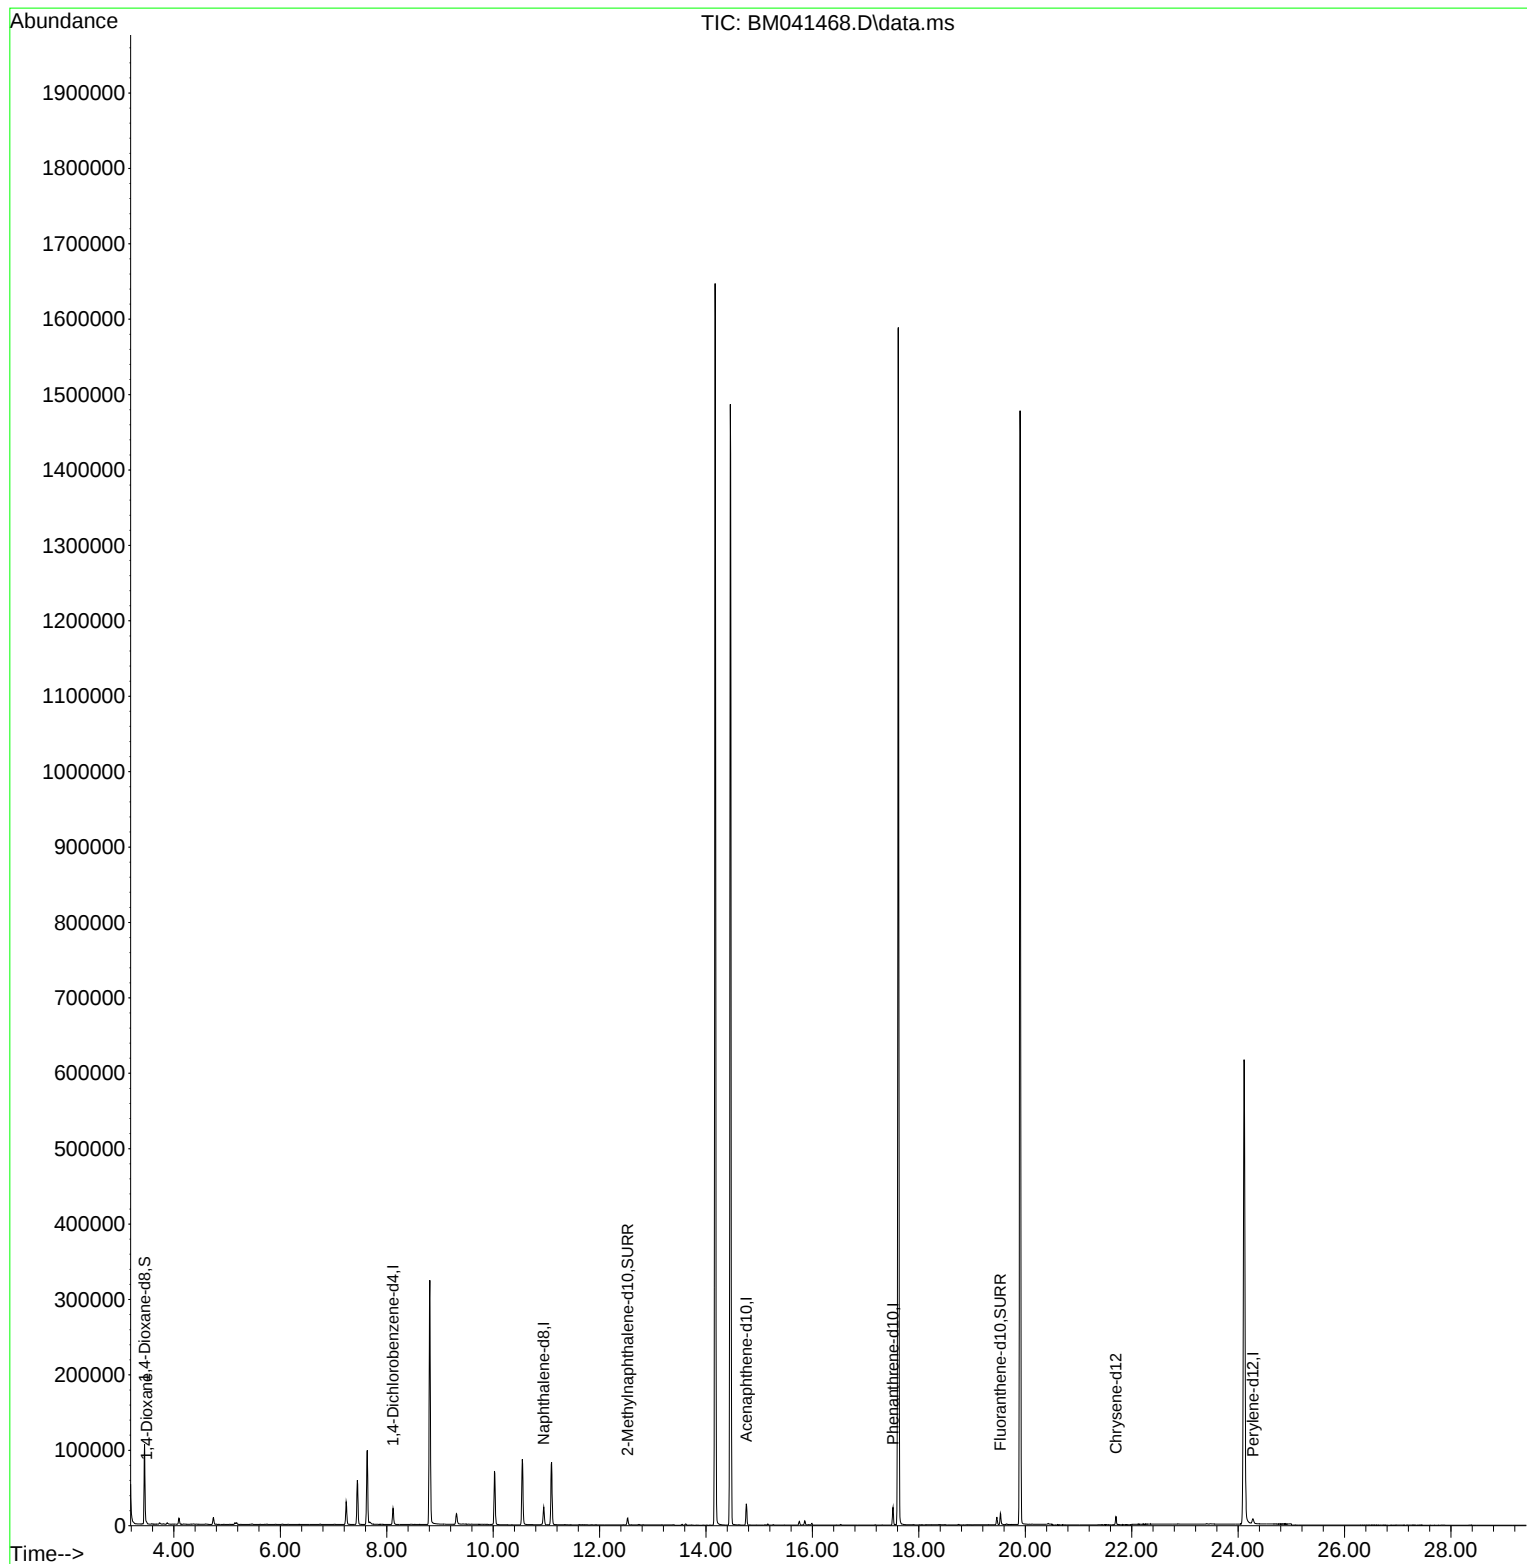

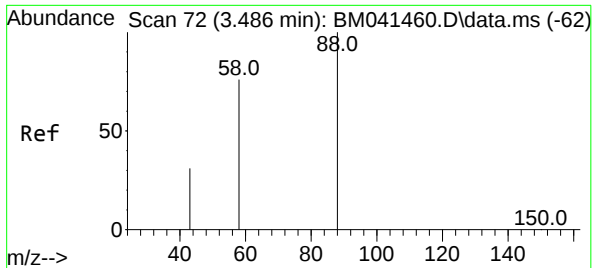

#2
 1,4-Dioxane
 Concen: 0.085 ng/ul
 RT: 3.486 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BM041468.D
 Acq: 24 Aug 2023 16:45

Instrument :
 BNA_M
 ClientSampleId :
 BH8X9

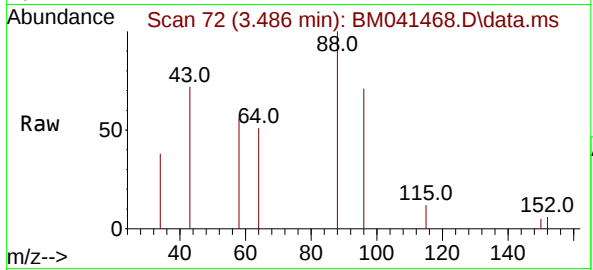

Tgt Ion:	88	Resp:	1157
Ion Ratio	Lower	Upper	
88	100		
43	72.3	35.4	53.2#
58	56.0	57.3	85.9#

