

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041470.D
 Acq On : 24 Aug 2023 17:59
 Operator : MA/JU
 Sample : 04105-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHAB1

Quant Time: Aug 24 18:43:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.118	152	10584	0.400	ng/ul	0.00
4) Naphthalene-d8	10.949	136	31813	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.758	164	15798	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	29454	0.400	ng/ul	0.00
17) Chrysene-d12	21.702	240	8935	0.400	ng/ul	0.00
23) Perylene-d12	24.278	264	9256	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	61155	4.565	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.528	152	11938	0.284	ng/ul	0.00
18) Fluoranthene-d10	19.533	212	15257	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	9177	0.666	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041470.D
Acq On : 24 Aug 2023 17:59
Operator : MA/JU
Sample : 04105-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHAB1

Quant Time: Aug 24 18:43:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

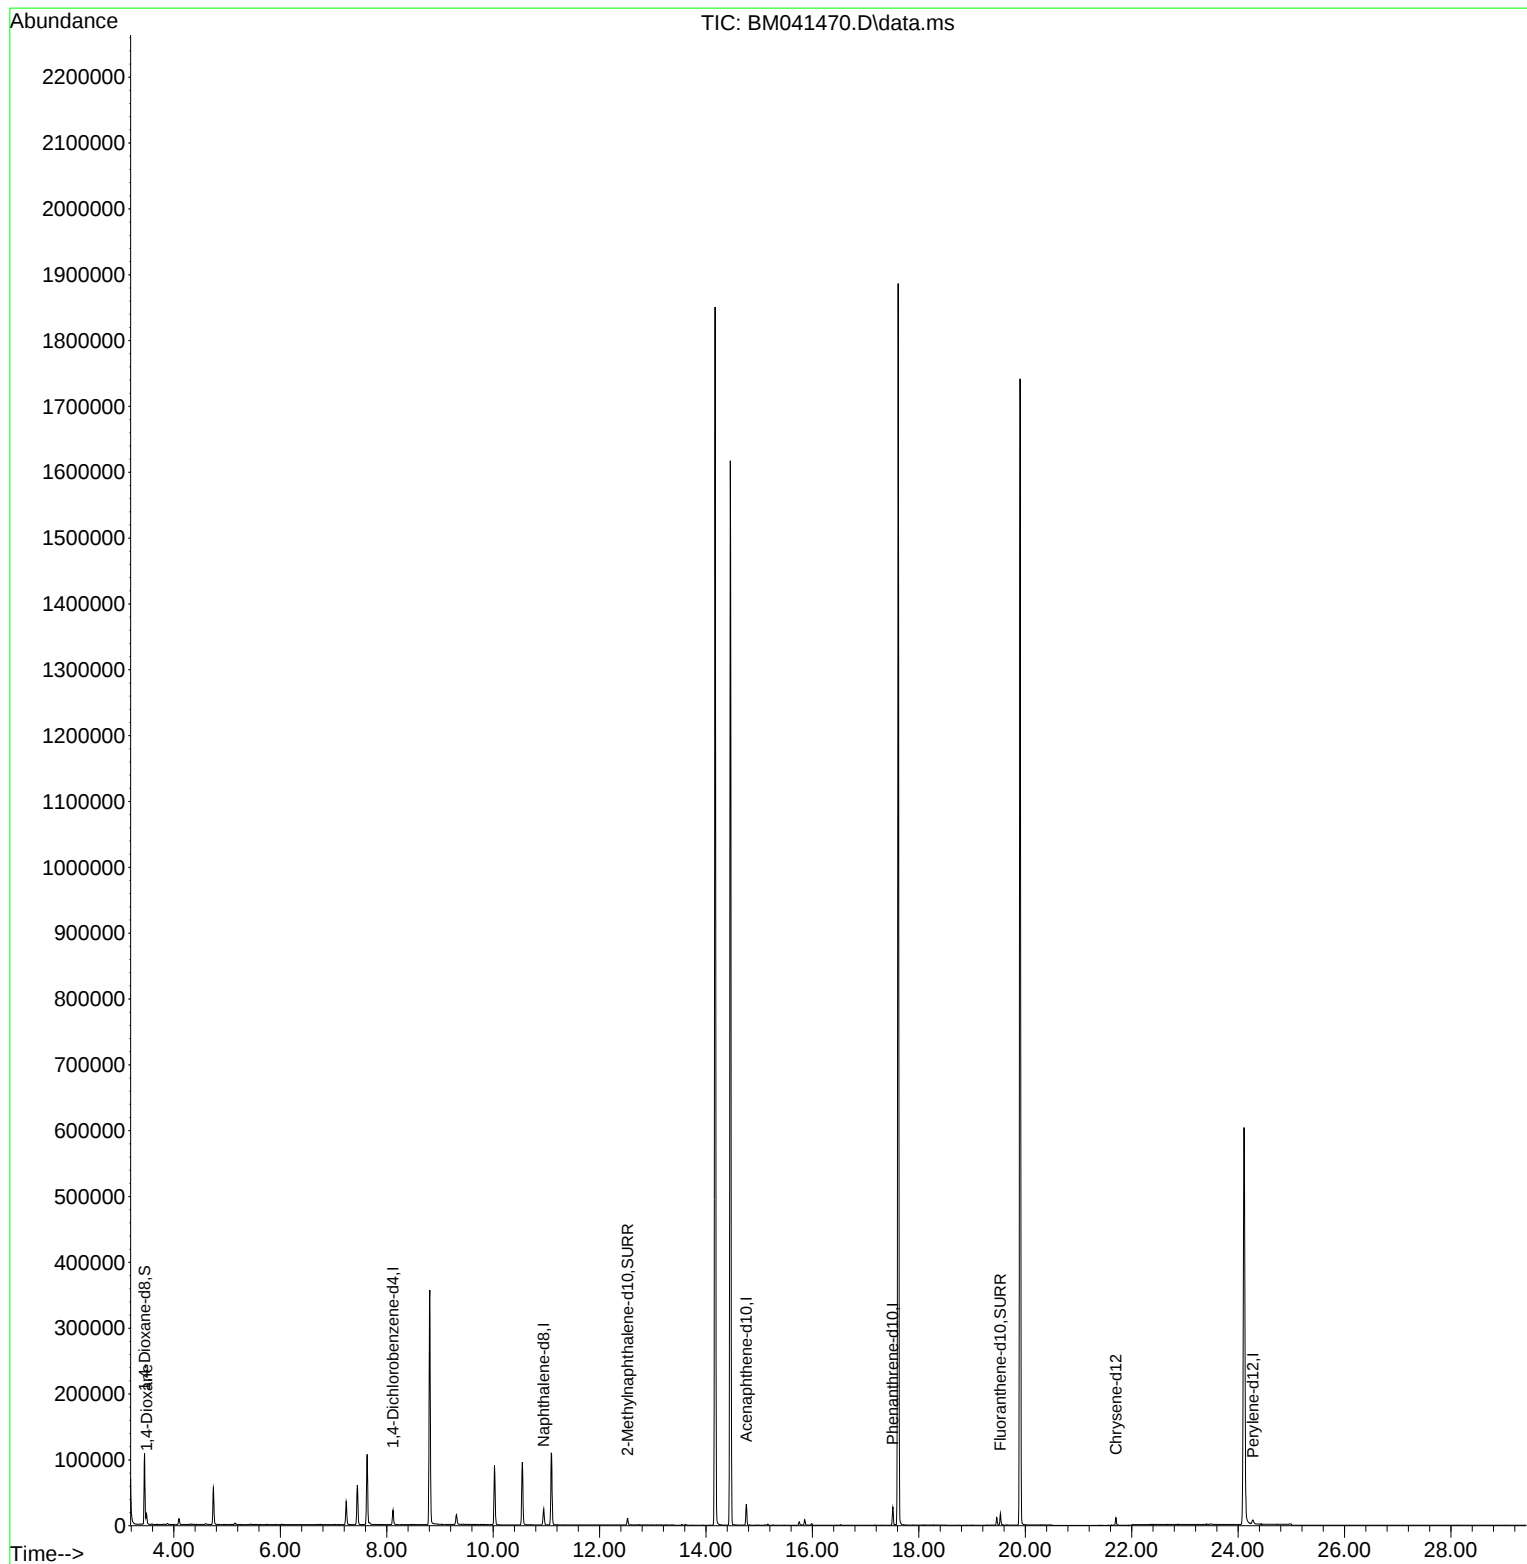

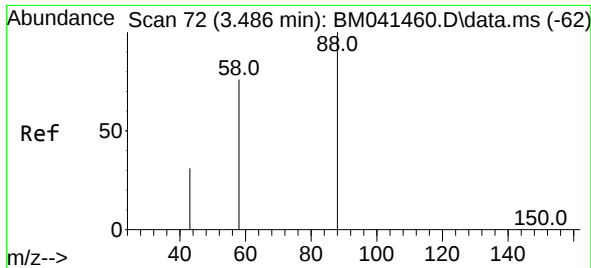

#2
 1,4-Dioxane
 Concen: 0.666 ng/ul
 RT: 3.486 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BM041470.D
 Acq: 24 Aug 2023 17:59

Instrument :
 BNA_M
 ClientSampleId :
 BHAB1

Tgt Ion: 88 Resp: 9177
 Ion Ratio Lower Upper
 88 100
 43 36.2 35.4 53.2
 58 71.9 57.3 85.9

