

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041477.D
 Acq On : 24 Aug 2023 22:53
 Operator : MA/JU
 Sample : 04105-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH8X3

Quant Time: Aug 25 02:33:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.119	152	11709	0.400	ng/ul	0.00
4) Naphthalene-d8	10.950	136	35285	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	17550	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	32267	0.400	ng/ul	0.00
17) Chrysene-d12	21.700	240	9533	0.400	ng/ul	0.00
23) Perylene-d12	24.269	264	9927	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	71712	4.839	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.523	152	14803	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.534	212	18474	0.439	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	1825	0.120	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041477.D
Acq On : 24 Aug 2023 22:53
Operator : MA/JU
Sample : 04105-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH8X3


Quant Time: Aug 25 02:33:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

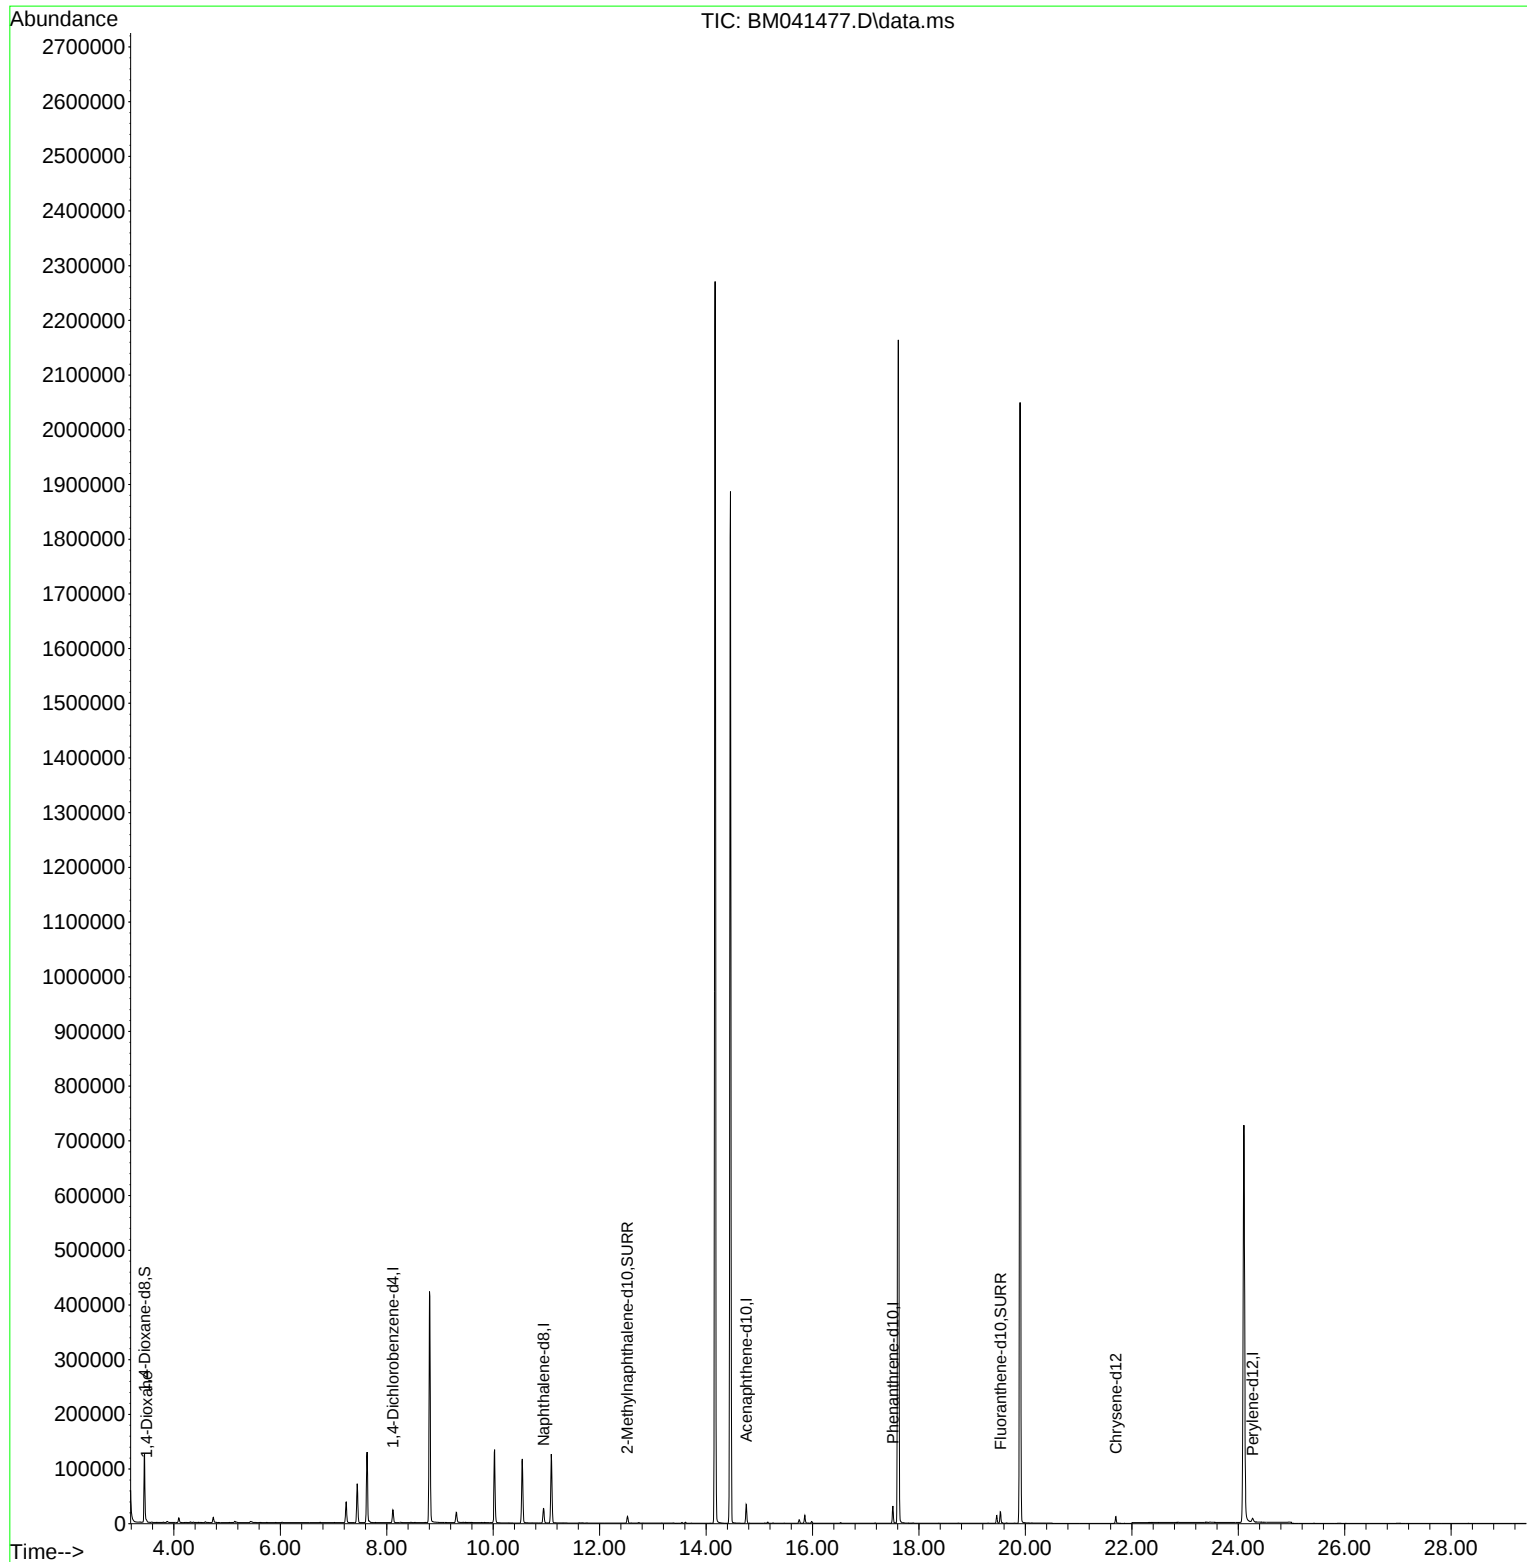


Abundance Scan 72 (3.486 min): BM041472.D\data.ms (-64)

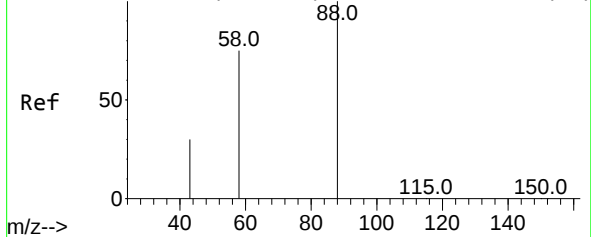

Abundance Scan 72 (3.486 min): BM041477.D\data.ms

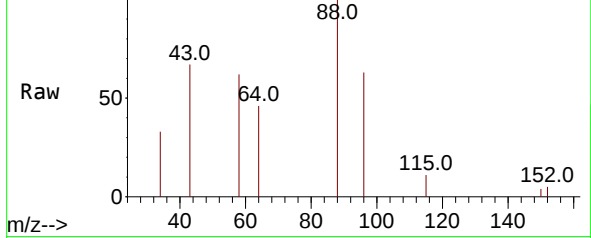

Abundance Scan 72 (3.486 min): BM041477.D\data.ms (-58)

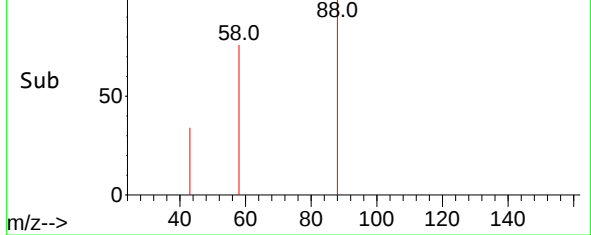

#2

1,4-Dioxane

Concen: 0.120 ng/ul

RT: 3.486 min Scan# 71

Delta R.T. 0.000 min

Lab File: BM041477.D

Acq: 24 Aug 2023 22:53

Instrument :

BNA_M

ClientSampleId :

BH8X3

Tgt Ion: 88 Resp: 1825

Ion Ratio Lower Upper

88 100

43 67.0 35.4 53.2#

58 62.0 57.3 85.9

