

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041479.D
 Acq On : 25 Aug 2023 00:07
 Operator : MA/JU
 Sample : 04105-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH929

Quant Time: Aug 25 02:33:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	13120	0.400	ng/ul	0.00
4) Naphthalene-d8	10.950	136	36940	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	16898	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	29732	0.400	ng/ul	0.00
17) Chrysene-d12	21.699	240	9730	0.400	ng/ul	0.00
23) Perylene-d12	24.269	264	11339	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	63292	3.812	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	9598	0.197	ng/ul	0.00
18) Fluoranthene-d10	19.529	212	11805	0.275	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	1167	0.068	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041479.D
Acq On : 25 Aug 2023 00:07
Operator : MA/JU
Sample : 04105-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH929

Quant Time: Aug 25 02:33:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

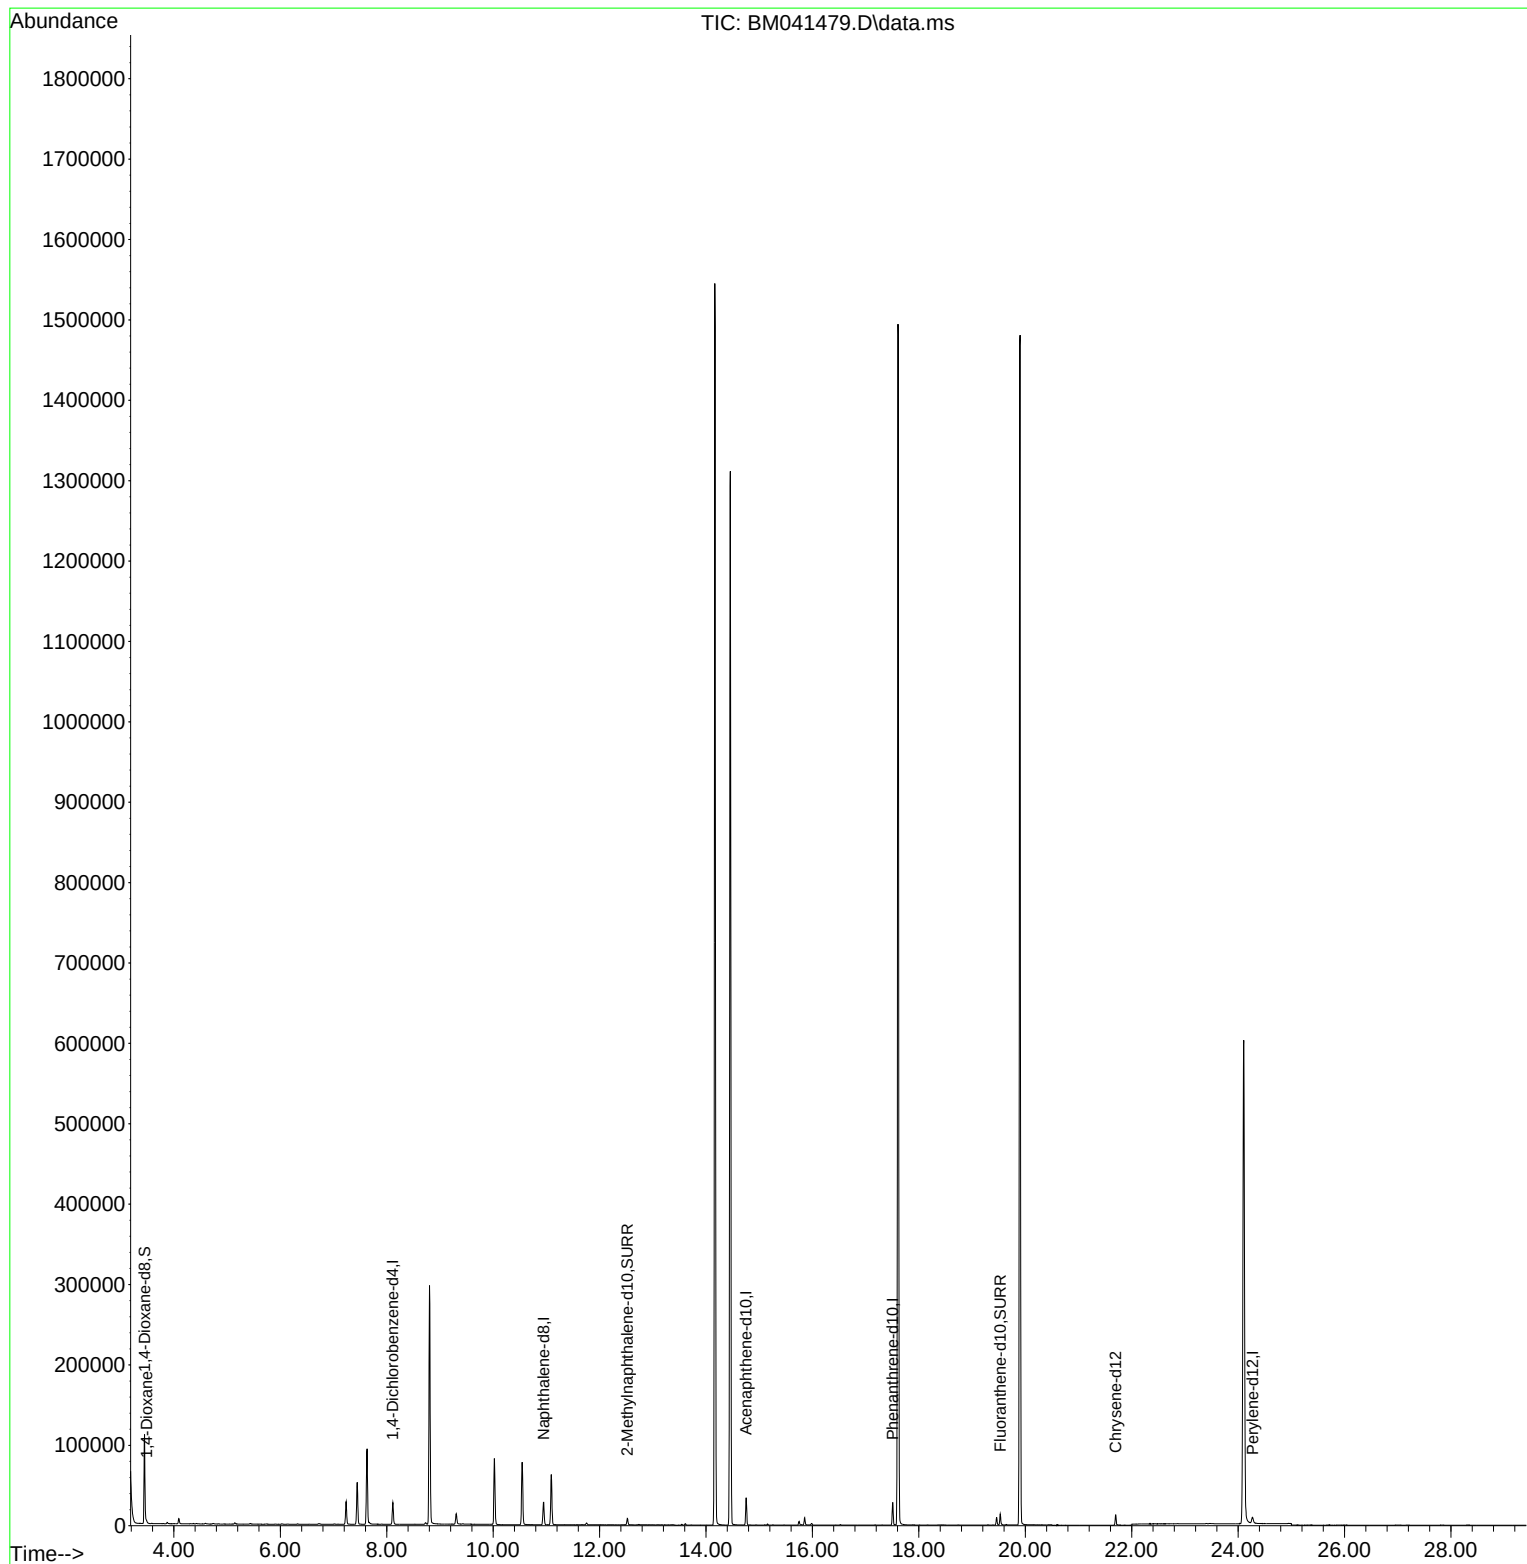

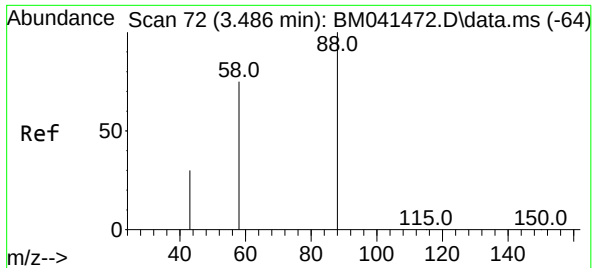

#2
 1,4-Dioxane
 Concen: 0.068 ng/ul
 RT: 3.486 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM041479.D
 Acq: 25 Aug 2023 00:07

Instrument :
 BNA_M
 ClientSampleId :
 BH929

Tgt Ion:	88	Resp:	1167
Ion	Ratio	Lower	Upper
88	100		
43	45.7	35.4	53.2
58	41.4	57.3	85.9

