

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041480.D
 Acq On : 25 Aug 2023 00:43
 Operator : MA/JU
 Sample : 04105-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH962

Quant Time: Aug 25 02:33:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	11857	0.400	ng/u1	0.00
4) Naphthalene-d8	10.950	136	36291	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.754	164	18181	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.510	188	35527	0.400	ng/u1	0.00
17) Chrysene-d12	21.697	240	12209	0.400	ng/u1	# 0.00
23) Perylene-d12	24.269	264	12998	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	75591	5.037	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.522	152	14862	0.310	ng/u1	0.00
18) Fluoranthene-d10	19.529	212	20940	0.389	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	3280	0.212	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041480.D
Acq On : 25 Aug 2023 00:43
Operator : MA/JU
Sample : 04105-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH962


Quant Time: Aug 25 02:33:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

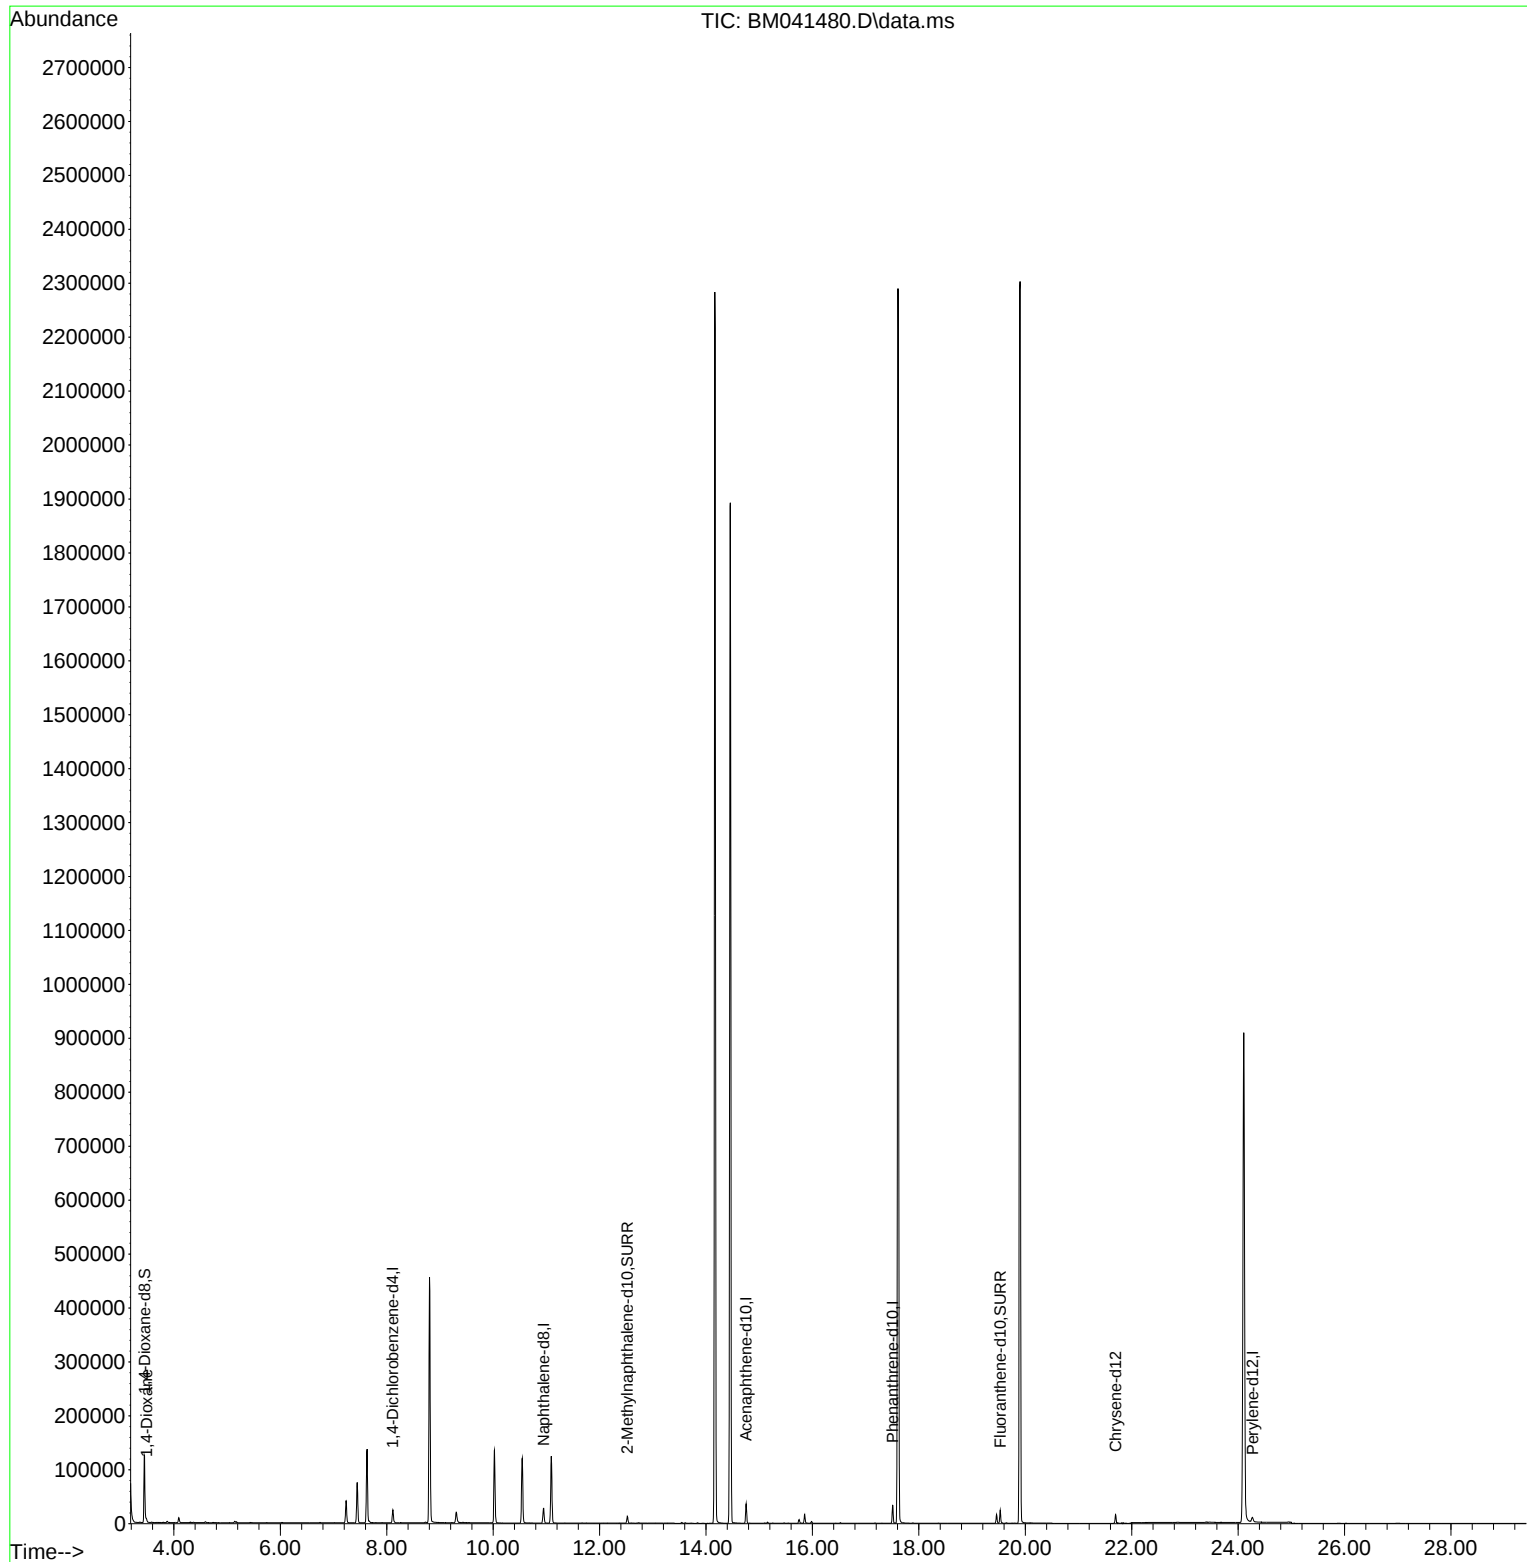

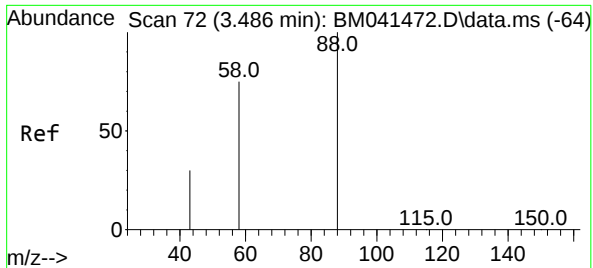

#2
 1,4-Dioxane
 Concen: 0.212 ng/ul
 RT: 3.486 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BM041480.D
 Acq: 25 Aug 2023 00:43

Instrument :
 BNA_M
 ClientSampleId :
 BH962

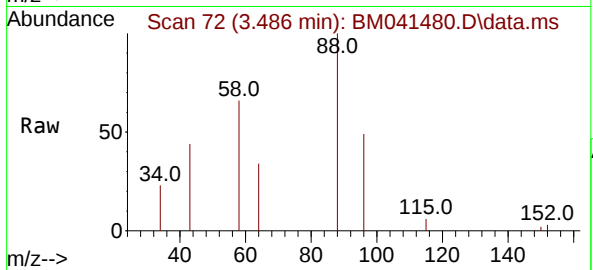

Tgt Ion:	88	Resp:	3280
Ion	Ratio	Lower	Upper
88	100		
43	44.1	35.4	53.2
58	66.3	57.3	85.9

