

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041481.D
 Acq On : 25 Aug 2023 01:20
 Operator : MA/JU
 Sample : 04105-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH927

Quant Time: Aug 25 02:33:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	12361	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	36698	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	18961	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.510	188	33234	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.697	240	10636	0.400	ng/ul	# 0.00
23) Perylene-d12	24.269	264	11561	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	85735	5.480	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	17896	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.529	212	21683	0.462	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.486	88	720	0.045	ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041481.D
Acq On : 25 Aug 2023 01:20
Operator : MA/JU
Sample : 04105-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH927

Quant Time: Aug 25 02:33:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

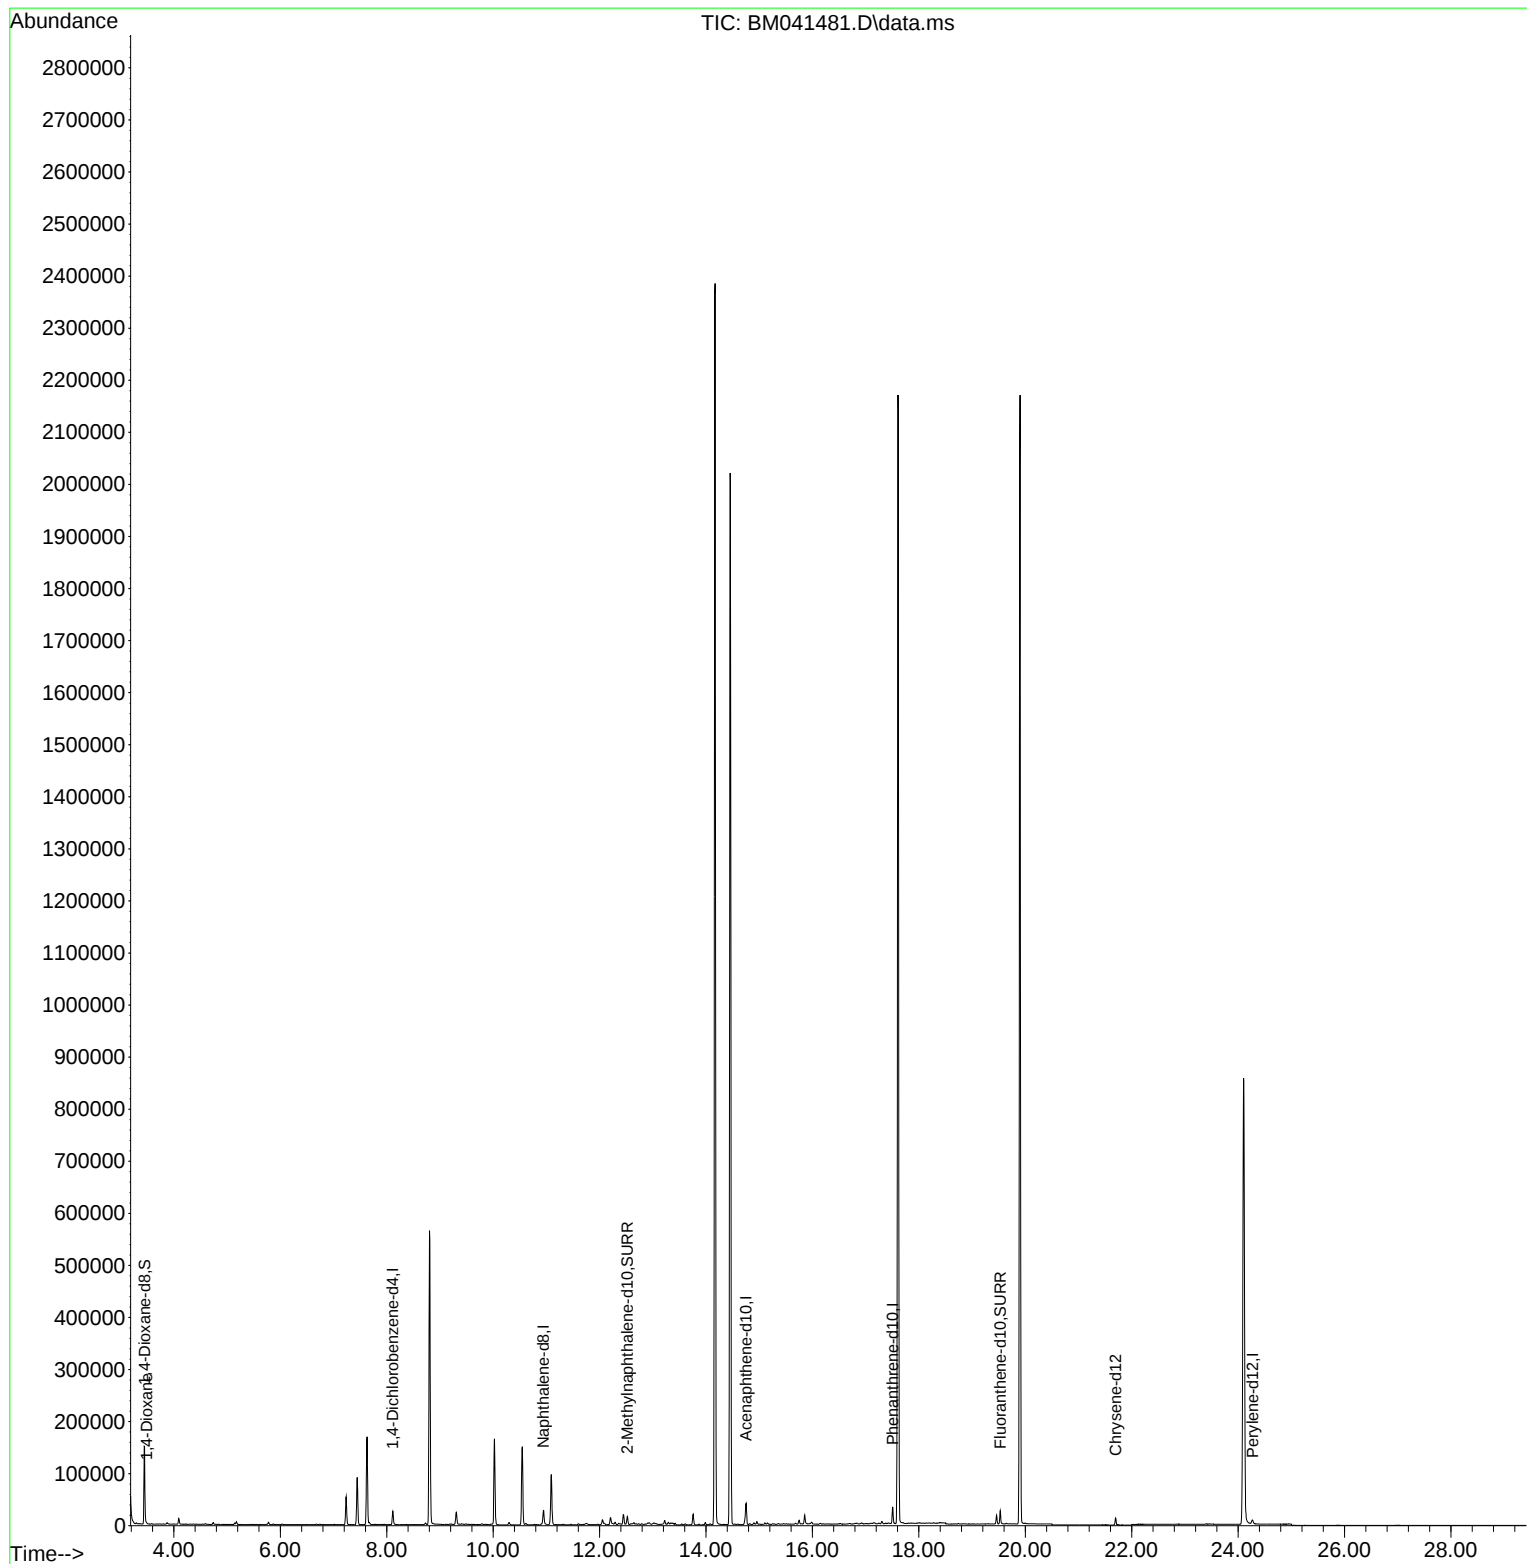

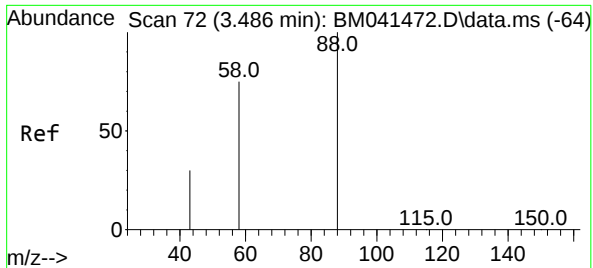

#2
 1,4-Dioxane
 Concen: 0.045 ng/ul
 RT: 3.486 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BM041481.D
 Acq: 25 Aug 2023 01:20

Instrument :
 BNA_M
 ClientSampleId :
 BH927

Tgt Ion: 88 Resp: 720
 Ion Ratio Lower Upper
 88 100
 43 161.5 35.4 53.2#
 58 73.8 57.3 85.9

