

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041489.D
 Acq On : 25 Aug 2023 09:35
 Operator : MA/JU
 Sample : 04105-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH962

Quant Time: Aug 26 00:16:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	13966	0.400	ng/u1	0.00
4) Naphthalene-d8	10.944	136	40337	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.754	164	19078	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.510	188	35227	0.400	ng/u1	0.00
17) Chrysene-d12	21.702	240	10847	0.400	ng/u1	# 0.00
23) Perylene-d12	24.275	264	12359	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	87242	4.936	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.522	152	16187	0.304	ng/u1	0.00
18) Fluoranthene-d10	19.534	212	19622	0.410	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.482	88	3888	0.214	ng/u1	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041489.D
Acq On : 25 Aug 2023 09:35
Operator : MA/JU
Sample : 04105-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH962

Quant Time: Aug 26 00:16:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration

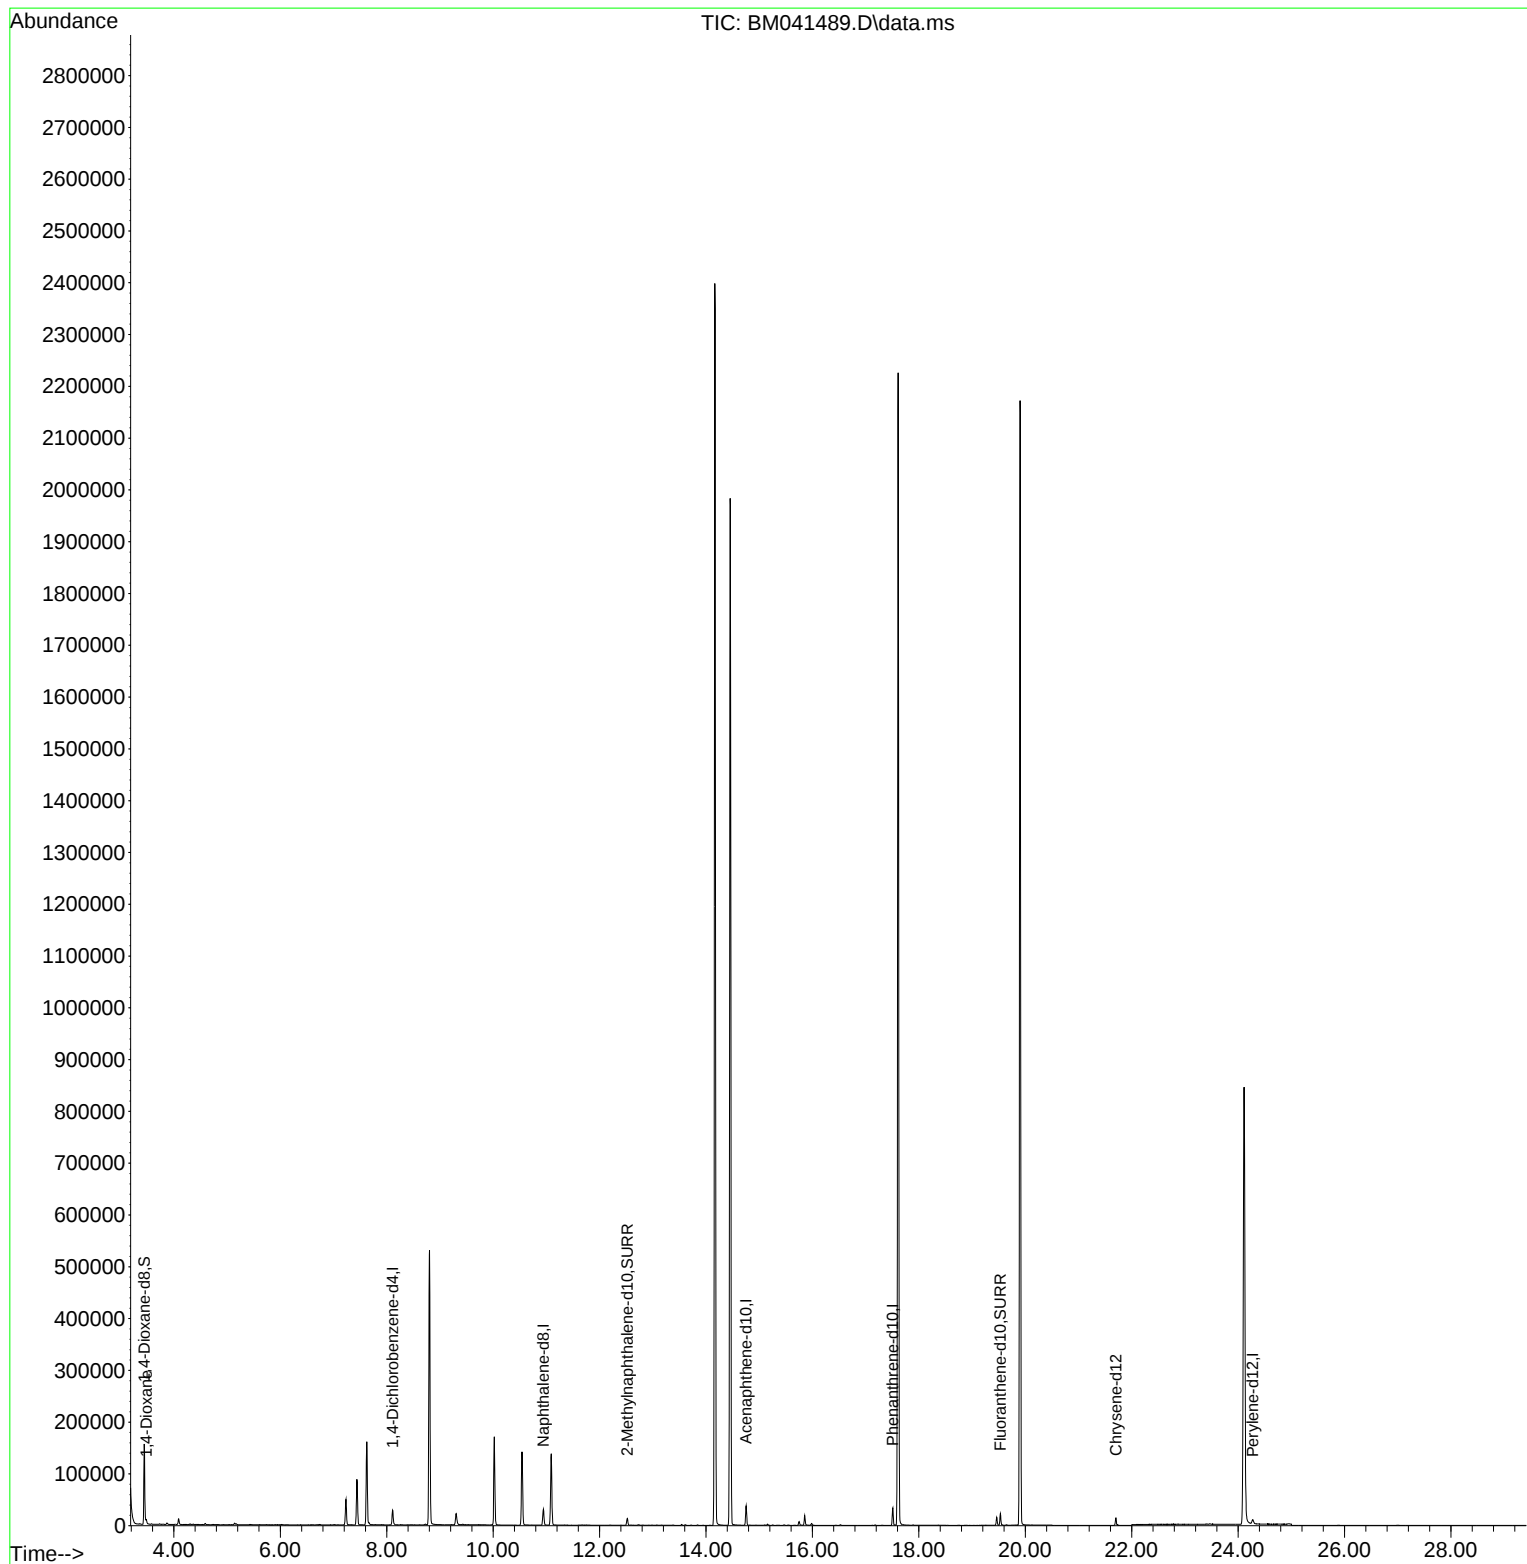

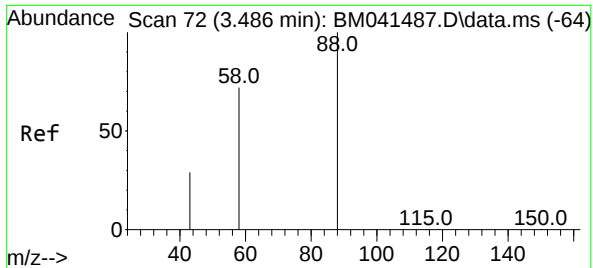

#2
 1,4-Dioxane
 Concen: 0.214 ng/ul
 RT: 3.482 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM041489.D
 Acq: 25 Aug 2023 09:35

Instrument :
 BNA_M
 ClientSampleId :
 BH962

Tgt Ion: 88 Resp: 3888

Ion	Ratio	Lower	Upper
88	100		
43	35.6	35.4	53.2
58	60.7	57.3	85.9

