

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022346.D
 Acq On : 27 Aug 2019 00:24
 Operator : HP/JU
 Sample : PB122397BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	33	rVB	6546	8676	0.84%	0.087%
2	3.440	74	77	80	rBV3	796	1082	0.10%	0.011%
3	3.810	138	140	144	rBV3	1332	1685	0.16%	0.017%
4	4.899	322	325	328	rVB3	882	1263	0.12%	0.013%
5	4.940	328	332	335	rBV2	752	1134	0.11%	0.011%
6	6.193	541	545	547	rBV	800	1159	0.11%	0.012%
7	6.745	633	639	652	rBV	134236	245298	23.70%	2.453%
8	6.904	660	666	677	rBV	96976	160929	15.55%	1.609%
9	7.081	691	696	707	rBV	167248	268594	25.95%	2.686%
10	7.545	768	775	785	rVB	130920	210195	20.31%	2.102%
11	8.269	892	898	917	rVB	181867	317676	30.69%	3.177%
12	8.716	968	974	991	rBV	153450	262196	25.33%	2.622%
13	9.428	1088	1095	1106	rBV	147549	245005	23.67%	2.450%
14	9.963	1180	1186	1205	rBV	168264	355803	34.37%	3.558%
15	10.316	1240	1246	1256	rVB	200796	324145	31.31%	3.242%
16	10.486	1269	1275	1292	rBV	143227	326561	31.55%	3.266%
17	11.945	1519	1523	1526	rBB	1841	2471	0.24%	0.025%
18	13.627	1803	1809	1819	rBV	392559	564791	54.56%	5.648%
19	13.892	1848	1854	1864	rBV	463667	671929	64.91%	6.719%
20	14.204	1901	1907	1915	rVB	322715	476177	46.00%	4.762%
21	14.486	1950	1955	1969	rBV2	55110	162802	15.73%	1.628%
22	15.204	2071	2077	2090	rBV	549753	835672	80.73%	8.357%
23	15.380	2102	2107	2118	rBV	88115	155350	15.01%	1.554%
24	15.451	2118	2119	2123	rVB2	5191	3626	0.35%	0.036%
25	15.721	2163	2165	2169	rBV	723	1227	0.12%	0.012%
26	16.962	2371	2376	2387	rVB2	424238	581184	56.15%	5.812%
27	17.068	2387	2394	2406	rBV	615908	910872	88.00%	9.109%
28	17.186	2411	2414	2415	rVB2	1307	1048	0.10%	0.010%
29	17.321	2434	2437	2439	rBV	1033	1044	0.10%	0.010%
30	17.468	2461	2462	2467	rVB	807	1193	0.12%	0.012%
31	17.515	2467	2470	2474	rBV	771	1345	0.13%	0.013%
32	17.580	2477	2481	2483	rBV2	806	1100	0.11%	0.011%
33	17.857	2526	2528	2531	rBV2	1103	1081	0.10%	0.011%
34	17.945	2540	2543	2545	rBV3	1566	1983	0.19%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022346.D
 Acq On : 27 Aug 2019 00:24
 Operator : HP/JU
 Sample : PB122397BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	17.986	2548	2550	2556	rVB2	1207	1770	0.17%	0.018%
36	18.204	2583	2587	2589	rBV3	998	1290	0.12%	0.013%
37	18.386	2617	2618	2622	rVB3	2015	2231	0.22%	0.022%
38	18.415	2622	2623	2626	rBV	1193	1209	0.12%	0.012%
39	18.792	2685	2687	2688	rBV	2108	1390	0.13%	0.014%
40	19.003	2721	2723	2730	rVB3	3726	5022	0.49%	0.050%
41	19.080	2734	2736	2738	rBV3	1141	1308	0.13%	0.013%
42	19.121	2741	2743	2746	rBV4	1507	1458	0.14%	0.015%
43	19.192	2753	2755	2758	rBV3	1693	1625	0.16%	0.016%
44	19.262	2764	2767	2770	rBV2	3702	4737	0.46%	0.047%
45	19.374	2780	2786	2797	rBV	753648	1035124	100.00%	10.352%
46	21.180	3088	3093	3103	rBV	390357	561868	54.28%	5.619%
47	23.227	3435	3441	3451	rVB	431016	796913	76.99%	7.969%
48	23.368	3460	3465	3474	rVB	255682	477491	46.13%	4.775%


Sum of corrected areas: 9999732

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
Data File : BM022346.D
Acq On : 27 Aug 2019 00:24
Operator : HP/JU
Sample : PB122397BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK97

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

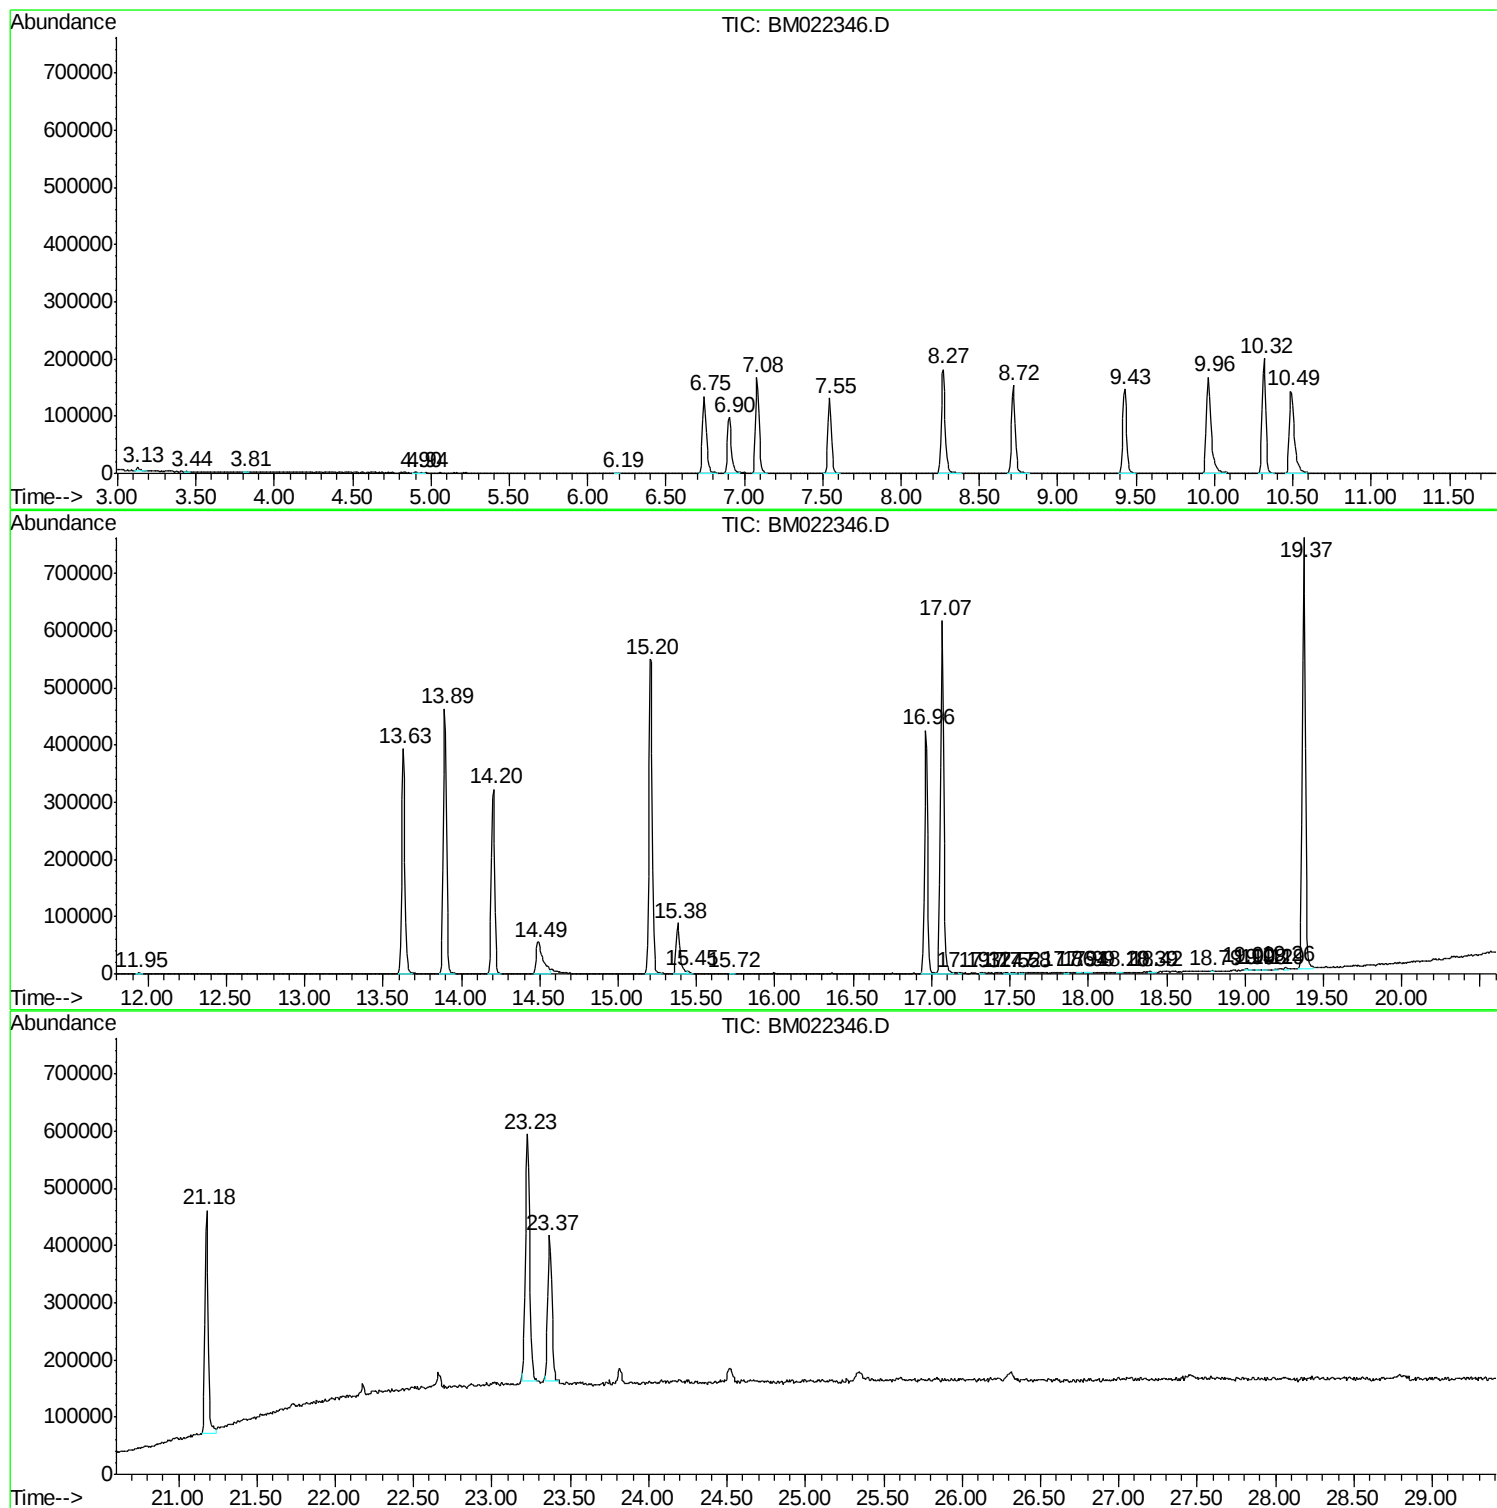

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022346.D
Acq On : 27 Aug 2019 00:24
Operator : HP/JU
Sample : PB122397BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK97

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022346.D
Acq On : 27 Aug 2019 00:24
Operator : HP/JU
Sample : PB122397BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK97

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc