

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022357.D
 Acq On : 27 Aug 2019 08:16
 Operator : HP/JU
 Sample : PB122457BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	33	rVB3	5189	10432	1.15%	0.114%
2	3.193	33	35	39	rBV3	723	1184	0.13%	0.013%
3	3.357	60	63	66	rVB2	1260	1565	0.17%	0.017%
4	3.387	66	68	71	rBV2	1122	1154	0.13%	0.013%
5	3.822	136	142	144	rBV4	1270	2253	0.25%	0.025%
6	6.745	633	639	648	rBV	113931	205809	22.65%	2.242%
7	6.904	658	666	677	rBV	80783	136658	15.04%	1.488%
8	6.992	679	681	684	rVB	1013	1053	0.12%	0.011%
9	7.028	684	687	690	rBV	743	1023	0.11%	0.011%
10	7.081	690	696	706	rVB	138910	223134	24.55%	2.430%
11	7.539	769	774	785	rBB	134407	221242	24.35%	2.410%
12	8.269	892	898	914	rVB	150741	263887	29.04%	2.874%
13	8.716	968	974	985	rBV	128779	219248	24.13%	2.388%
14	9.428	1089	1095	1108	rBV	119862	206361	22.71%	2.248%
15	9.963	1180	1186	1206	rBV	143043	296180	32.59%	3.226%
16	10.316	1239	1246	1253	rBV	212528	343870	37.84%	3.745%
17	10.492	1268	1276	1293	rBV	123304	276445	30.42%	3.011%
18	11.945	1518	1523	1526	rBB3	1401	2256	0.25%	0.025%
19	13.627	1803	1809	1822	rBV	318380	483630	53.22%	5.267%
20	13.892	1848	1854	1864	rBV	397848	572455	63.00%	6.235%
21	14.198	1900	1906	1917	rVB	339692	514756	56.65%	5.606%
22	14.498	1952	1957	1978	rBV2	42705	144607	15.91%	1.575%
23	15.204	2071	2077	2090	rBV	466178	707322	77.84%	7.704%
24	15.380	2102	2107	2116	rBV	79152	133168	14.65%	1.450%
25	15.445	2116	2118	2123	rVB	3824	5125	0.56%	0.056%
26	16.751	2337	2340	2345	rVB2	721	1125	0.12%	0.012%
27	16.962	2370	2376	2386	rBV2	491513	650616	71.60%	7.086%
28	17.062	2386	2393	2408	rVV	525332	788286	86.75%	8.585%
29	17.404	2448	2451	2454	rBV	638	1175	0.13%	0.013%
30	17.821	2518	2522	2524	rBV2	1343	1725	0.19%	0.019%
31	17.968	2545	2547	2550	rBV2	808	1076	0.12%	0.012%
32	18.015	2552	2555	2556	rBV2	1073	1135	0.12%	0.012%
33	18.098	2565	2569	2570	rBV2	1161	1275	0.14%	0.014%
34	18.198	2582	2586	2589	rVB3	977	1195	0.13%	0.013%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022357.D
 Acq On : 27 Aug 2019 08:16
 Operator : HP/JU
 Sample : PB122457BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	18.598	2652	2654	2656	rBV	1527	1516	0.17%	0.017%
36	18.645	2659	2662	2664	rBV2	1007	995	0.11%	0.011%
37	18.715	2672	2674	2677	rVB3	1804	1771	0.19%	0.019%
38	18.751	2677	2680	2681	rBV2	1871	1904	0.21%	0.021%
39	18.768	2681	2683	2685	rVV2	1224	1148	0.13%	0.013%
40	18.803	2687	2689	2691	rVB	1310	1220	0.13%	0.013%
41	18.833	2691	2694	2695	rBV3	1563	1500	0.17%	0.016%
42	18.898	2703	2705	2707	rBV3	1137	949	0.10%	0.010%
43	19.015	2718	2725	2727	rBV3	4451	6516	0.72%	0.071%
44	19.262	2764	2767	2772	rVB	3333	4445	0.49%	0.048%
45	19.303	2772	2774	2776	rBV2	1288	1333	0.15%	0.015%
46	19.374	2780	2786	2796	rVV	647099	908725	100.00%	9.897%
47	19.839	2863	2865	2868	rBV3	2342	1681	0.18%	0.018%
48	20.145	2916	2917	2919	rBV2	3030	2091	0.23%	0.023%
49	21.180	3088	3093	3102	rBV	429004	607103	66.81%	6.612%
50	23.233	3435	3442	3453	rVB	356994	692841	76.24%	7.546%
51	23.374	3460	3466	3473	rVB	276397	523536	57.61%	5.702%


Sum of corrected areas: 9181699

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
Data File : BM022357.D
Acq On : 27 Aug 2019 08:16
Operator : HP/JU
Sample : PB122457BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

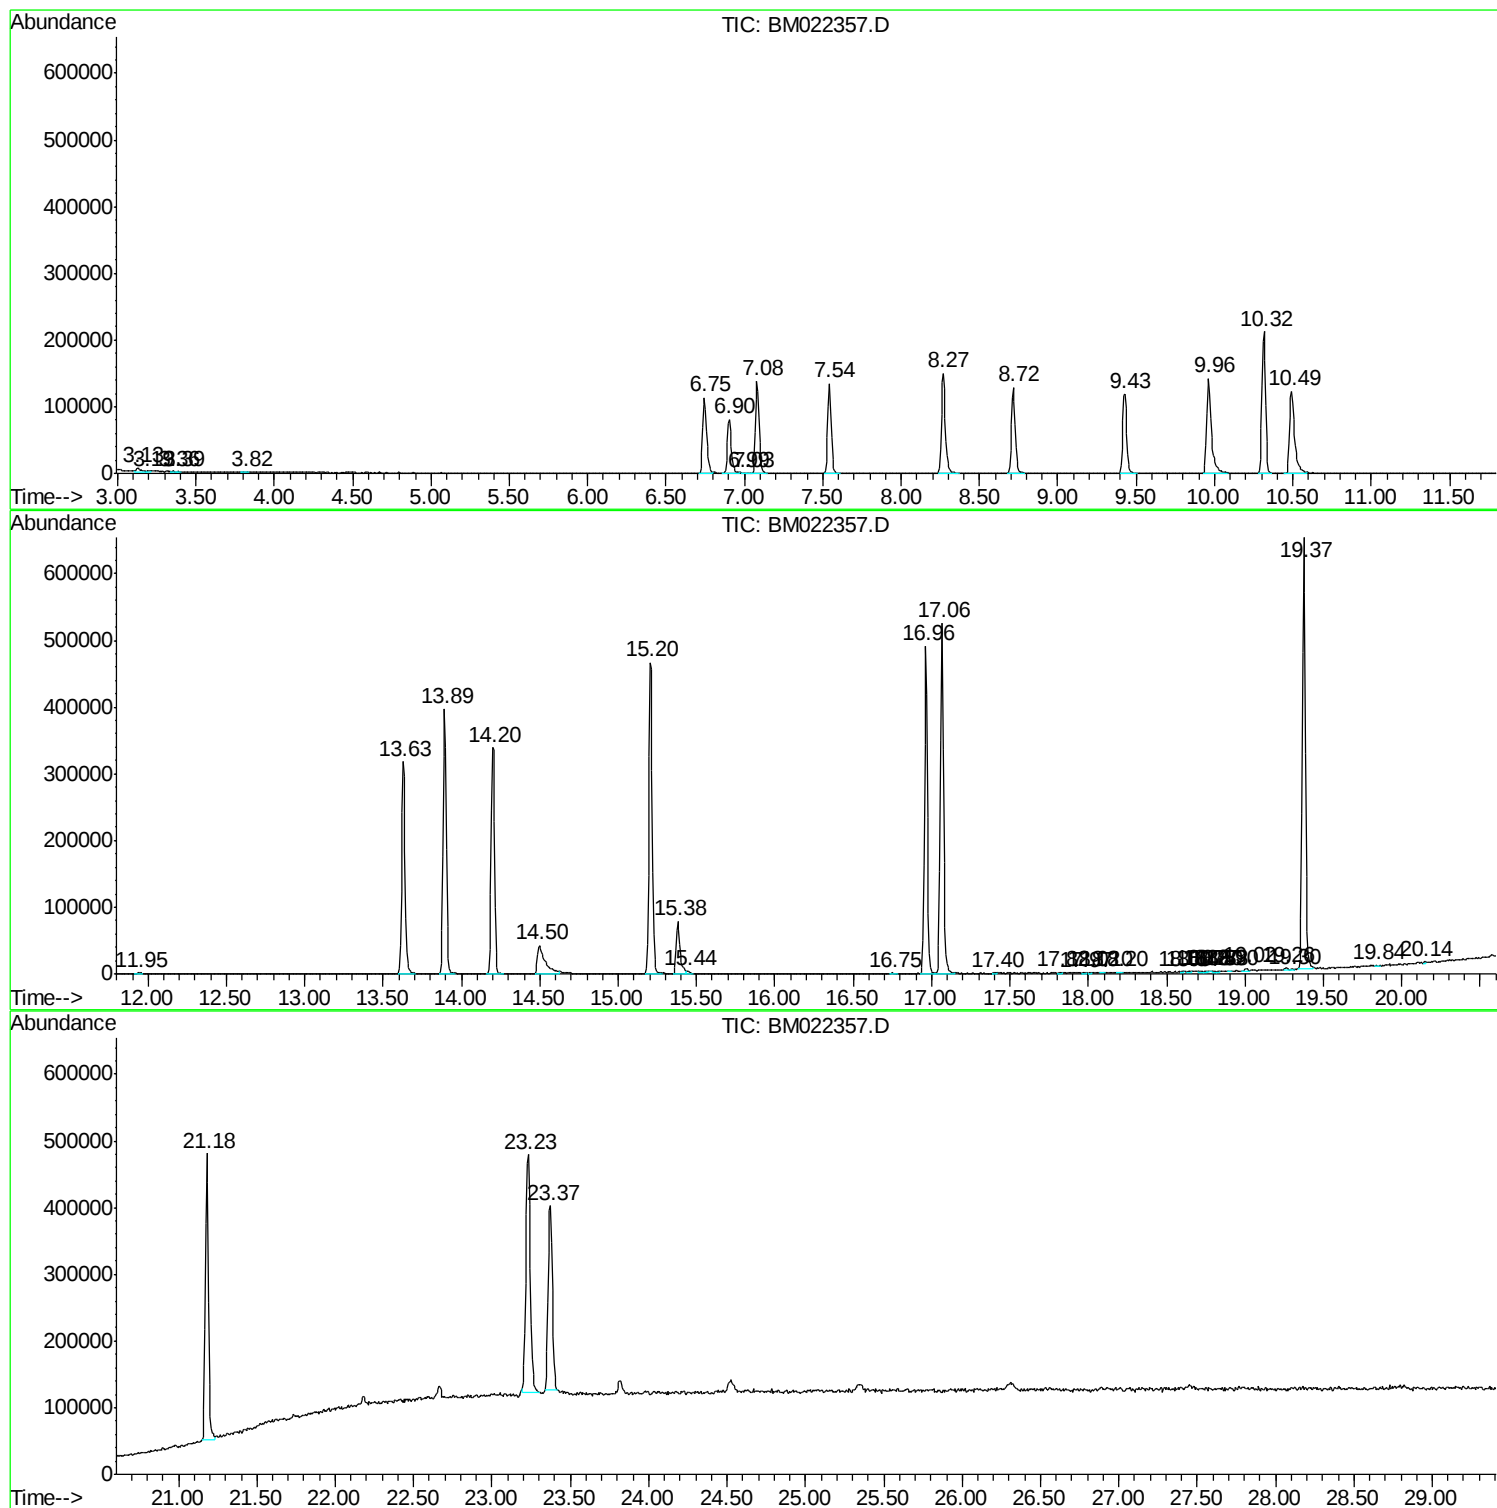

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022357.D
Acq On : 27 Aug 2019 08:16
Operator : HP/JU
Sample : PB122457BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022357.D
Acq On : 27 Aug 2019 08:16
Operator : HP/JU
Sample : PB122457BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc