

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022363.D
 Acq On : 27 Aug 2019 11:54
 Operator : HP/JU
 Sample : K4414-02MS
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJQ7MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	30	rVB	5659	8112	0.60%	0.045%
2	3.711	118	123	130	rBV2	4277	7984	0.59%	0.044%
3	3.805	135	139	148	rVV	64473	99401	7.32%	0.552%
4	4.199	202	206	209	rVV	2420	2901	0.21%	0.016%
5	5.081	351	356	363	rVB	31265	44985	3.31%	0.250%
6	5.228	373	381	387	rBV2	23869	51606	3.80%	0.287%
7	5.563	432	438	444	rBV3	59056	116296	8.56%	0.646%
8	6.516	596	600	601	rBV	1522	1772	0.13%	0.010%
9	6.616	613	617	621	rBB2	2666	3970	0.29%	0.022%
10	6.681	622	628	632	rBB2	1187	2511	0.18%	0.014%
11	6.763	634	642	655	rVB3	47381	130859	9.63%	0.727%
12	6.899	659	665	674	rVV	91440	160637	11.82%	0.892%
13	6.963	674	676	680	rVB	2518	2943	0.22%	0.016%
14	7.081	690	696	698	rBV	134990	214257	15.77%	1.190%
15	7.110	698	701	708	rVV	137686	213887	15.74%	1.188%
16	7.175	708	712	720	rVB3	23370	41458	3.05%	0.230%
17	7.275	725	729	733	rBB	2006	2718	0.20%	0.015%
18	7.540	768	774	777	rBV	168305	276036	20.32%	1.533%
19	7.575	777	780	787	rVV	194013	287184	21.14%	1.595%
20	7.634	787	790	796	rVB2	7202	10118	0.74%	0.056%
21	7.716	800	804	808	rVB3	3481	5198	0.38%	0.029%
22	7.893	829	834	841	rBB	24690	35280	2.60%	0.196%
23	8.063	857	863	871	rVB	160651	254409	18.72%	1.413%
24	8.269	892	898	906	rBV	95357	163761	12.05%	0.909%
25	8.352	906	912	922	rVV	163009	249819	18.39%	1.387%
26	8.710	967	973	986	rBV	150648	254792	18.75%	1.415%
27	9.022	1020	1026	1029	rBV	3748	4553	0.34%	0.025%
28	9.422	1088	1094	1104	rVB	143261	239822	17.65%	1.332%
29	9.557	1113	1117	1120	rBV2	1785	1823	0.13%	0.010%
30	9.710	1137	1143	1144	rBV3	6471	10213	0.75%	0.057%
31	9.740	1144	1148	1155	rVB3	9167	17759	1.31%	0.099%
32	9.804	1155	1159	1163	rBV3	7900	13708	1.01%	0.076%
33	9.846	1163	1166	1170	rVB	4924	7805	0.57%	0.043%
34	9.963	1179	1186	1201	rBV	154026	349992	25.76%	1.944%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022363.D
 Acq On : 27 Aug 2019 11:54
 Operator : HP/JU
 Sample : K4414-02MS
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJQ7MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	10.175	1214	1222	1232	rBB	279546	436958	32.16%	2.427%
36	10.310	1238	1245	1249	rBV	238486	398542	29.33%	2.213%
37	10.363	1249	1254	1262	rVV	753747	1182103	87.00%	6.565%
38	10.487	1268	1275	1287	rBB2	15747	29520	2.17%	0.164%
39	11.504	1444	1448	1451	rBB	2303	2967	0.22%	0.016%
40	11.640	1465	1471	1489	rBV	180056	347863	25.60%	1.932%
41	11.916	1515	1518	1522	rBB	1815	2934	0.22%	0.016%
42	11.992	1526	1531	1538	rBB	9957	15278	1.12%	0.085%
43	12.210	1559	1568	1575	rBB	45497	71144	5.24%	0.395%
44	13.022	1702	1706	1713	rBB2	16509	24010	1.77%	0.133%
45	13.510	1785	1789	1793	rBV2	4421	6796	0.50%	0.038%
46	13.569	1795	1799	1802	rBB	1307	1916	0.14%	0.011%
47	13.628	1802	1809	1814	rBV	425202	614171	45.20%	3.411%
48	13.675	1814	1817	1824	rVB	22447	31424	2.31%	0.175%
49	13.739	1825	1828	1836	rBB2	1986	3298	0.24%	0.018%
50	13.886	1847	1853	1864	rBV	484475	758765	55.85%	4.214%
51	14.198	1899	1906	1911	rBV	405611	582024	42.84%	3.232%
52	14.263	1911	1917	1926	rVB	541396	779333	57.36%	4.328%
53	14.504	1950	1958	1971	rBV6	27777	88770	6.53%	0.493%
54	14.622	1972	1978	1989	rVB	276154	430803	31.71%	2.392%
55	14.757	1997	2001	2006	rBV	12245	17543	1.29%	0.097%
56	15.204	2071	2077	2083	rBV	654859	906357	66.71%	5.034%
57	15.257	2083	2086	2092	rVB2	3483	5812	0.43%	0.032%
58	15.375	2101	2106	2114	rBV	165908	248911	18.32%	1.382%
59	15.439	2114	2117	2120	rVB2	4514	6320	0.47%	0.035%
60	15.992	2207	2211	2212	rBV	2212	2089	0.15%	0.012%
61	16.622	2313	2318	2329	rBV	329863	468472	34.48%	2.602%
62	16.786	2342	2346	2348	rVB	2176	2606	0.19%	0.014%
63	16.963	2370	2376	2380	rBV	557298	732333	53.90%	4.067%
64	17.004	2380	2383	2387	rVV	52633	66339	4.88%	0.368%
65	17.063	2387	2393	2403	rVB	804299	1073540	79.01%	5.962%
66	17.398	2447	2450	2455	rVB3	1450	2133	0.16%	0.012%
67	17.569	2475	2479	2483	rVB2	19907	22907	1.69%	0.127%
68	17.857	2522	2528	2538	rBV2	67218	94755	6.97%	0.526%
69	18.033	2552	2558	2562	rBV2	5855	9846	0.72%	0.055%
70	18.133	2573	2575	2579	rBV4	1697	2104	0.15%	0.012%
71	18.363	2609	2614	2615	rVV4	1479	1877	0.14%	0.010%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022363.D
 Acq On : 27 Aug 2019 11:54
 Operator : HP/JU
 Sample : K4414-02MS
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJQ7MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	18.486	2631	2635	2637	rBV5	1772	1820	0.13%	0.010%
73	18.598	2652	2654	2655	rBV2	2179	1805	0.13%	0.010%
74	18.745	2675	2679	2680	rBV2	1974	2620	0.19%	0.015%
75	18.774	2683	2684	2688	rVB4	2598	1732	0.13%	0.010%
76	18.886	2700	2703	2706	rBV3	1896	1894	0.14%	0.011%
77	18.921	2706	2709	2711	rBV3	1348	1806	0.13%	0.010%
78	18.974	2715	2718	2720	rVV2	2130	3056	0.22%	0.017%
79	19.004	2720	2723	2726	rVV	8742	11147	0.82%	0.062%
80	19.033	2726	2728	2733	rVB	11006	12565	0.92%	0.070%
81	19.151	2744	2748	2753	rBV3	31857	45785	3.37%	0.254%
82	19.186	2753	2754	2759	rVV2	4461	5336	0.39%	0.030%
83	19.257	2763	2766	2768	rVV	6711	8165	0.60%	0.045%
84	19.280	2768	2770	2774	rVB	8181	9318	0.69%	0.052%
85	19.310	2774	2775	2779	rBV4	1503	1862	0.14%	0.010%
86	19.368	2779	2785	2788	rBV	952543	1358667	100.00%	7.545%
87	19.404	2788	2791	2799	rVB	960852	1178633	86.75%	6.546%
88	19.716	2842	2844	2847	rBV3	2269	2419	0.18%	0.013%
89	19.880	2869	2872	2873	rBV2	2992	3050	0.22%	0.017%
90	19.904	2873	2876	2878	rVB2	7030	7189	0.53%	0.040%
91	20.174	2920	2922	2923	rBV2	2768	2167	0.16%	0.012%
92	20.398	2958	2960	2965	rVB4	11413	13699	1.01%	0.076%
93	20.868	3036	3040	3045	rBV2	64635	86772	6.39%	0.482%
94	21.174	3087	3092	3100	rBV	531199	703324	51.77%	3.906%
95	21.304	3111	3114	3119	rBV2	33074	37457	2.76%	0.208%
96	21.727	3183	3186	3189	rBV2	29483	34158	2.51%	0.190%
97	22.174	3259	3262	3267	rBV3	39278	45845	3.37%	0.255%
98	22.662	3341	3345	3351	rVB2	45493	65806	4.84%	0.365%
99	23.227	3433	3441	3450	rVB	504819	966459	71.13%	5.367%
100	23.368	3459	3465	3477	rVB	313803	630807	46.43%	3.503%


Sum of corrected areas: 18006495

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
Data File : BM022363.D
Acq On : 27 Aug 2019 11:54
Operator : HP/JU
Sample : K4414-02MS
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJQ7MS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

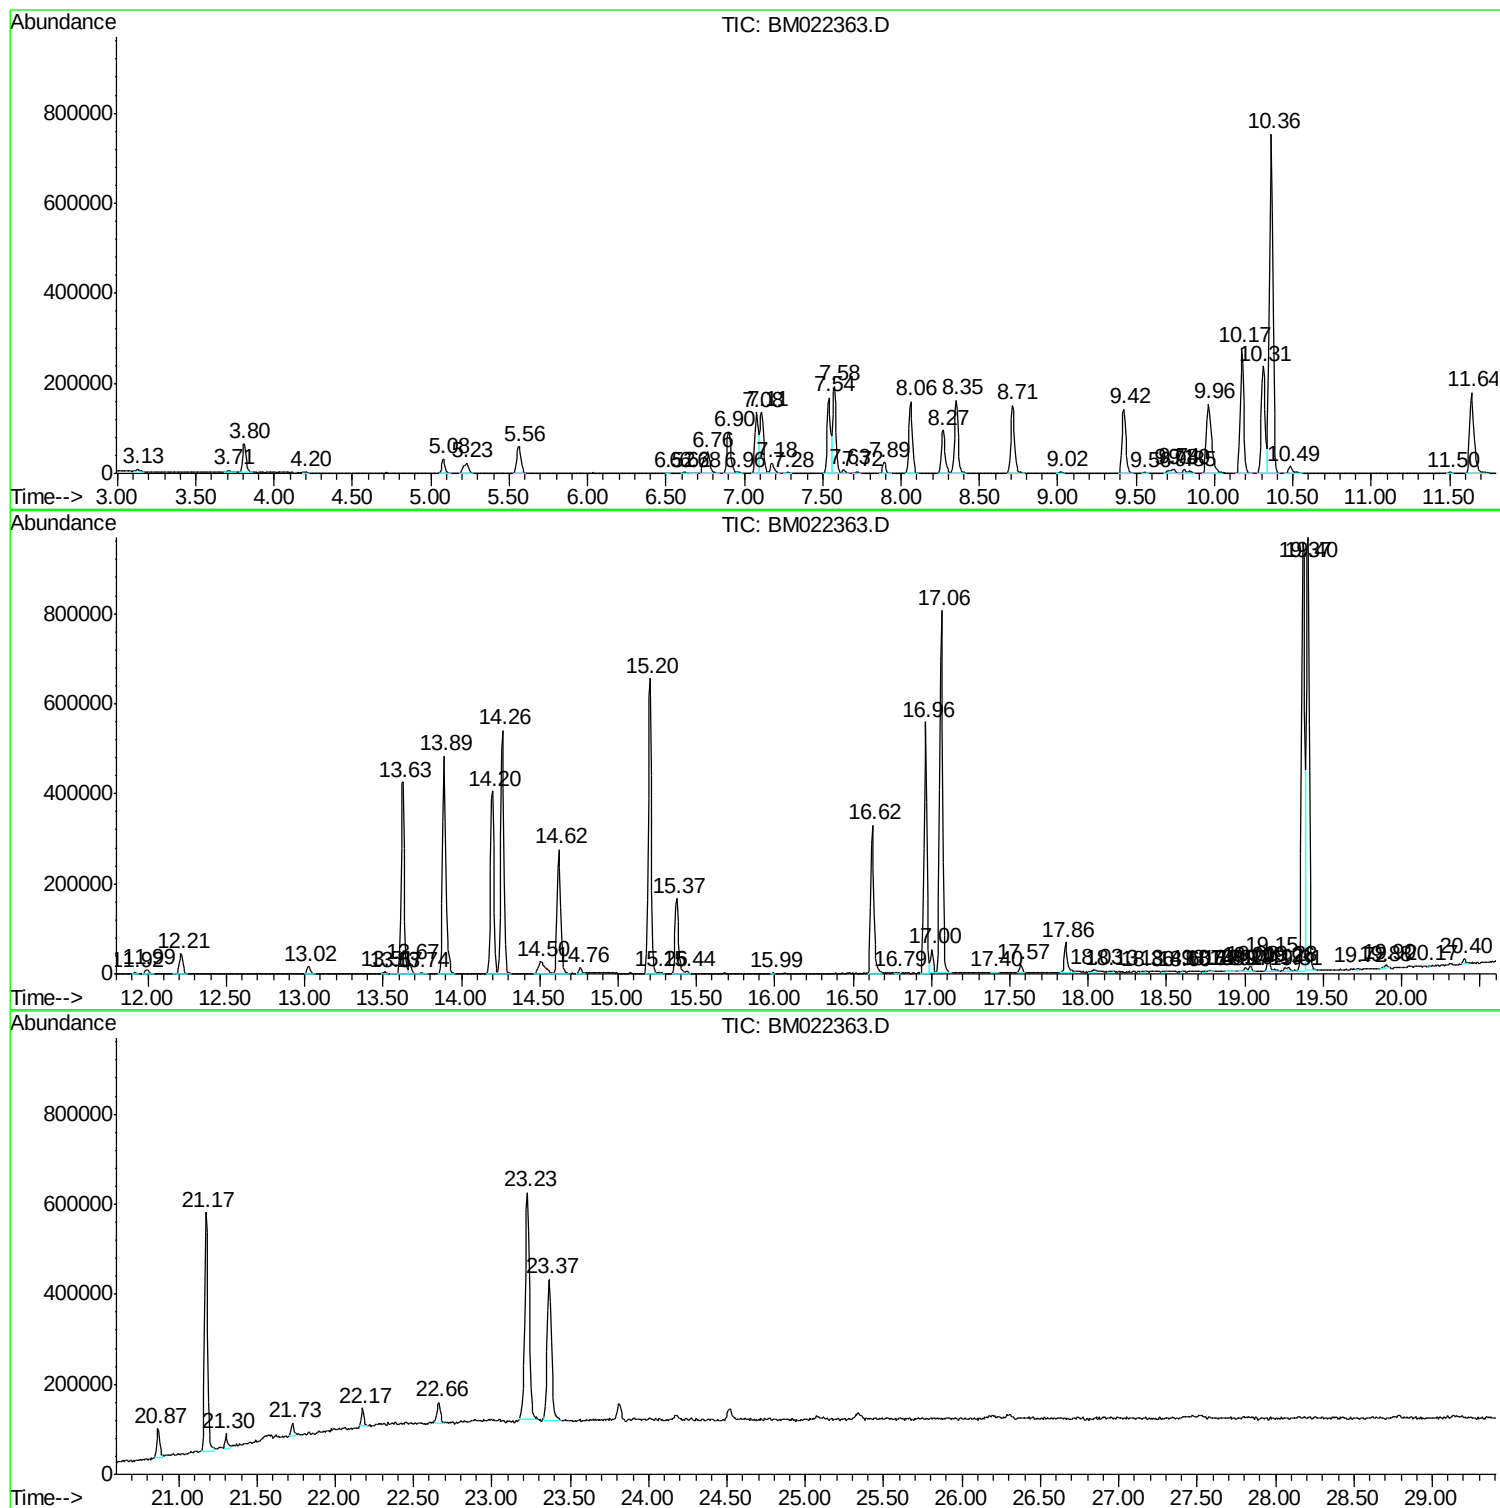

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022363.D
Acq On : 27 Aug 2019 11:54
Operator : HP/JU
Sample : K4414-02MS
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJQ7MS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022363.D
Acq On : 27 Aug 2019 11:54
Operator : HP/JU
Sample : K4414-02MS
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJQ7MS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc