

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022371.D
 Acq On : 27 Aug 2019 17:48
 Operator : HP/JU
 Sample : K4373-14DL2 500X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD2DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	100	102	106	rVB2	729	696	0.17%	0.031%
2	3.657	111	114	118	rVB3	906	1243	0.31%	0.054%
3	3.916	155	158	160	rBV2	813	910	0.23%	0.040%
4	4.257	215	216	219	rBV	890	704	0.17%	0.031%
5	4.557	265	267	271	rBV	791	1088	0.27%	0.048%
6	4.598	271	274	276	rVB2	992	933	0.23%	0.041%
7	4.634	276	280	282	rBV2	596	914	0.23%	0.040%
8	4.740	296	298	301	rVB	754	727	0.18%	0.032%
9	4.763	301	302	305	rBV	647	632	0.16%	0.028%
10	4.804	308	309	311	rBV2	844	688	0.17%	0.030%
11	5.163	366	370	373	rBV	402	651	0.16%	0.029%
12	5.622	446	448	451	rVB	514	565	0.14%	0.025%
13	5.681	455	458	461	rBV	773	1007	0.25%	0.044%
14	5.775	470	474	475	rVB	541	680	0.17%	0.030%
15	5.810	479	480	484	rBV	395	625	0.16%	0.027%
16	5.916	495	498	499	rBV	710	697	0.17%	0.031%
17	6.063	520	523	526	rBB	683	743	0.18%	0.033%
18	6.298	560	563	566	rBB	507	691	0.17%	0.030%
19	6.328	566	568	571	rBB	706	681	0.17%	0.030%
20	6.357	571	573	576	rBV	549	694	0.17%	0.030%
21	6.834	651	654	657	rBB	496	670	0.17%	0.029%
22	7.275	725	729	730	rBB	797	808	0.20%	0.035%
23	7.428	752	755	759	rBB	438	668	0.17%	0.029%
24	7.539	769	774	791	rBB	80557	142322	35.35%	6.239%
25	7.687	797	799	803	rBV	388	746	0.19%	0.033%
26	7.898	830	835	841	rBV	3845	5968	1.48%	0.262%
27	8.081	862	866	869	rBV2	1051	1383	0.34%	0.061%
28	9.298	1071	1073	1077	rBB	442	656	0.16%	0.029%
29	9.551	1111	1116	1118	rBV	5189	8299	2.06%	0.364%
30	9.675	1134	1137	1138	rBV	651	568	0.14%	0.025%
31	9.692	1138	1140	1143	rVB	675	620	0.15%	0.027%
32	9.863	1163	1169	1176	rBB3	4248	9100	2.26%	0.399%
33	9.998	1190	1192	1194	rBV3	675	648	0.16%	0.028%
34	10.263	1233	1237	1239	rBV	747	989	0.25%	0.043%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022371.D
 Acq On : 27 Aug 2019 17:48
 Operator : HP/JU
 Sample : K4373-14DL2 500X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD2DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	10.310	1239	1245	1249	rVV	131524	222431	55.25%	9.751%
36	10.363	1249	1254	1267	rVV	184436	323920	80.46%	14.200%
37	10.492	1270	1276	1283	rVB2	9787	16273	4.04%	0.713%
38	10.898	1342	1345	1351	rBV	1092	2583	0.64%	0.113%
39	10.980	1356	1359	1362	rBV	829	1049	0.26%	0.046%
40	11.204	1390	1397	1400	rBV2	2016	2906	0.72%	0.127%
41	11.233	1400	1402	1404	rVB2	704	601	0.15%	0.026%
42	11.392	1427	1429	1431	rVB2	1225	843	0.21%	0.037%
43	11.439	1431	1437	1440	rBB	1977	2570	0.64%	0.113%
44	12.004	1527	1533	1542	rBB	11559	20343	5.05%	0.892%
45	12.222	1565	1570	1575	rBB2	5597	9730	2.42%	0.427%
46	14.198	1900	1906	1914	rBV	208655	329804	81.92%	14.458%
47	14.268	1914	1918	1922	rVB4	4968	8333	2.07%	0.365%
48	14.410	1938	1942	1944	rBV	780	1084	0.27%	0.048%
49	14.457	1948	1950	1954	rBB2	895	1248	0.31%	0.055%
50	14.574	1966	1970	1971	rBV2	1202	1360	0.34%	0.060%
51	14.633	1977	1980	1985	rVB	2433	3777	0.94%	0.166%
52	14.851	2013	2017	2019	rBB	417	658	0.16%	0.029%
53	14.992	2037	2041	2043	rBB	419	653	0.16%	0.029%
54	15.021	2043	2046	2047	rBV2	2548	2791	0.69%	0.122%
55	15.063	2051	2053	2057	rVB	702	1036	0.26%	0.045%
56	15.110	2058	2061	2065	rBV	496	970	0.24%	0.043%
57	15.280	2086	2090	2095	rBB2	2558	4322	1.07%	0.189%
58	16.010	2212	2214	2221	rBV3	1210	1852	0.46%	0.081%
59	16.274	2256	2259	2262	rBV	953	1278	0.32%	0.056%
60	16.968	2371	2377	2388	rBV	245951	402603	100.00%	17.650%
61	17.080	2394	2396	2402	rVB	1296	2141	0.53%	0.094%
62	17.251	2422	2425	2428	rBV	551	661	0.16%	0.029%
63	17.409	2448	2452	2457	rBV	4336	6045	1.50%	0.265%
64	17.815	2519	2521	2524	rVB	853	700	0.17%	0.031%
65	17.880	2528	2532	2534	rVB	749	889	0.22%	0.039%
66	17.933	2540	2541	2545	rBV	690	630	0.16%	0.028%
67	17.980	2547	2549	2550	rBV	794	608	0.15%	0.027%
68	18.033	2556	2558	2559	rBV	631	575	0.14%	0.025%
69	18.092	2567	2568	2575	rBV	695	1383	0.34%	0.061%
70	18.139	2575	2576	2578	rVB	1322	609	0.15%	0.027%
71	18.251	2593	2595	2596	rBV	856	699	0.17%	0.031%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022371.D
 Acq On : 27 Aug 2019 17:48
 Operator : HP/JU
 Sample : K4373-14DL2 500X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD2DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	18.315	2604	2606	2608	rVB	878	678	0.17%	0.030%
73	18.362	2612	2614	2616	rVB	1113	787	0.20%	0.035%
74	18.433	2623	2626	2627	rBV	1155	932	0.23%	0.041%
75	18.451	2627	2629	2631	rBV	806	751	0.19%	0.033%
76	18.492	2635	2636	2638	rVB	914	610	0.15%	0.027%
77	18.592	2651	2653	2654	rVB2	1069	647	0.16%	0.028%
78	18.609	2654	2656	2658	rBV	911	767	0.19%	0.034%
79	18.668	2664	2666	2669	rVB3	1137	1053	0.26%	0.046%
80	18.727	2674	2676	2677	rBV	943	777	0.19%	0.034%
81	19.062	2731	2733	2736	rBV2	1612	1041	0.26%	0.046%
82	21.180	3088	3093	3100	rBV	254777	367670	91.32%	16.118%
83	23.368	3461	3465	3478	rVB2	162458	336416	83.56%	14.748%


Sum of corrected areas: 2281101

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
Data File : BM022371.D
Acq On : 27 Aug 2019 17:48
Operator : HP/JU
Sample : K4373-14DL2 500X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

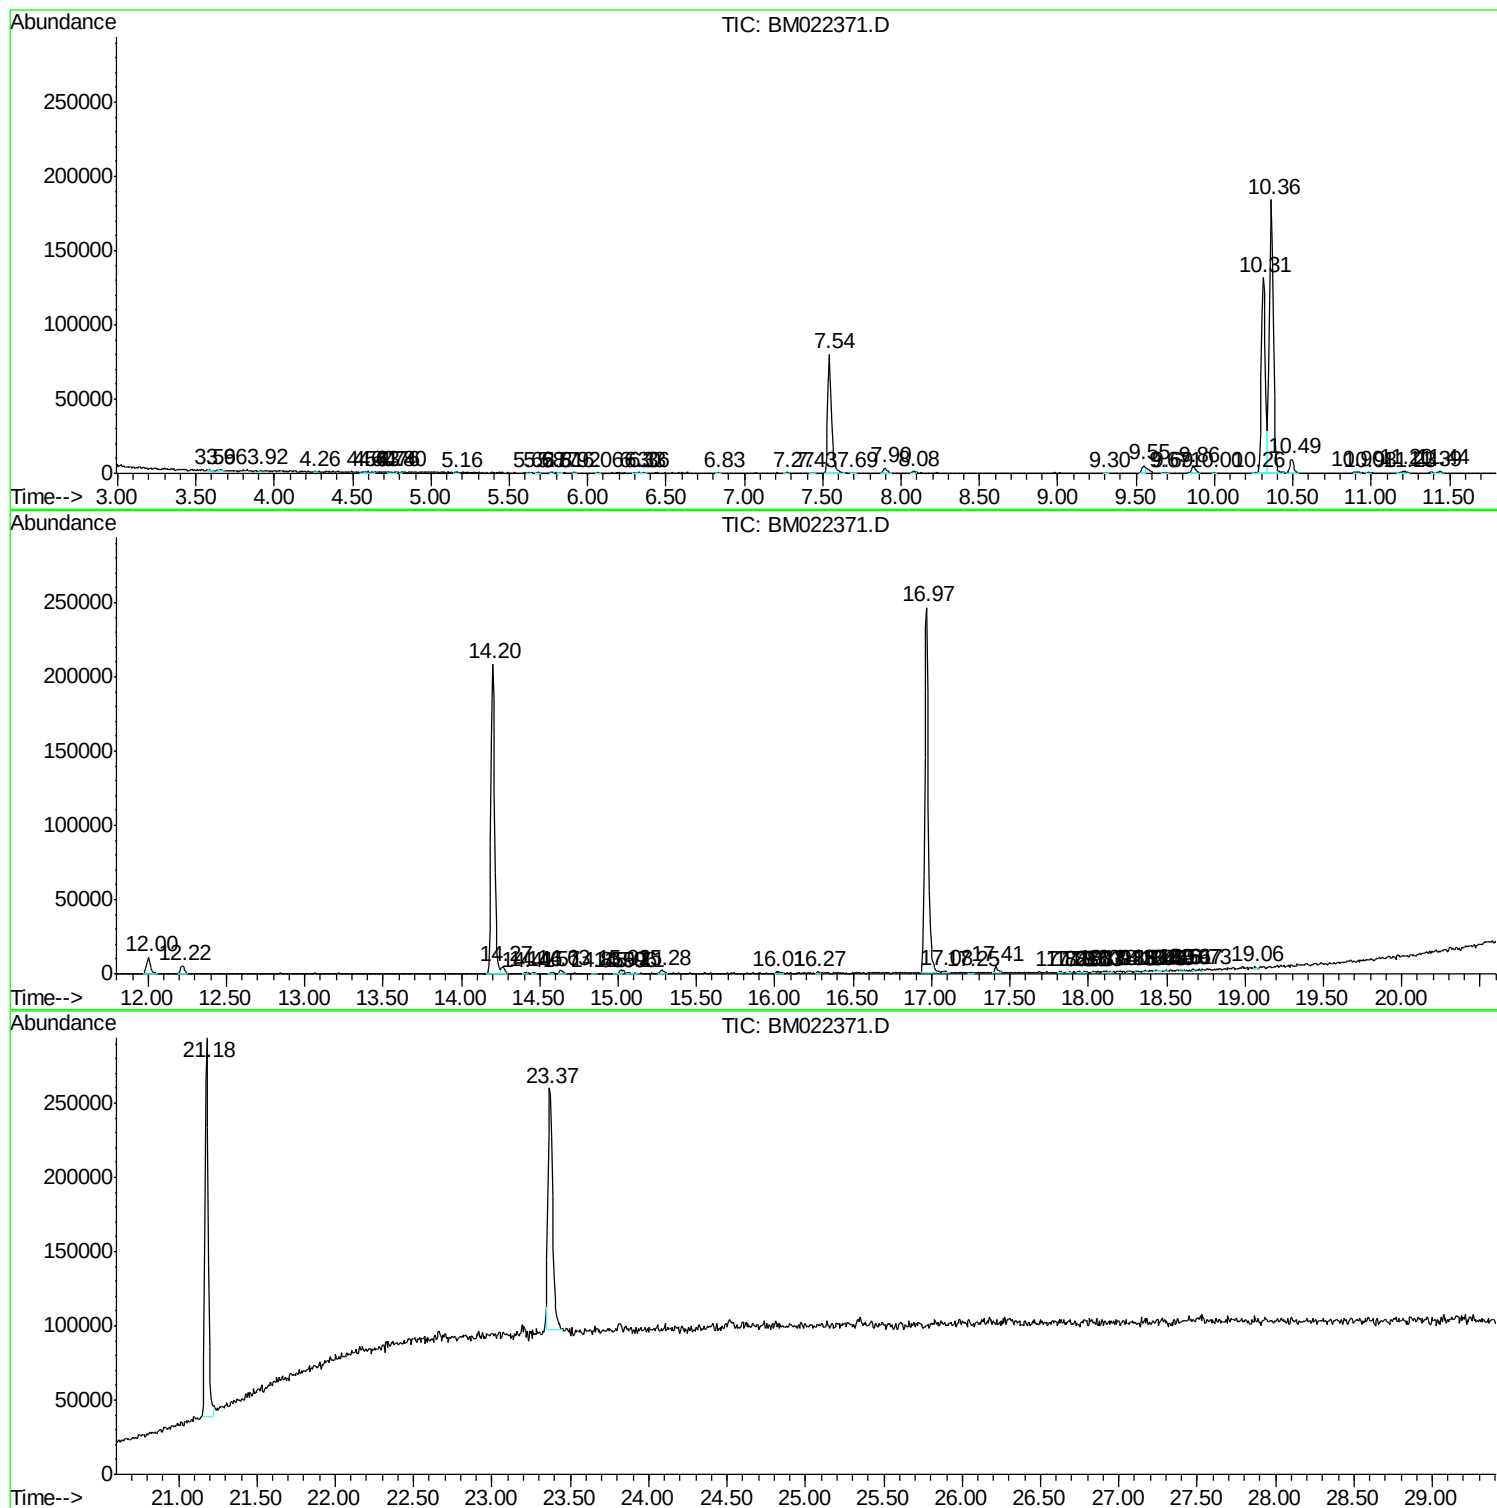

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022371.D
Acq On : 27 Aug 2019 17:48
Operator : HP/JU
Sample : K4373-14DL2 500X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022371.D
Acq On : 27 Aug 2019 17:48
Operator : HP/JU
Sample : K4373-14DL2 500X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc