

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022376.D
 Acq On : 27 Aug 2019 20:49
 Operator : HP/JU
 Sample : K4513-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	57	59	64	rVB3	888	1023	0.24%	0.051%
2	3.422	72	74	78	rVV4	685	849	0.20%	0.042%
3	3.463	79	81	83	rVB2	737	597	0.14%	0.030%
4	3.557	95	97	101	rVB2	521	670	0.16%	0.033%
5	4.016	174	175	179	rVB	640	693	0.16%	0.034%
6	4.381	236	237	240	rBV	827	579	0.14%	0.029%
7	4.487	252	255	256	rBV	638	706	0.17%	0.035%
8	4.504	256	258	260	rVB	736	600	0.14%	0.030%
9	4.622	275	278	283	rVV2	628	1083	0.26%	0.054%
10	4.763	299	302	304	rBV	694	761	0.18%	0.038%
11	4.887	320	323	327	rBV	641	951	0.22%	0.047%
12	5.040	348	349	354	rVV2	771	1025	0.24%	0.051%
13	5.087	356	357	361	rVV	699	532	0.13%	0.026%
14	5.122	361	363	367	rVB	472	548	0.13%	0.027%
15	5.810	479	480	485	rVB	845	1047	0.25%	0.052%
16	5.969	505	507	510	rBV	504	684	0.16%	0.034%
17	6.351	570	572	574	rVB	762	569	0.13%	0.028%
18	6.369	574	575	578	rBV	481	605	0.14%	0.030%
19	6.610	613	616	619	rVB2	976	1158	0.27%	0.057%
20	7.039	686	689	690	rBB2	682	525	0.12%	0.026%
21	7.110	699	701	706	rBB	476	840	0.20%	0.042%
22	7.175	710	712	715	rBB	473	531	0.13%	0.026%
23	7.228	718	721	723	rBB	415	546	0.13%	0.027%
24	7.316	733	736	737	rBV	436	520	0.12%	0.026%
25	7.481	761	764	767	rBV	399	749	0.18%	0.037%
26	7.539	769	774	789	rBV	86232	153165	36.15%	7.585%
27	7.634	789	790	792	rVB	933	507	0.12%	0.025%
28	7.710	800	803	805	rBV	427	635	0.15%	0.031%
29	7.881	830	832	837	rBB	406	756	0.18%	0.037%
30	7.969	845	847	851	rBV	453	740	0.17%	0.037%
31	8.004	851	853	856	rVB	432	528	0.12%	0.026%
32	8.081	864	866	869	rBB	525	557	0.13%	0.028%
33	8.169	879	881	884	rBB	407	544	0.13%	0.027%
34	8.469	929	932	933	rBV	460	511	0.12%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022376.D
 Acq On : 27 Aug 2019 20:49
 Operator : HP/JU
 Sample : K4513-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	8.663	964	965	968	rBV	492	556	0.13%	0.028%
36	9.004	1021	1023	1026	rBB	416	514	0.12%	0.025%
37	9.033	1026	1028	1031	rBV	417	599	0.14%	0.030%
38	9.110	1039	1041	1044	rBB	449	587	0.14%	0.029%
39	9.616	1125	1127	1130	rBB	461	560	0.13%	0.028%
40	9.651	1130	1133	1137	rBV	516	926	0.22%	0.046%
41	10.245	1232	1234	1237	rVB	459	527	0.12%	0.026%
42	10.316	1240	1246	1258	rBV	105458	220811	52.11%	10.935%
43	10.416	1262	1263	1267	rVB	897	855	0.20%	0.042%
44	10.704	1309	1312	1315	rBV	423	798	0.19%	0.040%
45	10.927	1348	1350	1353	rBV	414	605	0.14%	0.030%
46	11.057	1368	1372	1375	rBB	379	591	0.14%	0.029%
47	11.398	1428	1430	1433	rVB	448	526	0.12%	0.026%
48	11.563	1456	1458	1461	rVB	466	541	0.13%	0.027%
49	13.527	1790	1792	1795	rVB	403	510	0.12%	0.025%
50	13.904	1854	1856	1859	rBB	550	566	0.13%	0.028%
51	14.198	1901	1906	1917	rBV	188678	343368	81.03%	17.004%
52	14.310	1924	1925	1928	rVB	1283	834	0.20%	0.041%
53	14.404	1940	1941	1944	rBV	399	527	0.12%	0.026%
54	14.621	1975	1978	1981	rBV	465	814	0.19%	0.040%
55	14.857	2017	2018	2022	rBV	379	591	0.14%	0.029%
56	14.910	2025	2027	2029	rBV	405	521	0.12%	0.026%
57	15.157	2068	2069	2073	rVB	433	536	0.13%	0.027%
58	15.357	2099	2103	2104	rBV	527	780	0.18%	0.039%
59	15.421	2111	2114	2117	rVB	485	739	0.17%	0.037%
60	15.457	2117	2120	2123	rBV	457	802	0.19%	0.040%
61	15.580	2139	2141	2143	rVB	531	516	0.12%	0.026%
62	15.609	2143	2146	2147	rBV	478	593	0.14%	0.029%
63	15.827	2182	2183	2186	rBV	535	652	0.15%	0.032%
64	15.945	2201	2203	2207	rBV	552	927	0.22%	0.046%
65	16.968	2371	2377	2393	rBV2	217347	413841	97.66%	20.494%
66	17.439	2455	2457	2461	rBV	614	770	0.18%	0.038%
67	17.545	2473	2475	2479	rBV	499	646	0.15%	0.032%
68	17.651	2486	2493	2495	rBV	527	846	0.20%	0.042%
69	17.703	2499	2502	2503	rBV	588	571	0.13%	0.028%
70	17.739	2504	2508	2509	rVB	746	802	0.19%	0.040%
71	17.751	2509	2510	2514	rBV	1219	960	0.23%	0.048%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022376.D
 Acq On : 27 Aug 2019 20:49
 Operator : HP/JU
 Sample : K4513-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	17.886	2529	2533	2535	rVB	968	1029	0.24%	0.051%
73	17.968	2545	2547	2549	rVB	743	691	0.16%	0.034%
74	18.003	2552	2553	2555	rBV	756	582	0.14%	0.029%
75	18.062	2561	2563	2564	rBV	1478	586	0.14%	0.029%
76	18.086	2564	2567	2570	rBV	710	904	0.21%	0.045%
77	18.221	2587	2590	2591	rBV	1021	713	0.17%	0.035%
78	18.239	2591	2593	2597	rVB	747	687	0.16%	0.034%
79	18.286	2597	2601	2602	rBV2	1294	1459	0.34%	0.072%
80	18.409	2620	2622	2623	rVB	1050	617	0.15%	0.031%
81	18.492	2635	2636	2637	rBV	1268	741	0.17%	0.037%
82	18.580	2650	2651	2652	rVB	1856	655	0.15%	0.032%
83	18.603	2652	2655	2656	rBV2	1098	873	0.21%	0.043%
84	18.662	2662	2665	2668	rBV2	1686	2557	0.60%	0.127%
85	18.733	2675	2677	2678	rBV	1510	938	0.22%	0.046%
86	18.768	2681	2683	2687	rVB2	1302	1248	0.29%	0.062%
87	18.809	2687	2690	2691	rBV3	1052	712	0.17%	0.035%
88	18.833	2691	2694	2698	rVV3	1013	1001	0.24%	0.050%
89	18.915	2706	2708	2709	rBV2	837	655	0.15%	0.032%
90	18.980	2716	2719	2721	rBV2	1397	1618	0.38%	0.080%
91	19.062	2732	2733	2734	rBV	1201	504	0.12%	0.025%
92	19.092	2736	2738	2740	rVV	1062	867	0.20%	0.043%
93	19.192	2751	2755	2756	rVB2	2300	2182	0.51%	0.108%
94	19.445	2797	2798	2801	rBV2	2186	2274	0.54%	0.113%
95	19.503	2806	2808	2811	rBV3	1684	2027	0.48%	0.100%
96	19.621	2826	2828	2831	rBV3	1576	1957	0.46%	0.097%
97	19.786	2854	2856	2860	rBV4	1735	2276	0.54%	0.113%
98	19.850	2865	2867	2868	rBV2	1574	846	0.20%	0.042%
99	21.180	3088	3093	3101	rBV	277885	423736	100.00%	20.984%
100	23.368	3460	3465	3478	rVB	192769	387344	91.41%	19.182%


Sum of corrected areas: 2019321

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
Data File : BM022376.D
Acq On : 27 Aug 2019 20:49
Operator : HP/JU
Sample : K4513-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

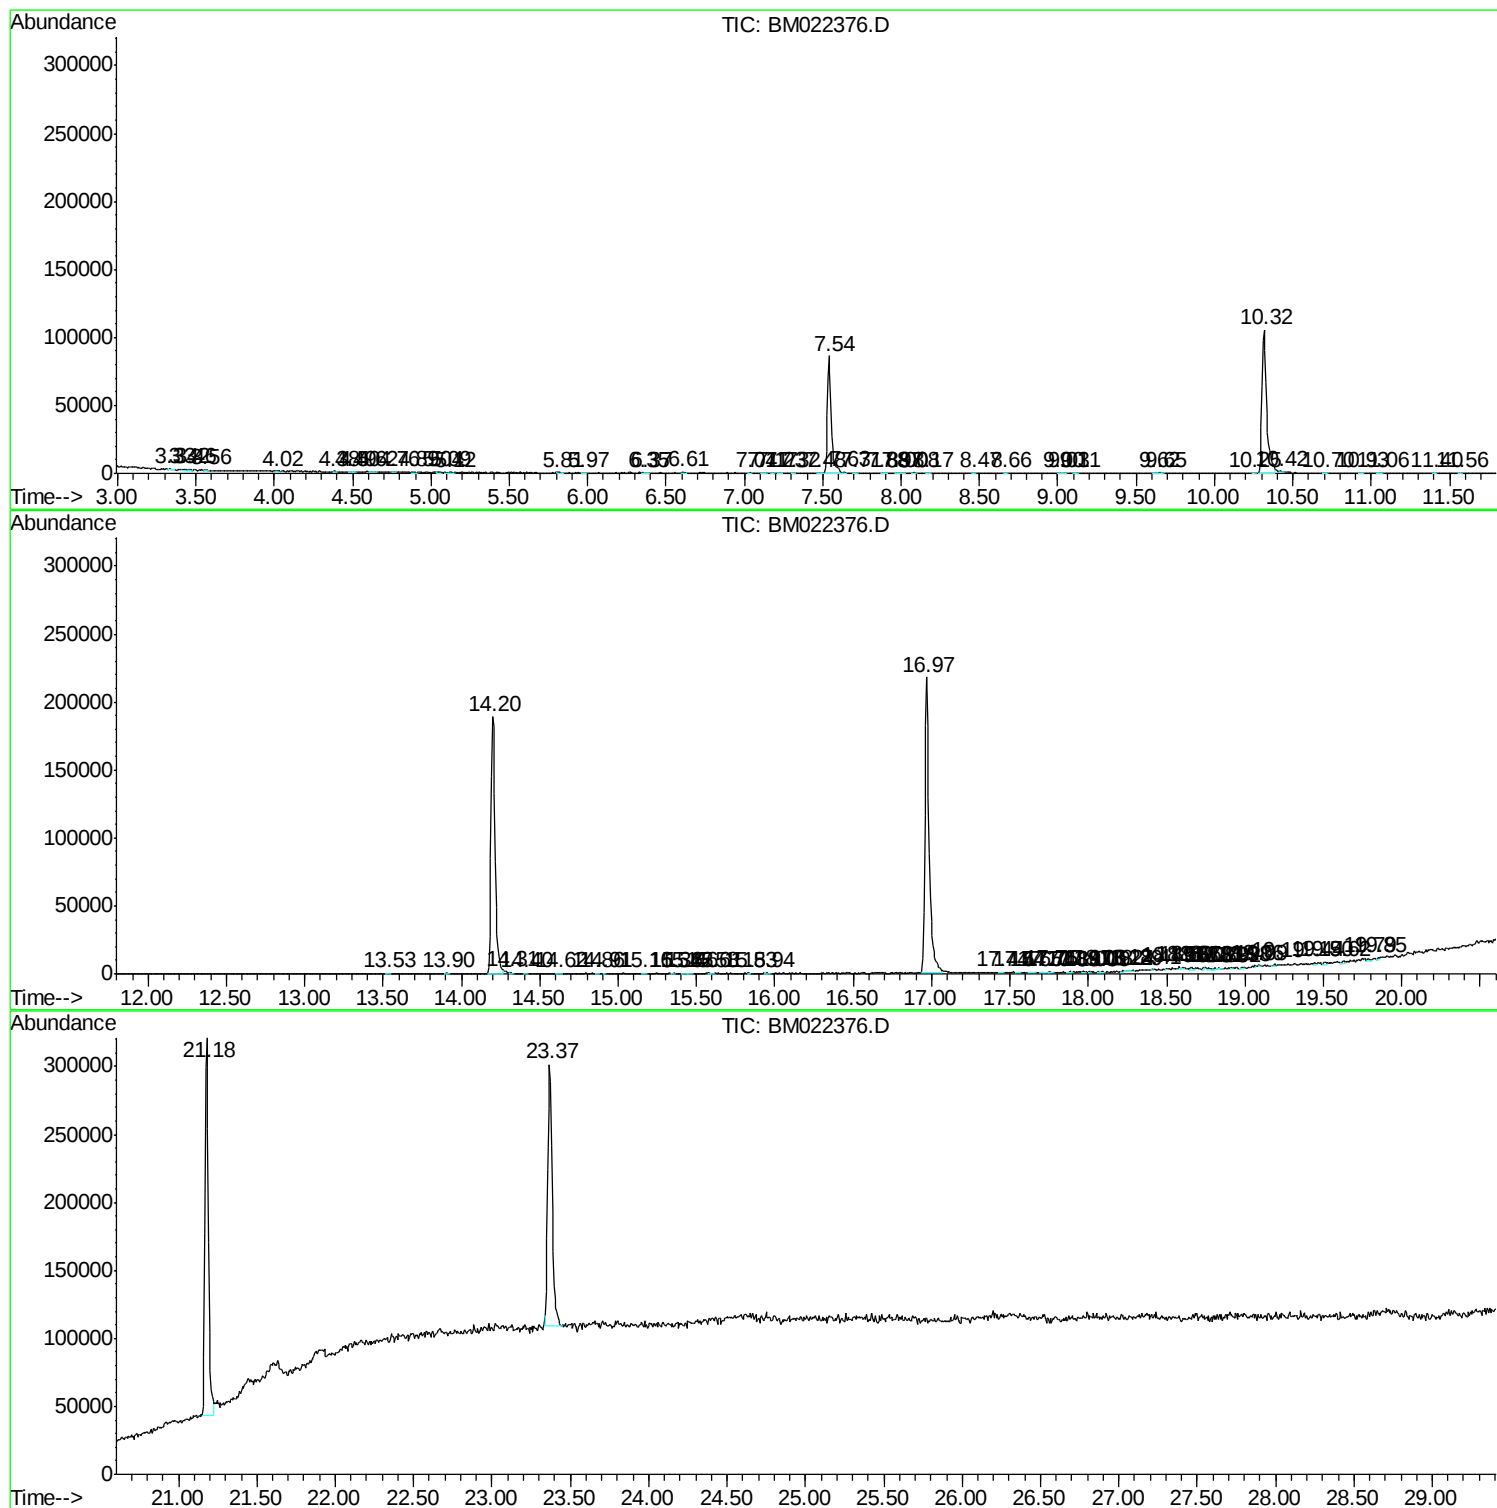

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022376.D
Acq On : 27 Aug 2019 20:49
Operator : HP/JU
Sample : K4513-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022376.D
Acq On : 27 Aug 2019 20:49
Operator : HP/JU
Sample : K4513-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
