

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022377.D
 Acq On : 27 Aug 2019 21:25
 Operator : HP/JU
 Sample : K4513-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	74	76	77	rVB2	1026	611	0.16%	0.033%
2	3.816	138	141	144	rBV3	1477	2013	0.52%	0.108%
3	4.016	174	175	179	rBV2	626	666	0.17%	0.036%
4	4.181	201	203	205	rBV2	639	693	0.18%	0.037%
5	4.257	214	216	217	rBV	882	536	0.14%	0.029%
6	4.457	247	250	252	rBV2	672	621	0.16%	0.033%
7	4.510	257	259	262	rVB	956	1130	0.29%	0.061%
8	4.616	273	277	278	rBV2	539	750	0.19%	0.040%
9	4.634	278	280	283	rVB	684	698	0.18%	0.037%
10	4.928	328	330	336	rVB	641	945	0.24%	0.051%
11	5.134	361	365	367	rBV	440	552	0.14%	0.030%
12	5.404	410	411	413	rBV	720	581	0.15%	0.031%
13	5.663	452	455	456	rVB	716	584	0.15%	0.031%
14	5.687	456	459	461	rBV	546	735	0.19%	0.039%
15	5.740	465	468	471	rVB	481	735	0.19%	0.039%
16	5.946	500	503	505	rBB	457	570	0.15%	0.031%
17	6.334	563	569	571	rVB	532	1090	0.28%	0.058%
18	6.357	571	573	575	rBV	689	676	0.17%	0.036%
19	6.463	589	591	594	rBV	756	792	0.20%	0.042%
20	6.587	610	612	614	rVB	895	601	0.15%	0.032%
21	6.616	614	617	619	rBB	738	688	0.18%	0.037%
22	6.646	619	622	625	rBV	470	797	0.20%	0.043%
23	6.746	636	639	641	rBV	484	714	0.18%	0.038%
24	7.063	690	693	697	rBB	434	633	0.16%	0.034%
25	7.540	769	774	788	rBV	83500	151802	38.84%	8.141%
26	8.151	875	878	881	rBB	550	690	0.18%	0.037%
27	9.116	1040	1042	1045	rBB	439	566	0.14%	0.030%
28	10.316	1240	1246	1266	rBV	103838	220094	56.32%	11.803%
29	11.886	1512	1513	1518	rBB	375	596	0.15%	0.032%
30	14.063	1880	1883	1886	rBB	443	537	0.14%	0.029%
31	14.198	1900	1906	1923	rBV2	184697	334678	85.64%	17.948%
32	14.610	1972	1976	1978	rBB	515	566	0.14%	0.030%
33	14.845	2015	2016	2020	rBV	403	601	0.15%	0.032%
34	15.145	2065	2067	2069	rBV	437	536	0.14%	0.029%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
 Data File : BM022377.D
 Acq On : 27 Aug 2019 21:25
 Operator : HP/JU
 Sample : K4513-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	15.274	2087	2089	2091	rBV	474	542	0.14%	0.029%
36	15.321	2096	2097	2100	rBV	495	598	0.15%	0.032%
37	15.669	2153	2156	2159	rBV	490	854	0.22%	0.046%
38	15.727	2164	2166	2169	rVB	508	588	0.15%	0.032%
39	15.774	2170	2174	2175	rBV	542	755	0.19%	0.040%
40	15.910	2194	2197	2199	rBV	551	700	0.18%	0.038%
41	16.074	2221	2225	2227	rVB	615	923	0.24%	0.049%
42	16.157	2236	2239	2241	rBV	729	915	0.23%	0.049%
43	16.968	2371	2377	2394	rBV	206572	390817	100.00%	20.959%
44	17.445	2455	2458	2460	rVB	749	796	0.20%	0.043%
45	17.798	2516	2518	2520	rBV	952	692	0.18%	0.037%
46	18.098	2567	2569	2570	rBV	1297	813	0.21%	0.044%
47	18.215	2587	2589	2593	rVB	720	857	0.22%	0.046%
48	18.286	2598	2601	2603	rVV	703	736	0.19%	0.039%
49	18.333	2606	2609	2610	rBV	905	916	0.23%	0.049%
50	18.398	2617	2620	2621	rVB	1088	813	0.21%	0.044%
51	18.421	2621	2624	2627	rBV2	1178	1252	0.32%	0.067%
52	18.468	2631	2632	2634	rBV2	2187	1598	0.41%	0.086%
53	18.645	2660	2662	2663	rVB2	1280	860	0.22%	0.046%
54	18.662	2663	2665	2667	rBV	1502	1311	0.34%	0.070%
55	18.680	2667	2668	2671	rVV2	1163	1141	0.29%	0.061%
56	18.727	2674	2676	2678	rVV	1126	1028	0.26%	0.055%
57	18.833	2692	2694	2696	rVB2	1231	780	0.20%	0.042%
58	18.857	2696	2698	2699	rBV	1156	870	0.22%	0.047%
59	18.939	2710	2712	2713	rBV2	1174	574	0.15%	0.031%
60	21.180	3088	3093	3101	rBV2	236168	382775	97.94%	20.527%
61	23.368	3460	3465	3475	rVB	174283	341128	87.29%	18.294%


Sum of corrected areas: 1864709

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082619\
Data File : BM022377.D
Acq On : 27 Aug 2019 21:25
Operator : HP/JU
Sample : K4513-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

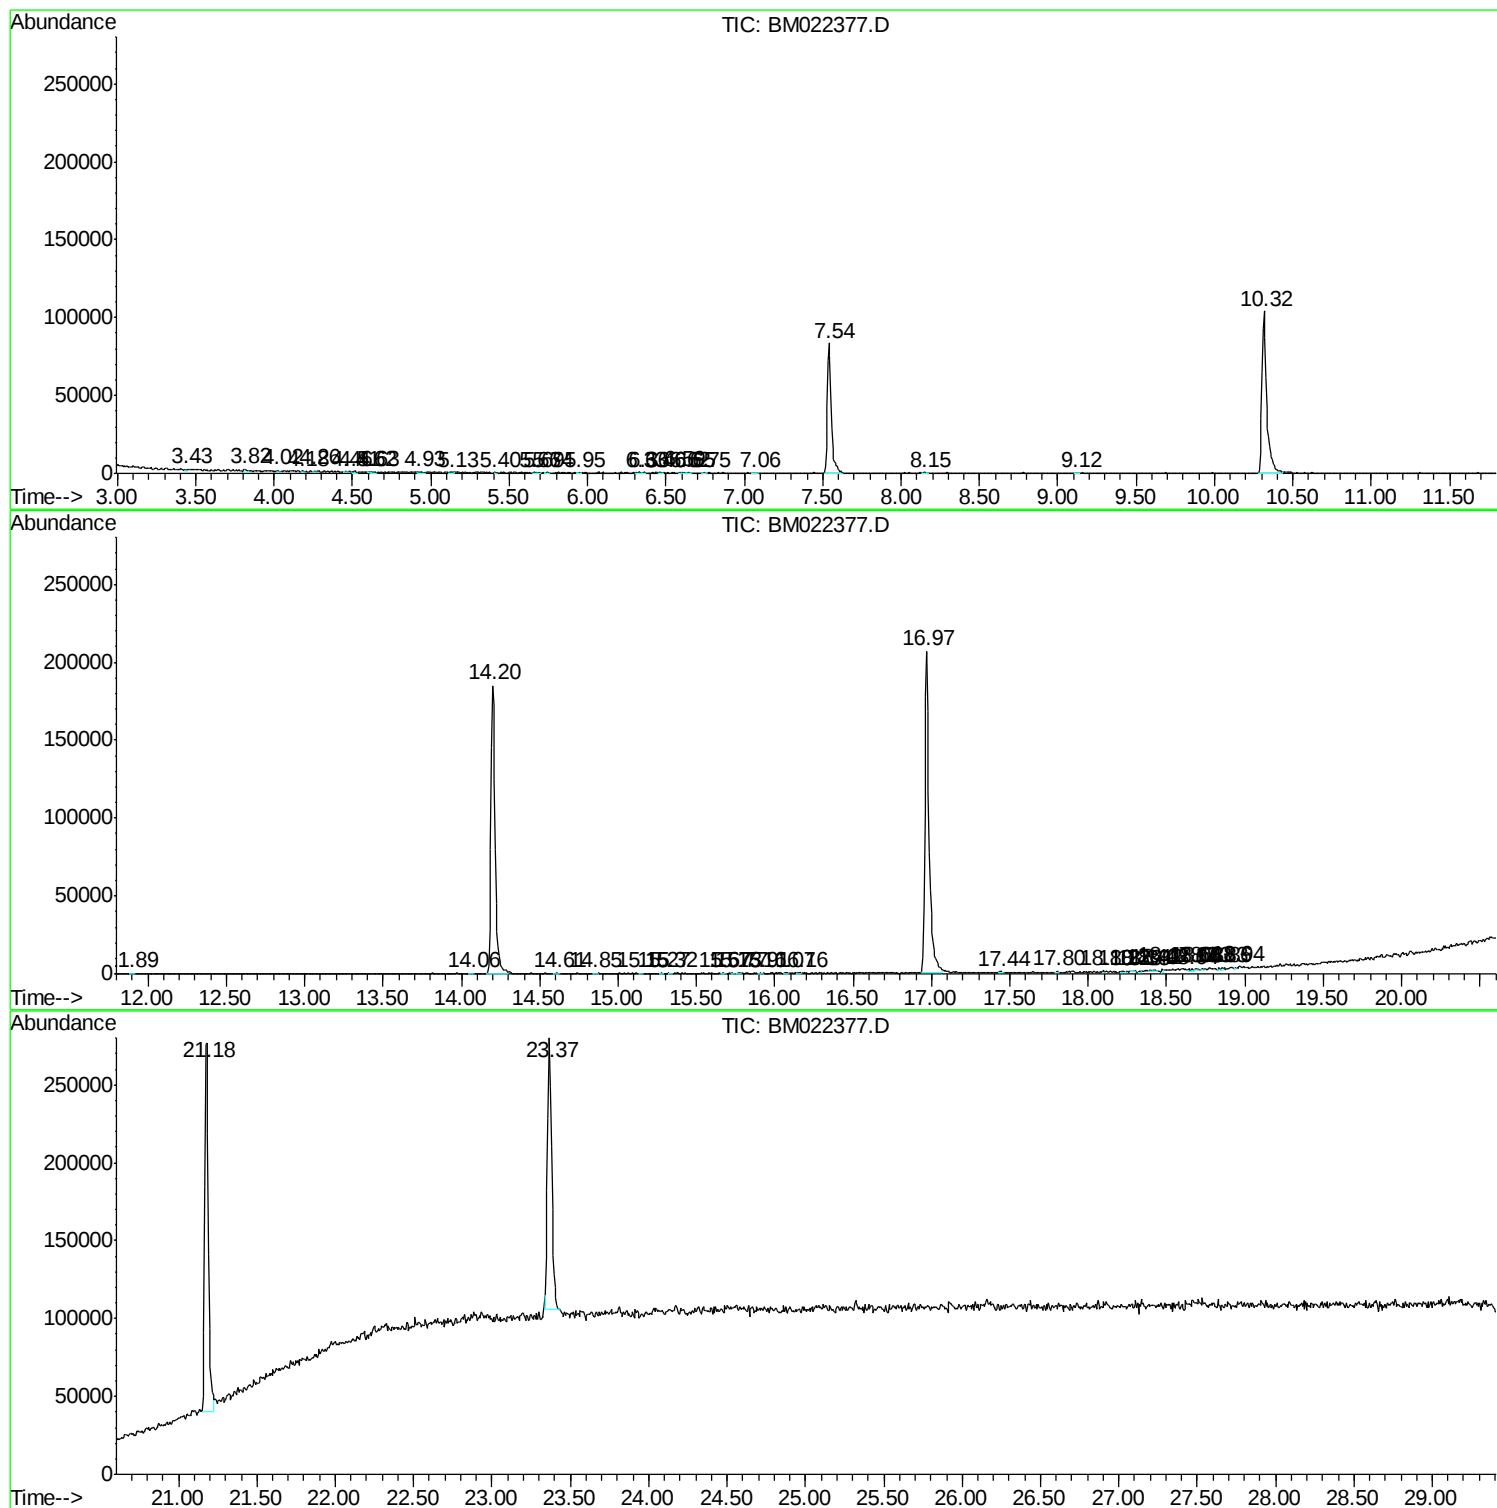

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022377.D
Acq On : 27 Aug 2019 21:25
Operator : HP/JU
Sample : K4513-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082619\
Data File : BM022377.D
Acq On : 27 Aug 2019 21:25
Operator : HP/JU
Sample : K4513-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
