
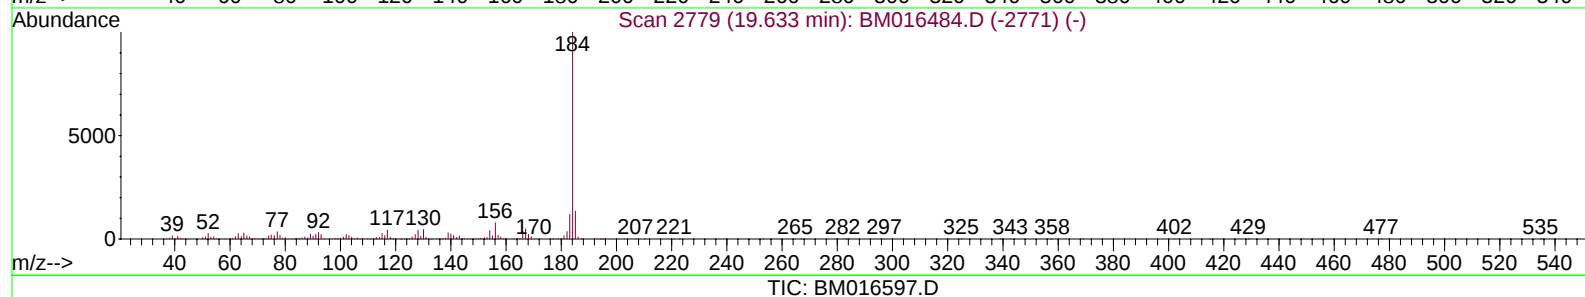
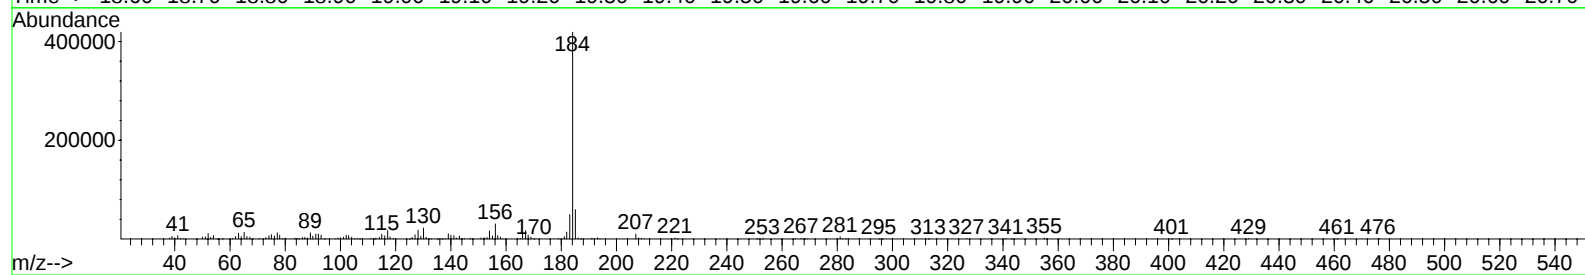


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082718\
Data File : BM016597.D
Acq On : 27 Aug 2018 09:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 16:08:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

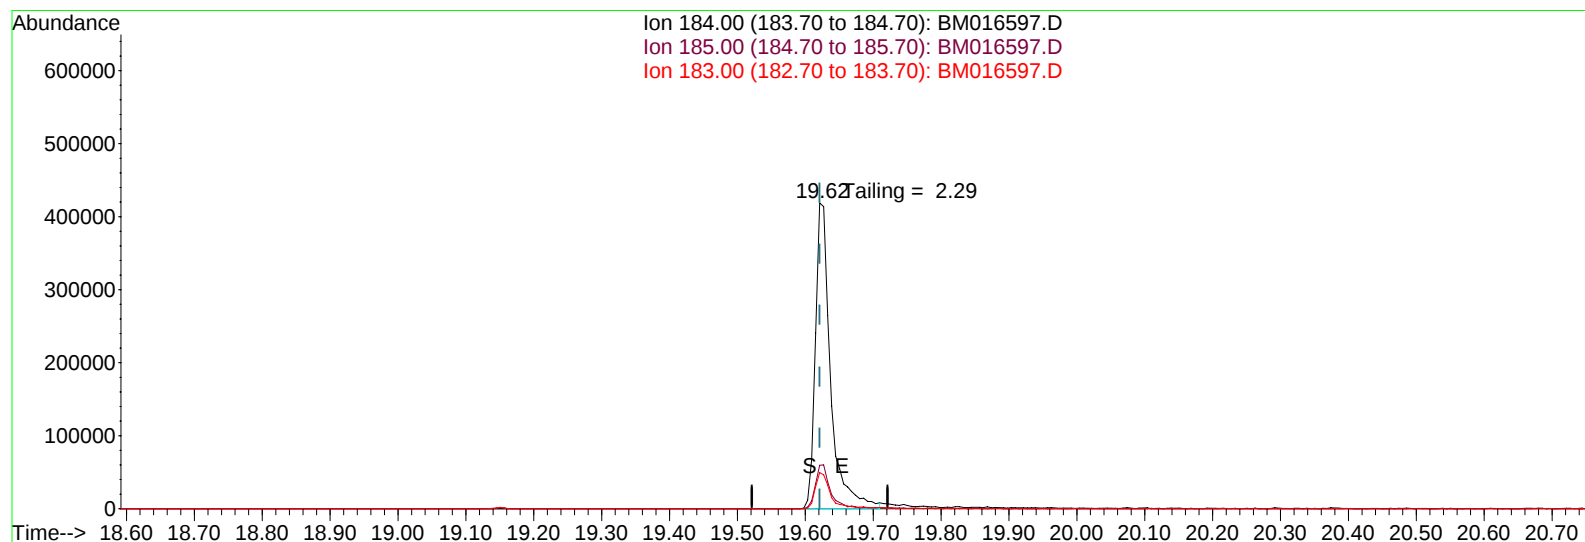

(76) Benzidine




19.621min (0.000) 183970.08ng

response 668671

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.25
183.00	11.10	11.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082718\
Data File : BM016597.D
Acq On : 27 Aug 2018 09:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 16:08:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

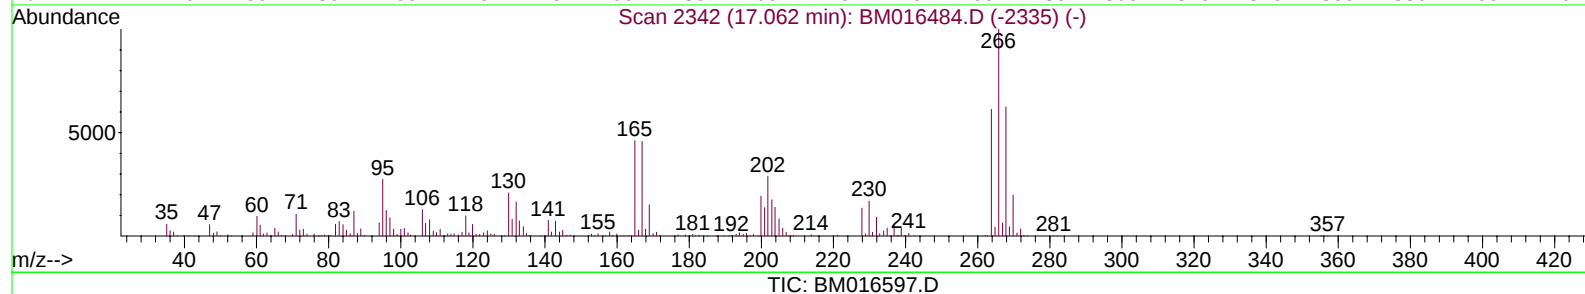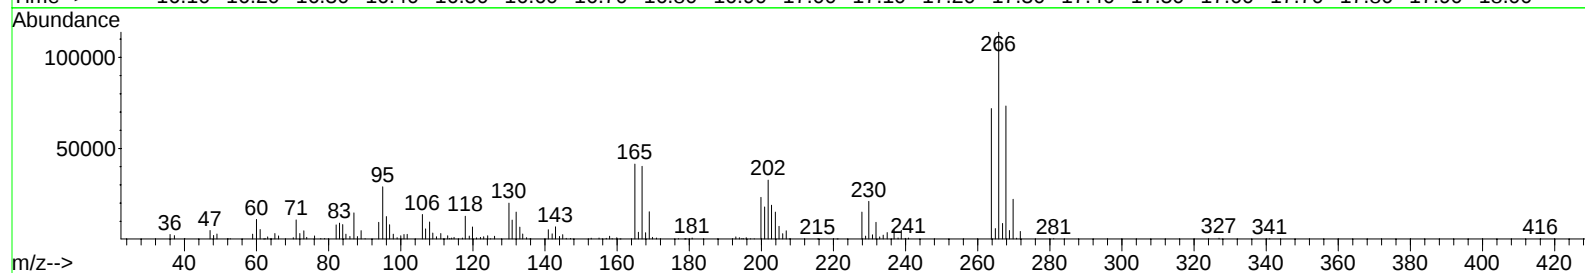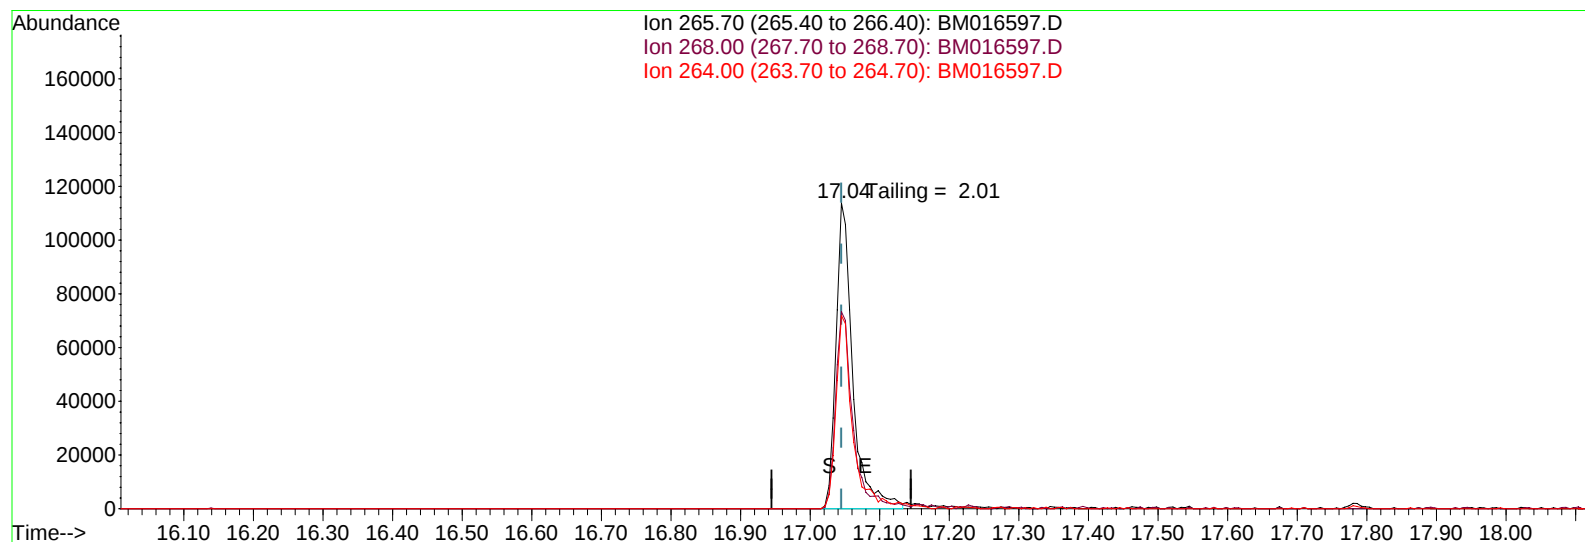

(69) Pentachlorophenol (C)

17.045min (0.000) 0.00ng

response 188154

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.42
264.00	61.20	63.18
0.00	0.00	0.00