
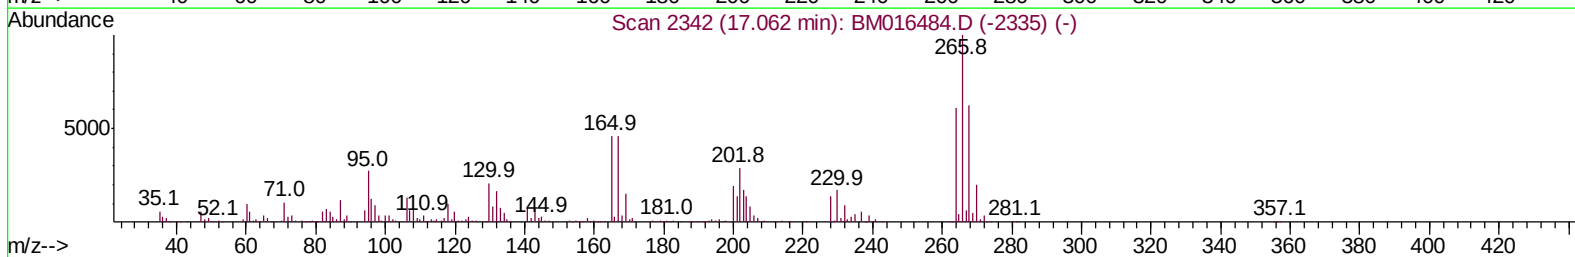
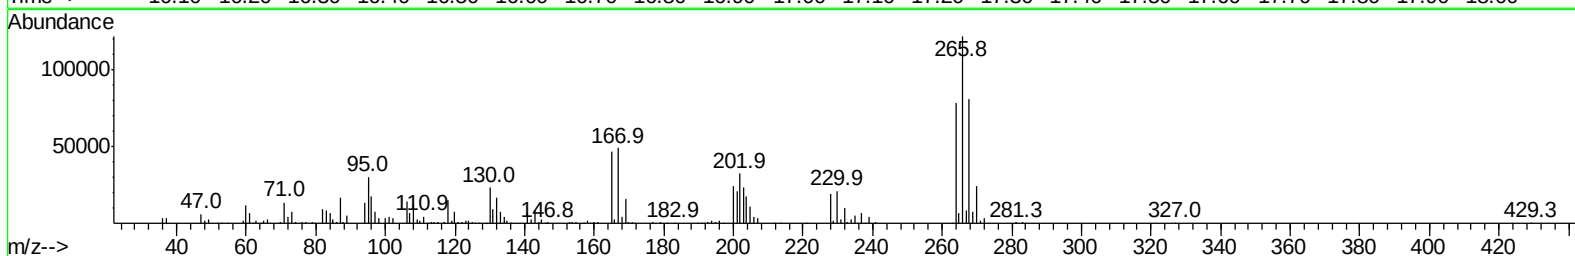


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016617.D
Acq On : 27 Aug 2018 22:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:42:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

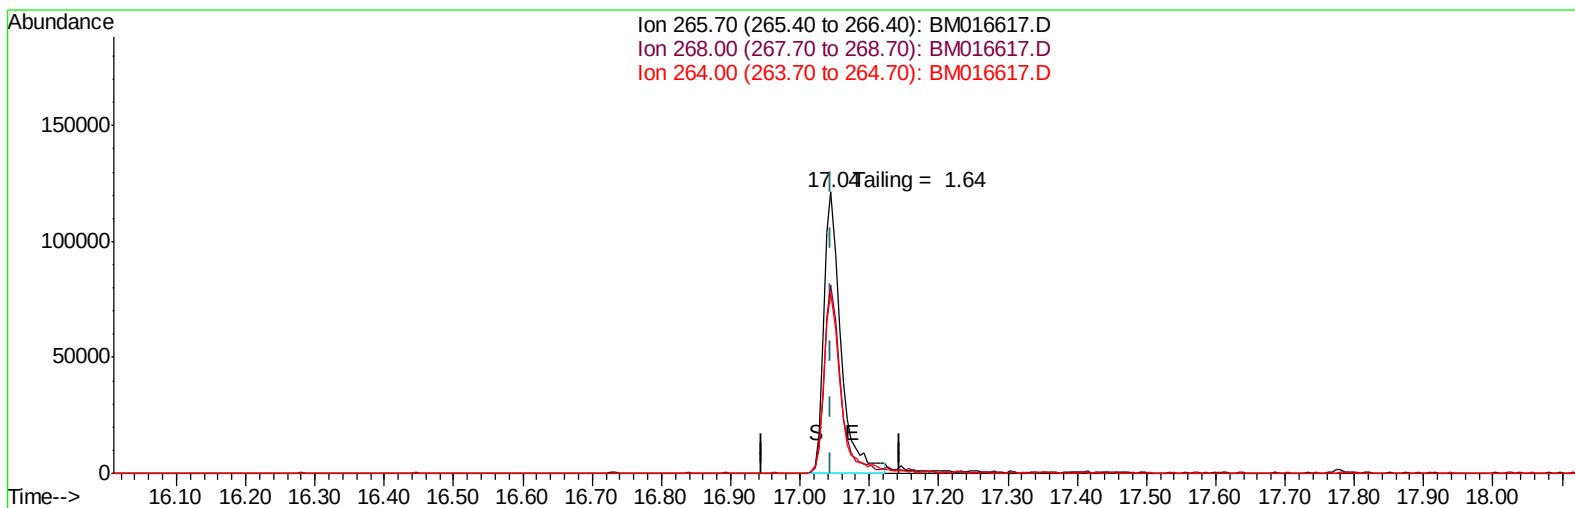

TIC: BM016617.D

(69) Pentachlorophenol (C)




17.045min (-0.000) 0.00ng

response 207186

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	66.80
264.00	61.20	64.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016617.D
Acq On : 27 Aug 2018 22:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:42:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

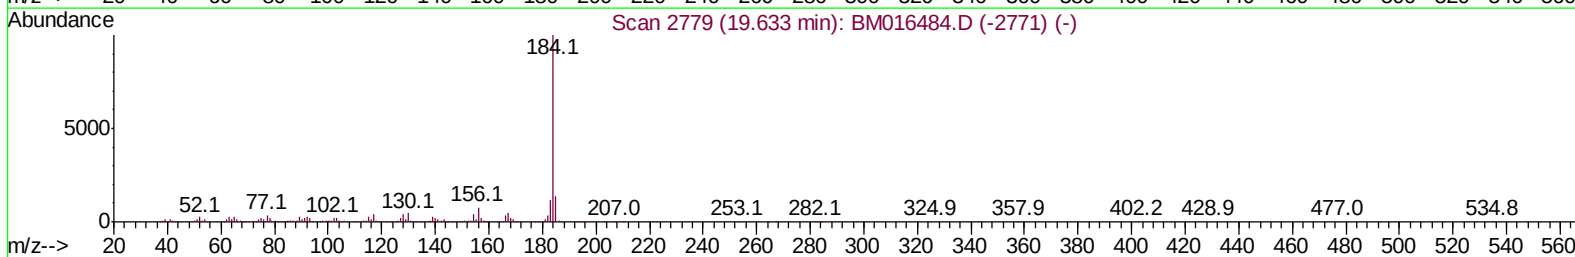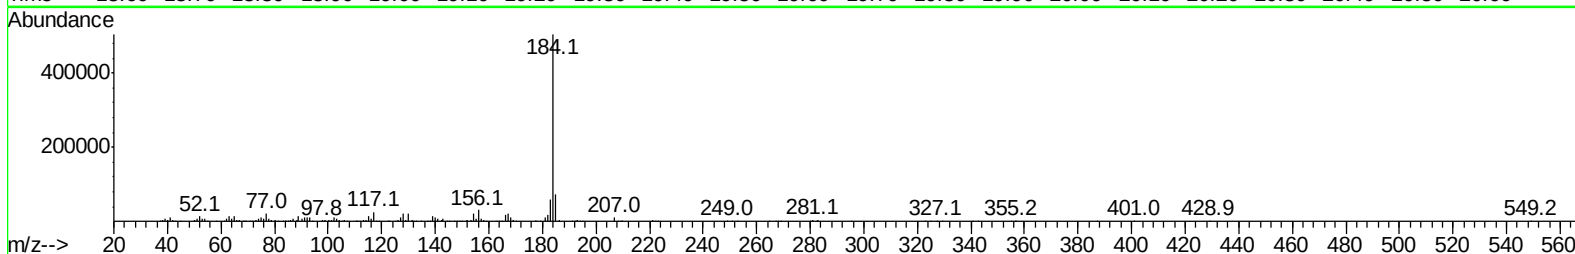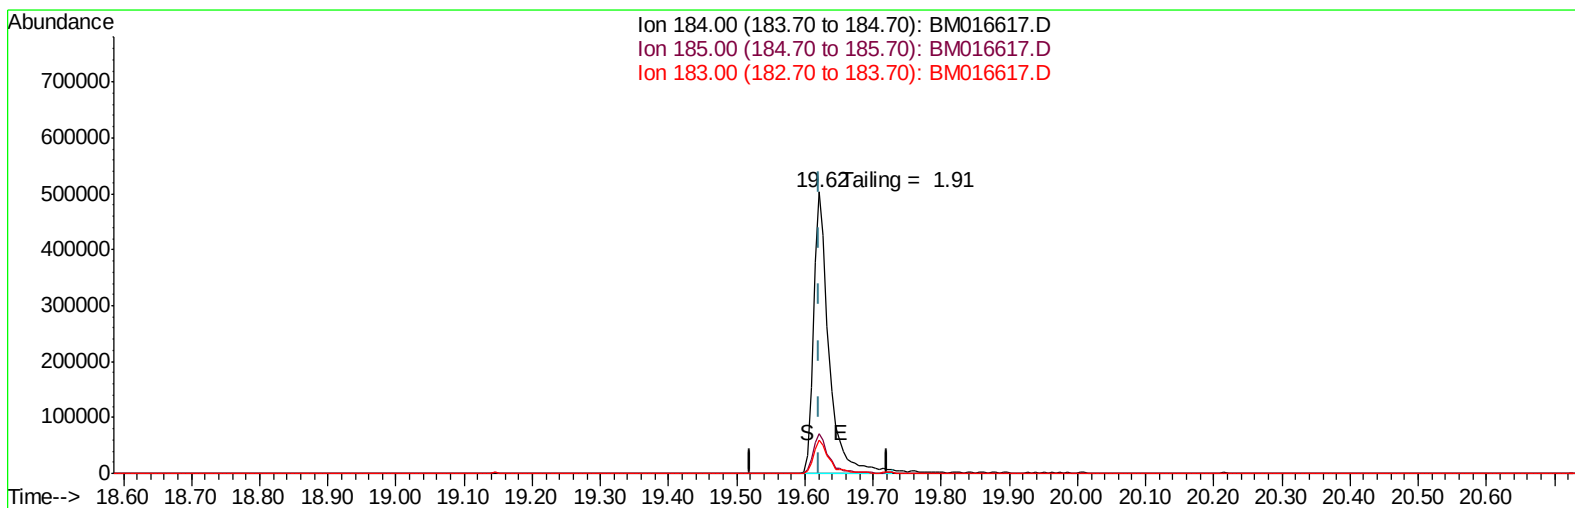

TIC: BM016617.D

(76) Benzidine

19.621min (-0.000) 58167.37ng

response 790865

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.13
183.00	11.10	11.83
0.00	0.00	0.00