

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
 Data File : BM016612.D
 Acq On : 27 Aug 2018 18:28
 Operator : SJ/JU
 Sample : J4618-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FM1026

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.552	380	385	400	rBV	521894	957136	5.58%	1.811%
2	7.187	658	663	681	rBV	307465	613843	3.58%	1.162%
3	7.534	715	722	738	rBV	1345810	2408428	14.04%	4.558%
4	8.005	796	802	814	rBV	477524	859384	5.01%	1.626%
5	8.322	849	856	871	rBV	1448410	2502634	14.59%	4.736%
6	9.193	996	1004	1021	rBV	865477	1613360	9.41%	3.053%
7	10.810	1270	1279	1295	rBV	574006	1043575	6.08%	1.975%
8	13.263	1688	1696	1713	rBV	3903851	5601678	32.66%	10.601%
9	14.645	1925	1931	1940	rBV2	1017950	1609497	9.38%	3.046%
10	16.139	2179	2185	2196	rBV	5248678	7226165	42.13%	13.676%
11	17.386	2392	2397	2407	rVB	1905384	2676802	15.61%	5.066%
12	19.980	2832	2838	2848	rBV	15089258	17151439	100.00%	32.460%
13	21.533	3097	3102	3109	rBV	3504136	4494155	26.20%	8.505%
14	23.809	3484	3489	3497	rVB	2087733	4081225	23.80%	7.724%


Sum of corrected areas: 52839321

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016612.D
Acq On : 27 Aug 2018 18:28
Operator : SJ/JU
Sample : J4618-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FM1026

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

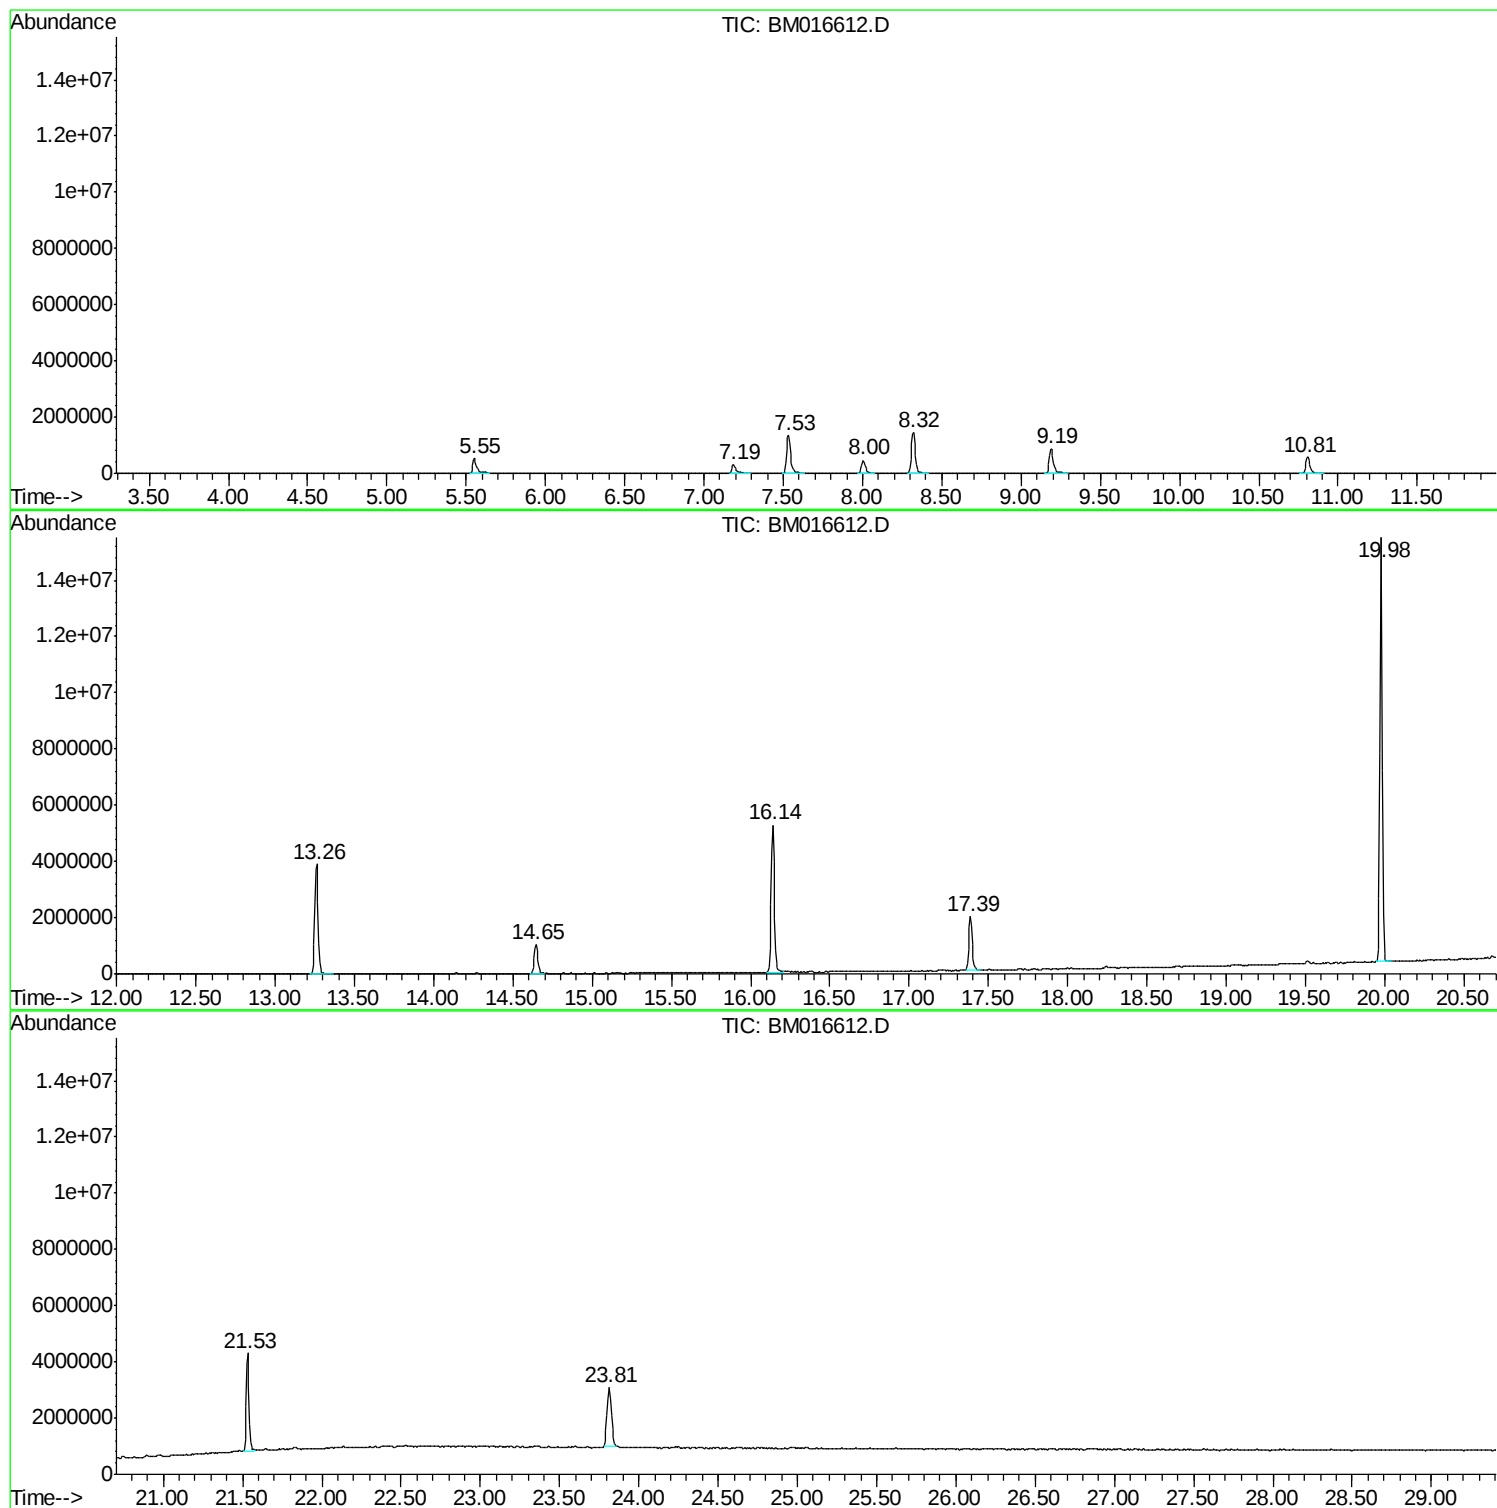

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016612.D
Acq On : 27 Aug 2018 18:28
Operator : SJ/JU
Sample : J4618-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FM1026










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	56.05 ng	2408430	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	22
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
4		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	11
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	10

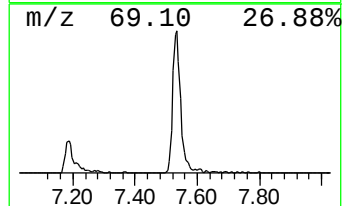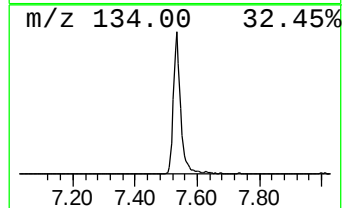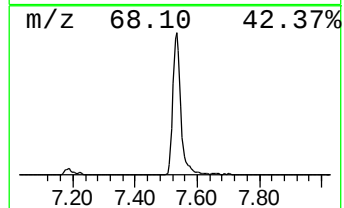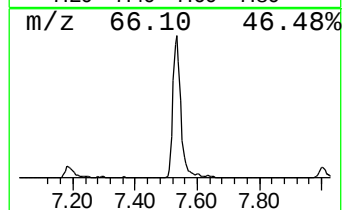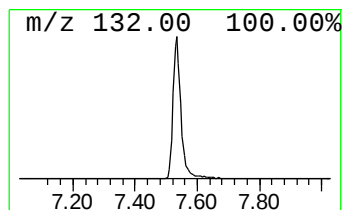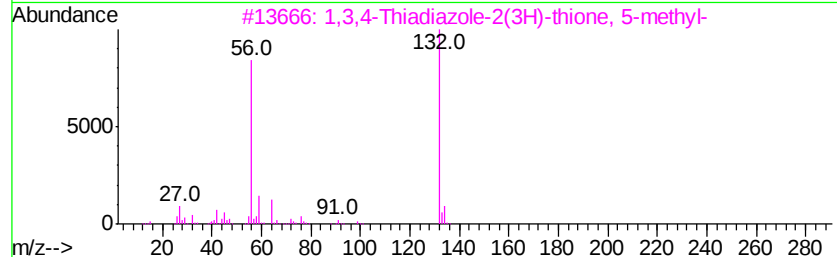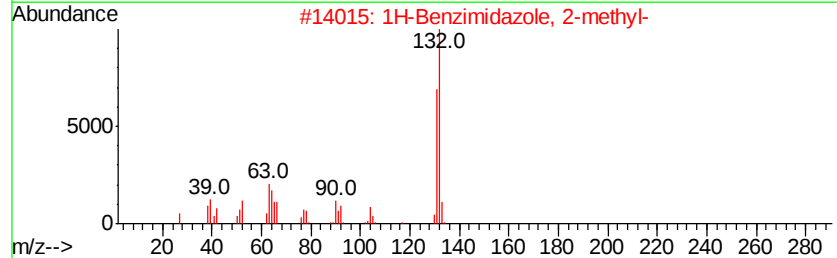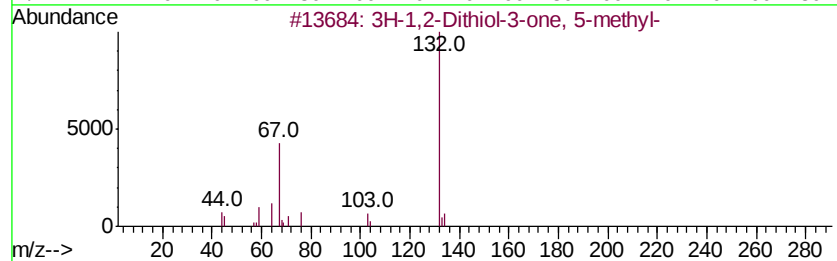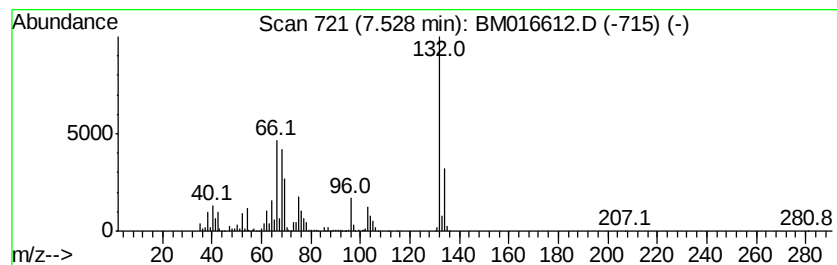

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082718\
Data File : BM016612.D
Acq On : 27 Aug 2018 18:28
Operator : SJ/JU
Sample : J4618-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FM1026

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	56.0	ng	2408430	1	8.00	859384	20.0