

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
 Data File : BM016620.D
 Acq On : 28 Aug 2018 00:28
 Operator : SJ/JU
 Sample : J4660-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 082318-DBRI-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.552	380	385	400	rBV	390643	743640	4.26%	1.567%
2	7.187	658	663	679	rBV	223840	473609	2.71%	0.998%
3	7.528	716	721	738	rBV	1111703	1914200	10.95%	4.032%
4	8.004	796	802	814	rBV2	336595	620153	3.55%	1.306%
5	8.316	848	855	872	rBV	2222334	3496619	20.01%	7.366%
6	9.187	997	1003	1022	rBV	1199751	2126182	12.17%	4.479%
7	10.810	1273	1279	1295	rBV	358635	685481	3.92%	1.444%
8	13.257	1689	1695	1713	rBV	5427292	7534848	43.12%	15.873%
9	14.645	1920	1931	1942	rBV2	624760	1039740	5.95%	2.190%
10	16.139	2178	2185	2207	rBV	3338704	4901012	28.05%	10.324%
11	17.386	2391	2397	2415	rBV	1019006	1555155	8.90%	3.276%
12	19.974	2832	2837	2845	rBV	15420237	17473512	100.00%	36.809%
13	21.203	3043	3046	3052	rBV8	90617	175038	1.00%	0.369%
14	21.533	3097	3102	3111	rBV	1715085	2379963	13.62%	5.014%
15	23.809	3484	3489	3500	rVB	1248168	2351463	13.46%	4.954%


Sum of corrected areas: 47470615

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016620.D
Acq On : 28 Aug 2018 00:28
Operator : SJ/JU
Sample : J4660-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

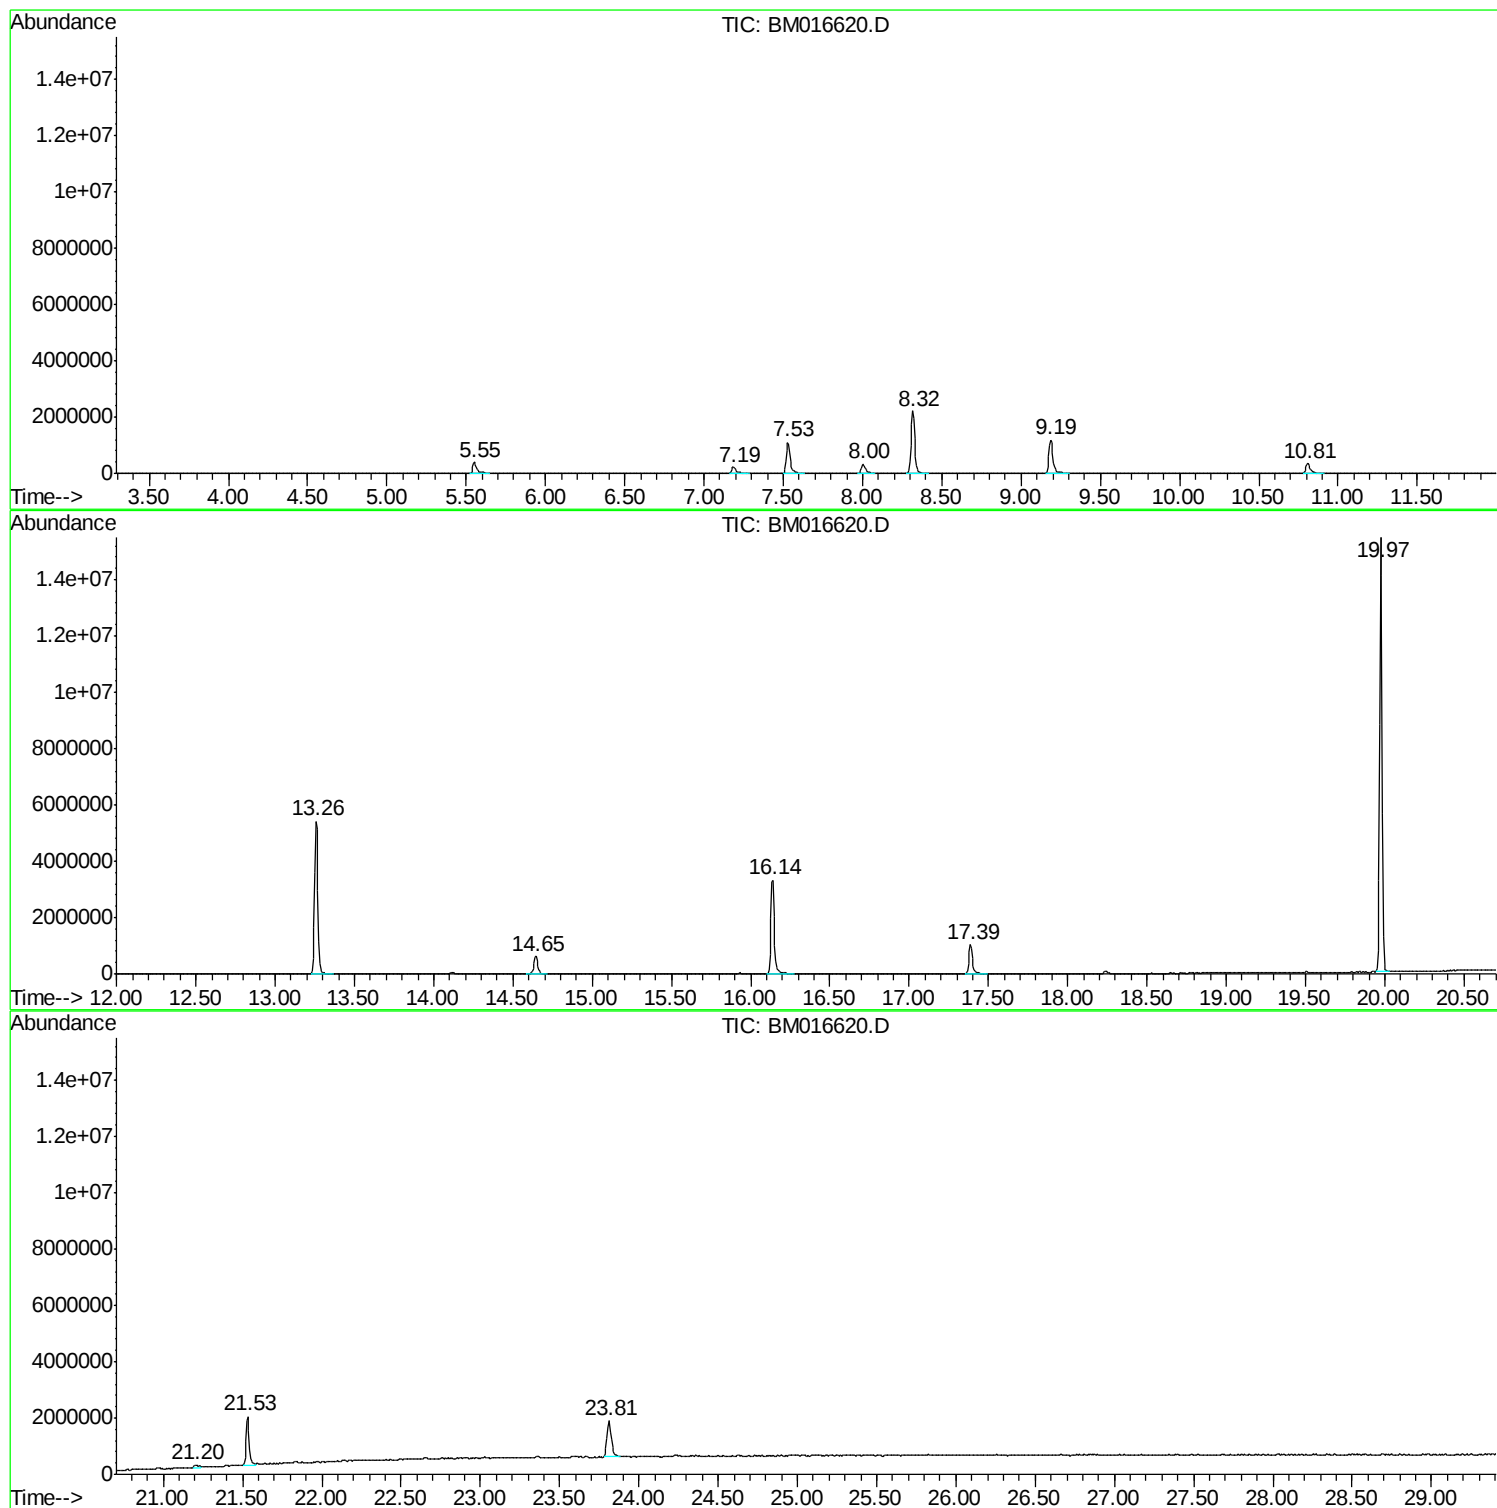

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016620.D
Acq On : 28 Aug 2018 00:28
Operator : SJ/JU
Sample : J4660-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-D-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	61.73 ng	1914200	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1-Penten-3-yne	66	C5H6	000646-05-9	27
2		3-Penten-1-yne, (Z)-	66	C5H6	001574-40-9	16
3		1,4,4a,8a-Tetrahydro-1,4-methano...	174	C11H10O2	001200-89-1	16
4		Bicyclo[2.2.1]hept-5-ene-2-aceti...	180	C11H16O2	074876-17-8	16
5		3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	12

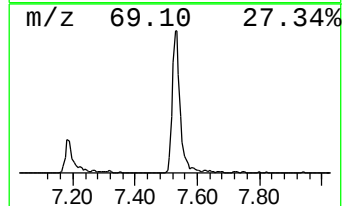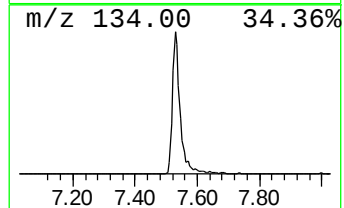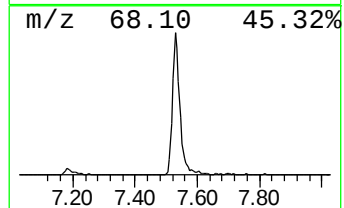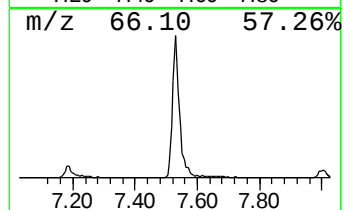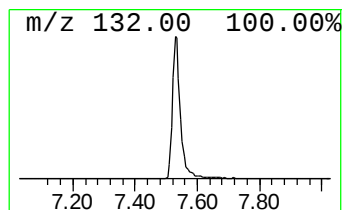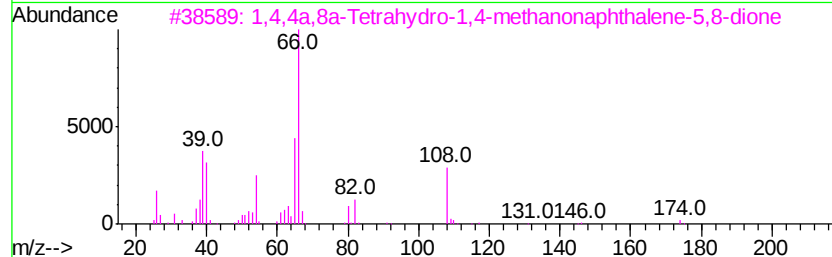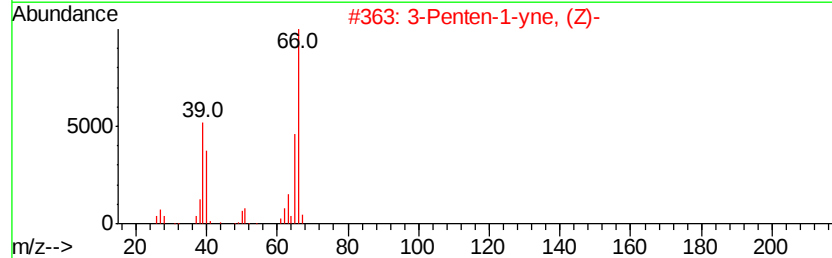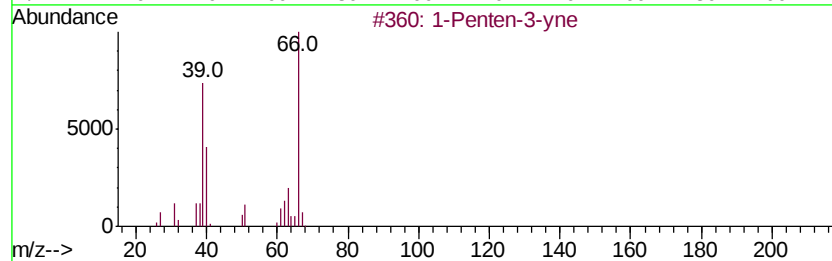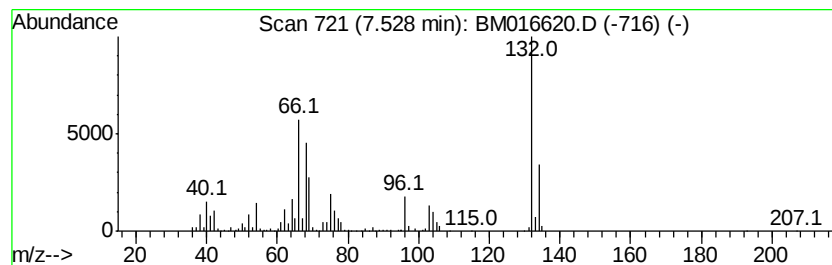

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082718\
Data File : BM016620.D
Acq On : 28 Aug 2018 00:28
Operator : SJ/JU
Sample : J4660-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	61.7	ng	1914200	1	8.00	620153	20.0