

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
 Data File : BM016622.D
 Acq On : 28 Aug 2018 01:40
 Operator : SJ/JU
 Sample : J4660-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 082318-DBRI-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	380	384	399	rBV	425388	822036	4.81%	1.722%
2	7.181	658	662	678	rBV	273127	550595	3.22%	1.153%
3	7.528	716	721	738	rBV	1155053	1974603	11.56%	4.136%
4	8.005	796	802	816	rBV2	341076	635508	3.72%	1.331%
5	8.316	849	855	873	rBV	2036376	3284023	19.22%	6.879%
6	9.187	997	1003	1019	rBV	1156051	2021533	11.83%	4.235%
7	10.810	1273	1279	1299	rBV	352956	707964	4.14%	1.483%
8	13.257	1686	1695	1712	rBV	5287718	7204287	42.16%	15.092%
9	14.110	1835	1840	1851	rBV	120292	208510	1.22%	0.437%
10	14.639	1920	1930	1943	rBV2	657594	1106540	6.48%	2.318%
11	16.133	2178	2184	2200	rBV	3422256	5145753	30.11%	10.779%
12	17.386	2391	2397	2410	rBV	1106724	1659423	9.71%	3.476%
13	19.974	2832	2837	2846	rBV	15683850	17088696	100.00%	35.797%
14	21.527	3097	3101	3111	rBV	1878839	2651550	15.52%	5.554%
15	23.809	3483	3489	3500	rBV	1310769	2676352	15.66%	5.606%


Sum of corrected areas: 47737373

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016622.D
Acq On : 28 Aug 2018 01:40
Operator : SJ/JU
Sample : J4660-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

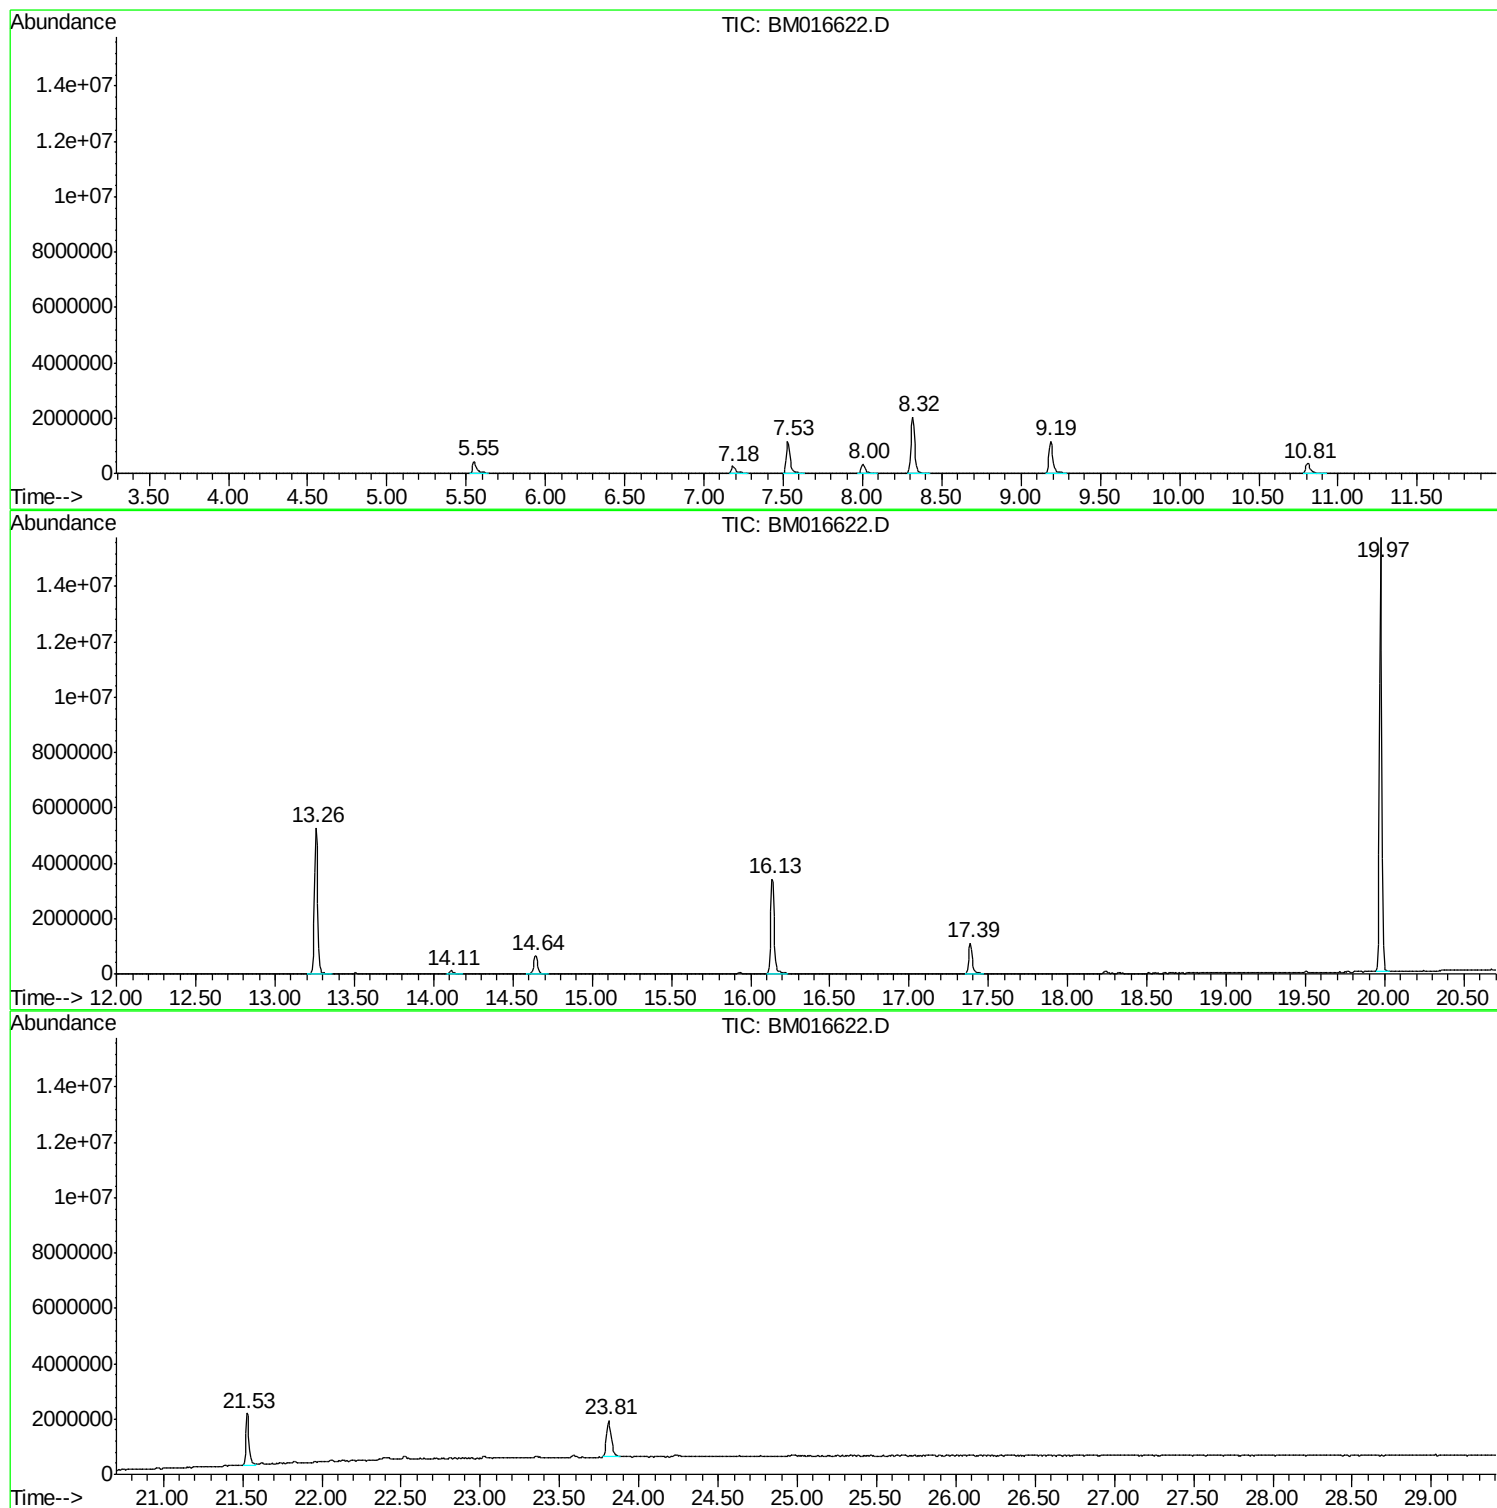

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016622.D
Acq On : 28 Aug 2018 01:40
Operator : SJ/JU
Sample : J4660-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-U-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	62.14 ng	1974600	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	The first isomer tricvclopentadiene	198	C15H18	1000222-21-0	47
2		3-Hexenedinitrile	106	C6H6N2	001119-85-3	27
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	22
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	18
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	18

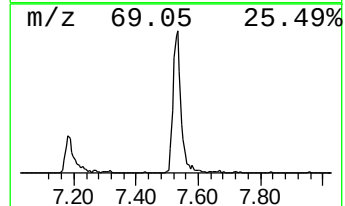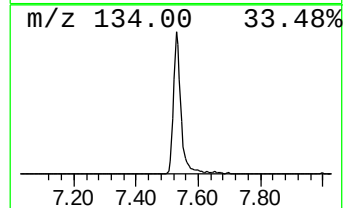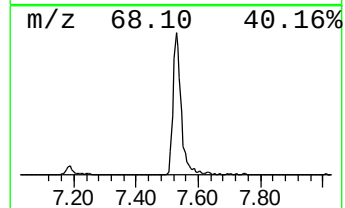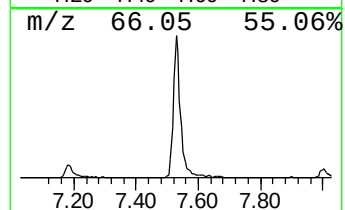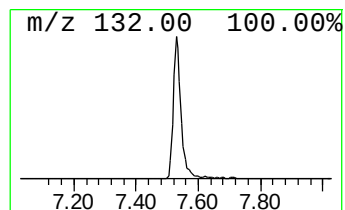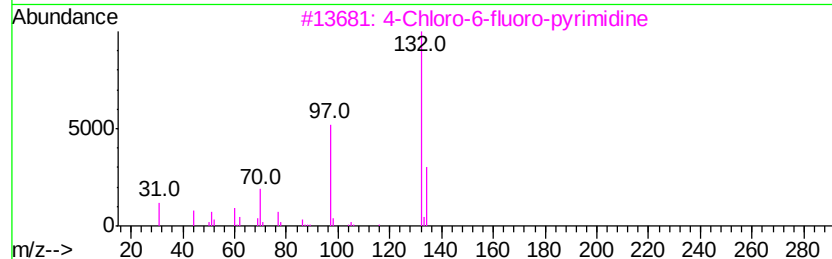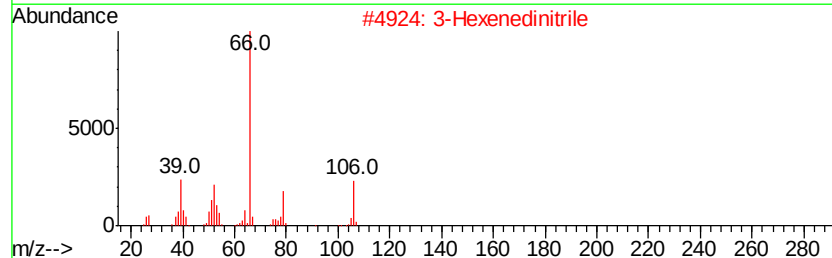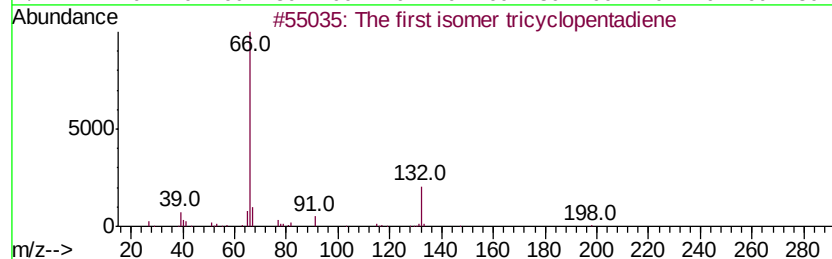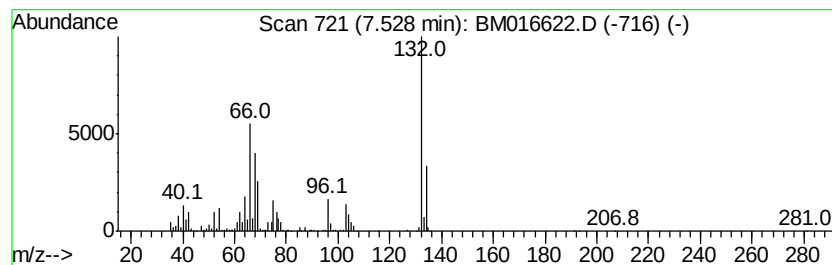

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082718\
Data File : BM016622.D
Acq On : 28 Aug 2018 01:40
Operator : SJ/JU
Sample : J4660-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.53	7.53	62.1	ng	1974600	1	8.00	635508	20.0