

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
 Data File : BM016623.D
 Acq On : 28 Aug 2018 02:16
 Operator : SJ/JU
 Sample : J4660-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 082318-DBRI-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	380	384	402	rBV	429531	844483	4.42%	1.680%
2	7.181	658	662	673	rBV	266034	507239	2.66%	1.009%
3	7.528	715	721	739	rBV	1117395	2013659	10.55%	4.005%
4	8.004	796	802	817	rBV	334620	621373	3.26%	1.236%
5	8.316	849	855	870	rBV	2066816	3374475	17.68%	6.711%
6	9.186	997	1003	1020	rBV	1210611	2105470	11.03%	4.188%
7	10.810	1272	1279	1290	rBV	369847	685416	3.59%	1.363%
8	13.257	1689	1695	1715	rBV	5487576	7453685	39.05%	14.825%
9	14.645	1923	1931	1943	rBV2	637243	1053991	5.52%	2.096%
10	16.139	2179	2185	2203	rBV	3651206	5324189	27.90%	10.589%
11	17.386	2390	2397	2412	rBV2	983783	1578087	8.27%	3.139%
12	19.974	2832	2837	2849	rBV	17109646	19085599	100.00%	37.959%
13	21.197	3042	3045	3053	rBV8	84937	195368	1.02%	0.389%
14	21.527	3097	3101	3110	rBV	1872245	2562512	13.43%	5.097%
15	23.809	3483	3489	3504	rBV	1355604	2873740	15.06%	5.716%


Sum of corrected areas: 50279286

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016623.D
Acq On : 28 Aug 2018 02:16
Operator : SJ/JU
Sample : J4660-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

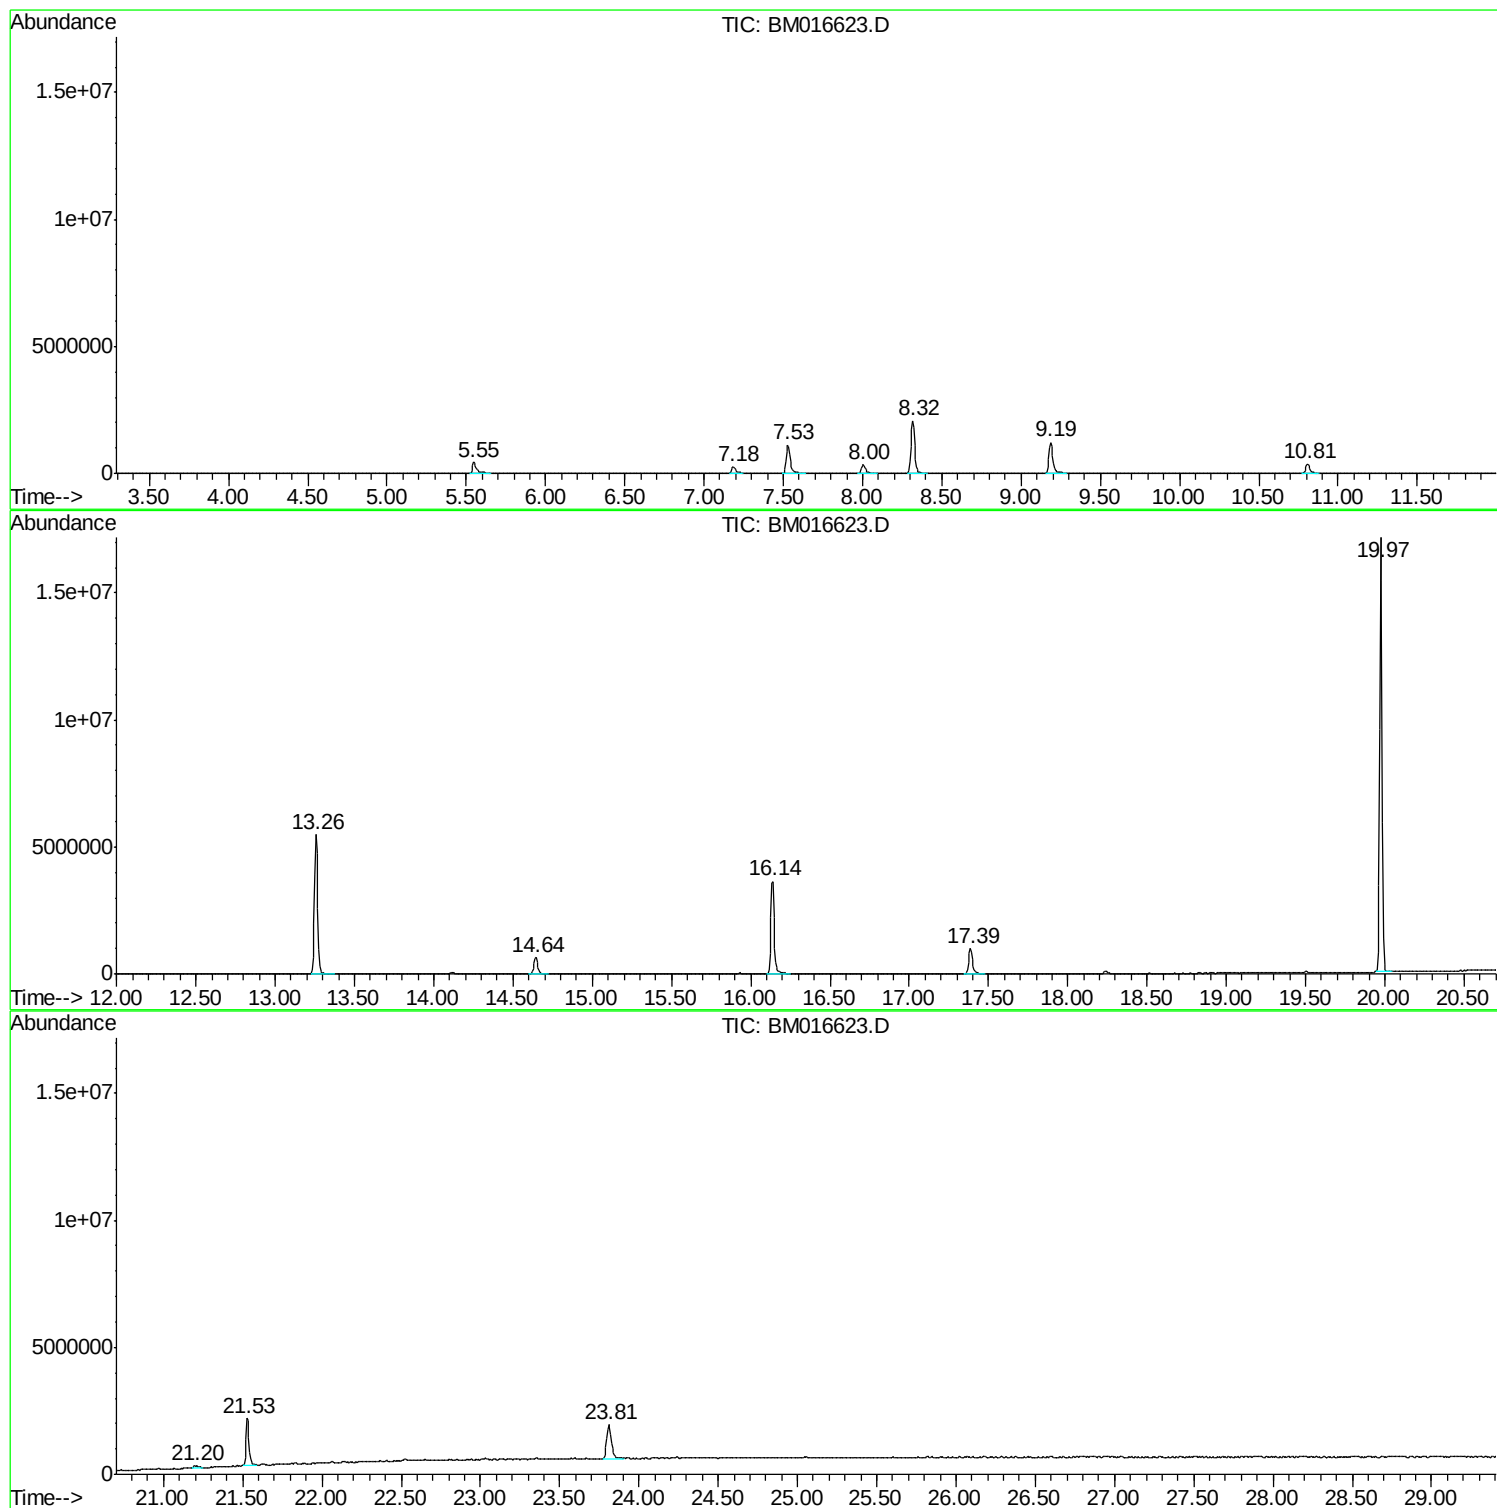

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016623.D
Acq On : 28 Aug 2018 02:16
Operator : SJ/JU
Sample : J4660-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-U-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	64.81 ng	2013660	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	endo-4-Oxatricyclo[5.2.1.0(2,6)]...	136	C9H12O	001528-23-0	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	22
3		1,3-Cyclopentadiene	66	C5H6	000542-92-7	16
4		3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	12
5		3-Penten-1-yne, (Z)-	66	C5H6	001574-40-9	12

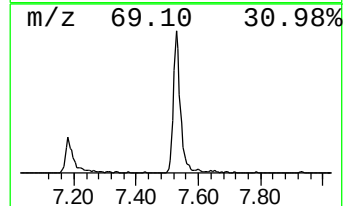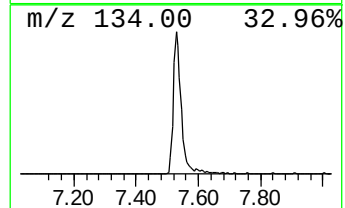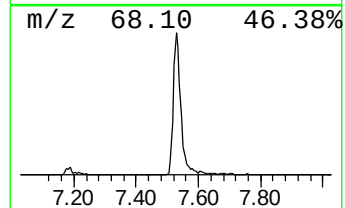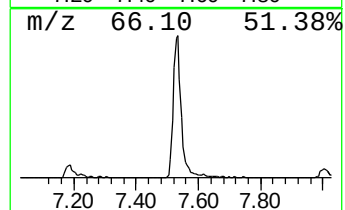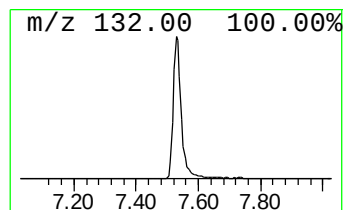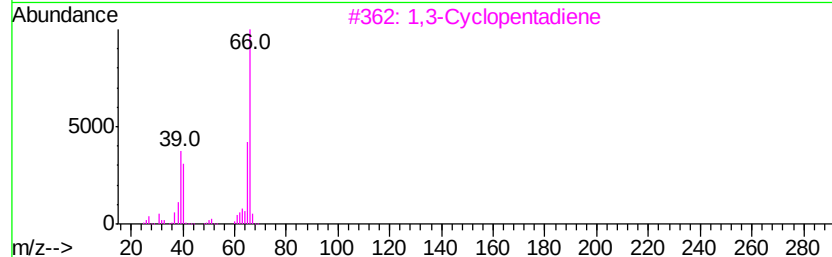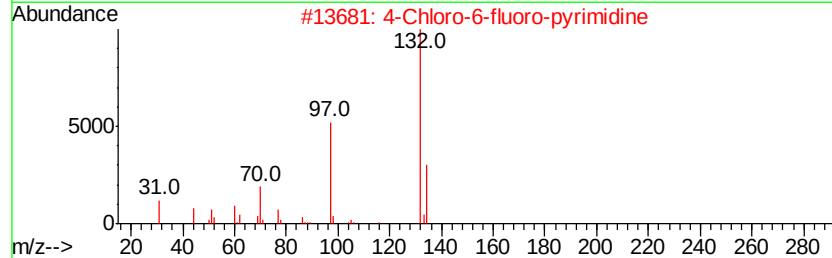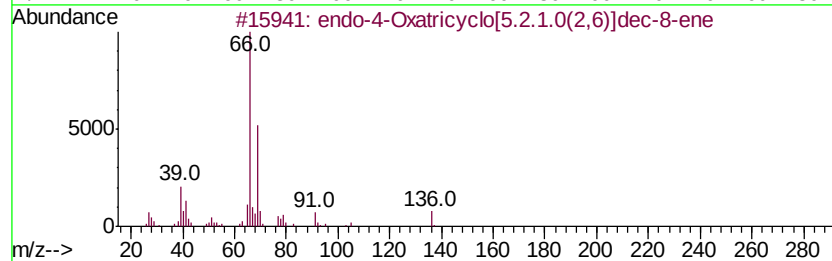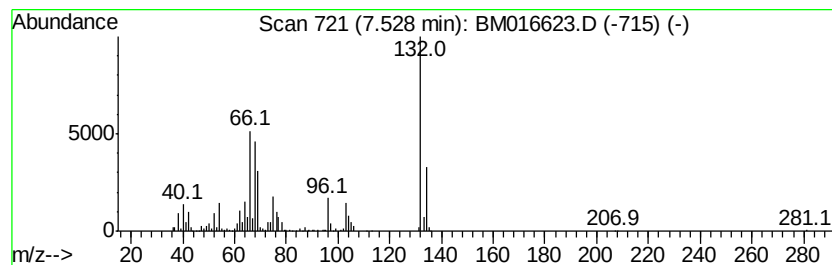

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082718\
Data File : BM016623.D
Acq On : 28 Aug 2018 02:16
Operator : SJ/JU
Sample : J4660-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082318-DBRI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	64.8	ng	2013660	1	8.00	621373	20.0