

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
 Data File : BM016631.D
 Acq On : 28 Aug 2018 07:03
 Operator : SJ/JU
 Sample : PB112404BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112404BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.545	379	384	401	rBV	1242999	2052537	14.01%	4.313%
2	7.175	656	661	677	rBV	1233973	2058662	14.05%	4.326%
3	7.528	715	721	741	rBV	1555639	2635003	17.98%	5.537%
4	8.004	796	802	814	rBV	379344	711823	4.86%	1.496%
5	8.316	848	855	870	rBV	2185399	3529930	24.09%	7.417%
6	9.186	996	1003	1017	rBV	1199684	2091241	14.27%	4.394%
7	10.804	1272	1278	1293	rBV	401823	798257	5.45%	1.677%
8	13.257	1688	1695	1709	rBV	5543765	7514675	51.29%	15.790%
9	14.639	1925	1930	1940	rBV2	702585	1141819	7.79%	2.399%
10	16.133	2178	2184	2196	rBV	3149100	4564129	31.15%	9.590%
11	17.386	2392	2397	2412	rBV	1068954	1702757	11.62%	3.578%
12	19.974	2831	2837	2852	rBV	13560821	14652603	100.00%	30.788%
13	21.527	3097	3101	3108	rBV	1496868	2106093	14.37%	4.425%
14	23.809	3484	3489	3501	rVB	1014290	2032813	13.87%	4.271%


Sum of corrected areas: 47592342

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016631.D
Acq On : 28 Aug 2018 07:03
Operator : SJ/JU
Sample : PB112404BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112404BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

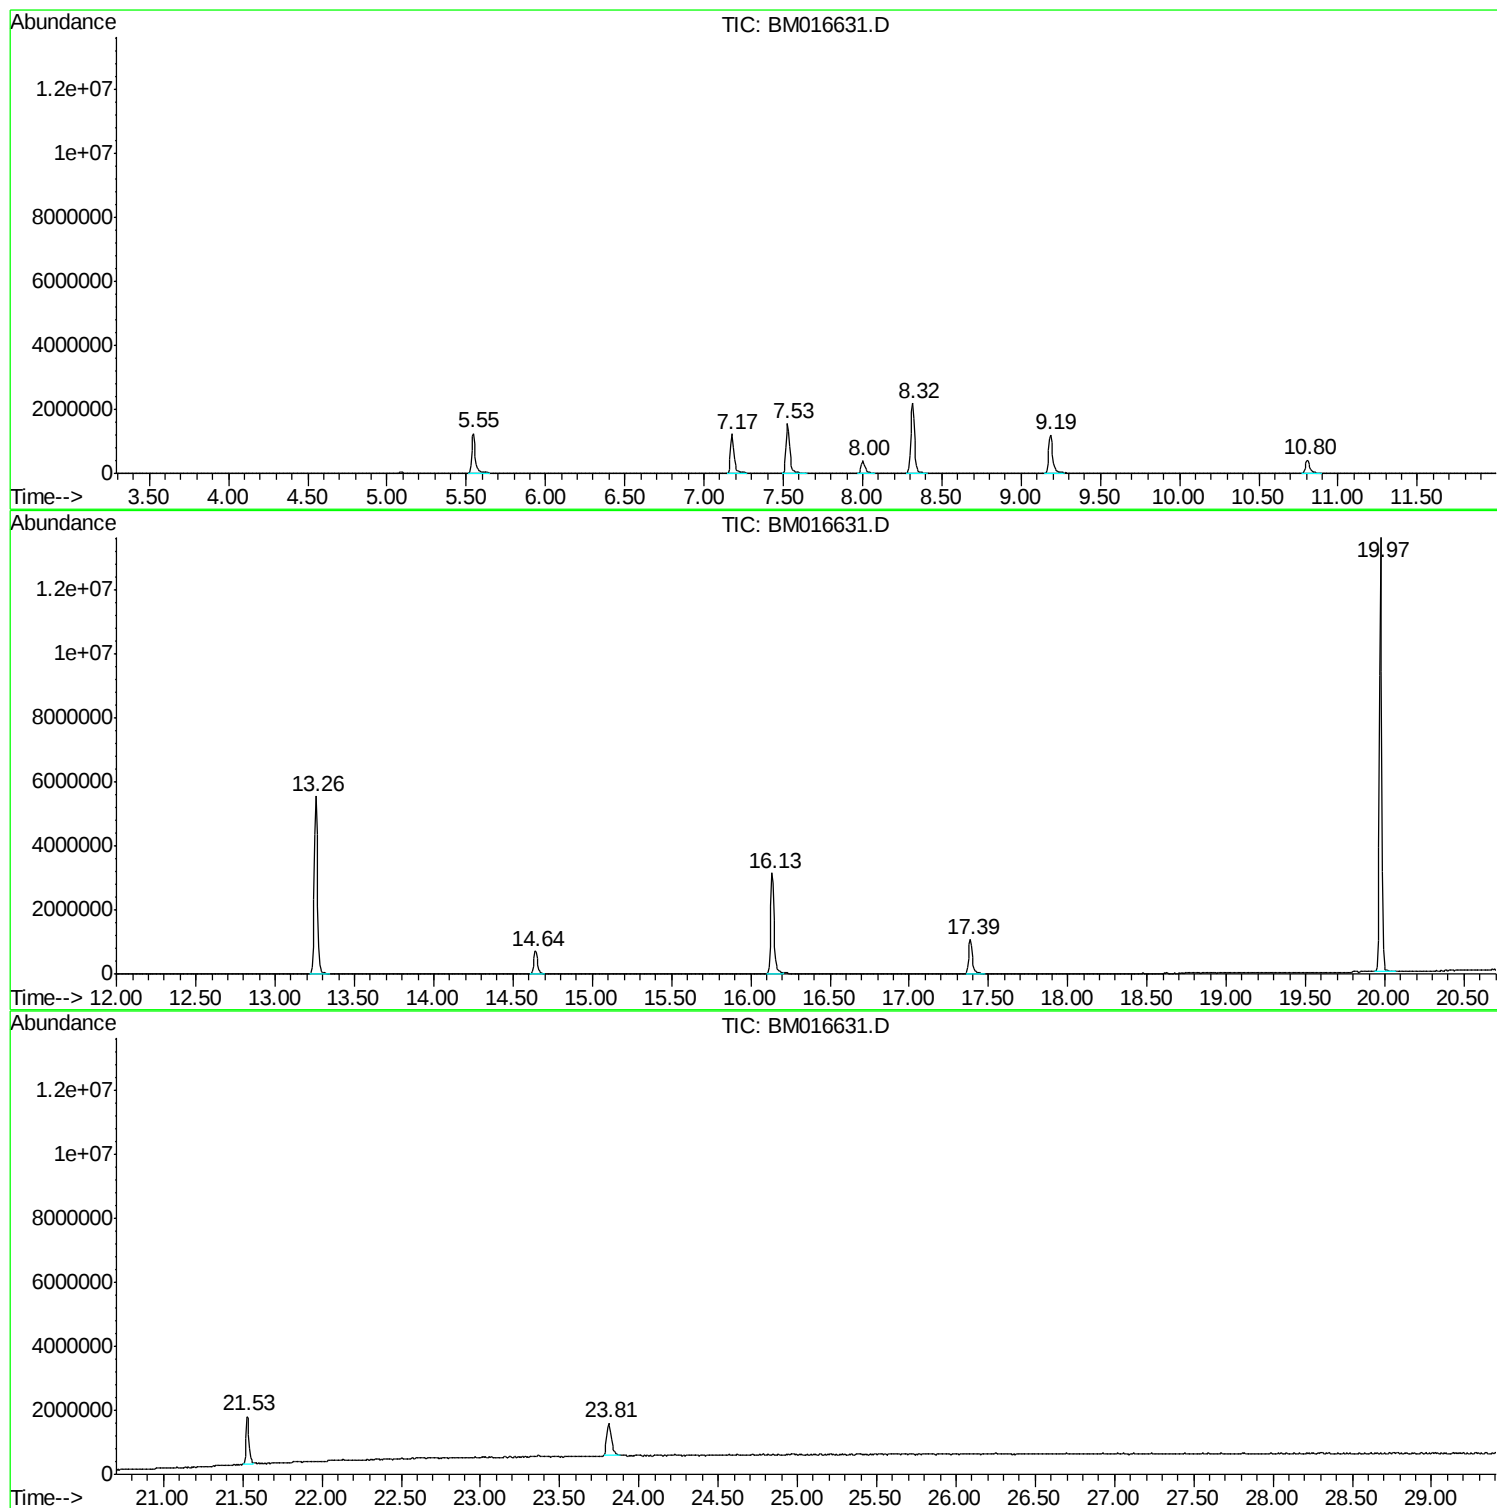

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082718\
Data File : BM016631.D
Acq On : 28 Aug 2018 07:03
Operator : SJ/JU
Sample : PB112404BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112404BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	74.04 ng	2635000	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	22
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

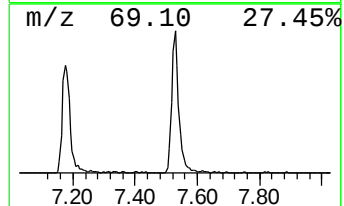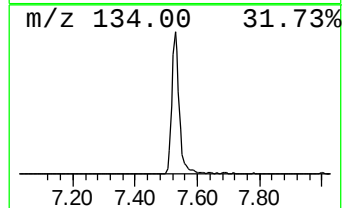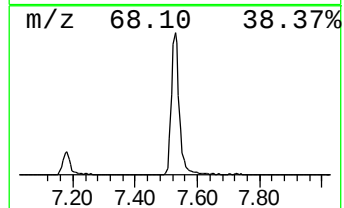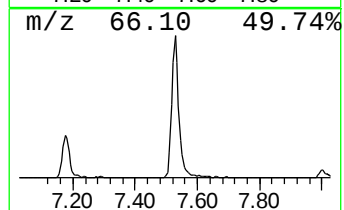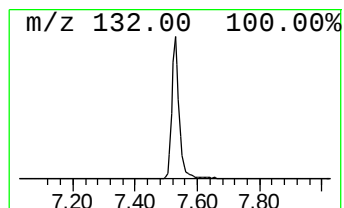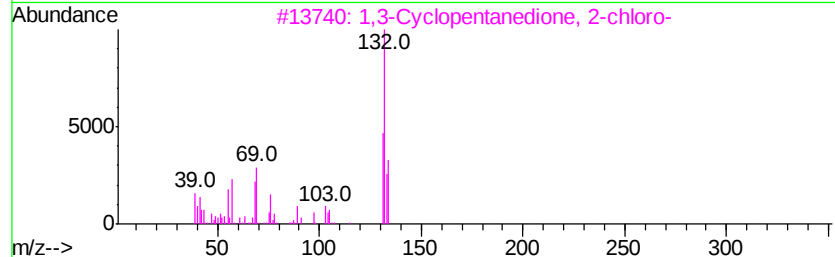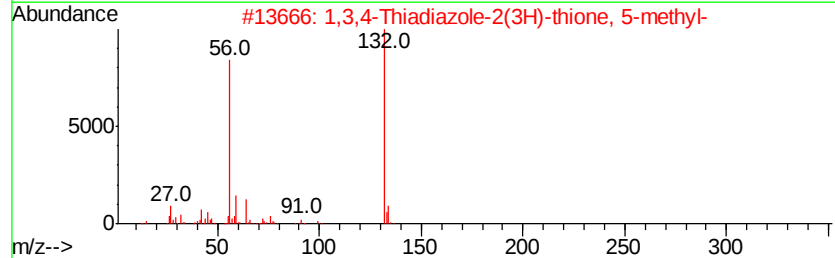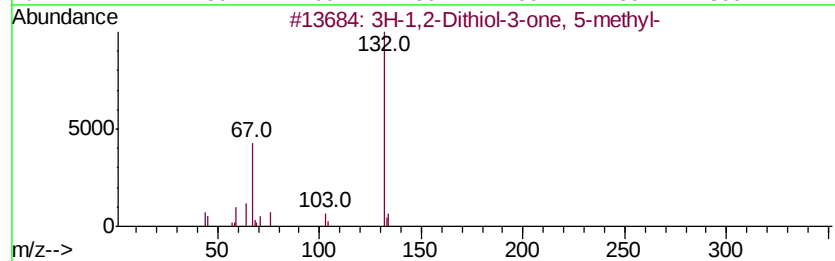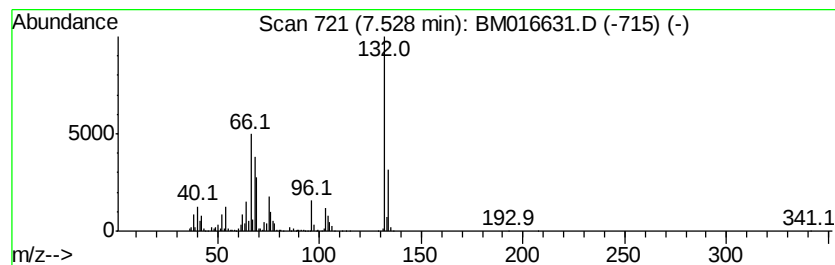

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082718\
Data File : BM016631.D
Acq On : 28 Aug 2018 07:03
Operator : SJ/JU
Sample : PB112404BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112404BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.53	7.53	74.0	ng	2635000	1	8.00	711823	20.0