


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082718\
 Data File : BM016597.D
 Acq On : 27 Aug 2018 09:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 27 13:01:22 2018

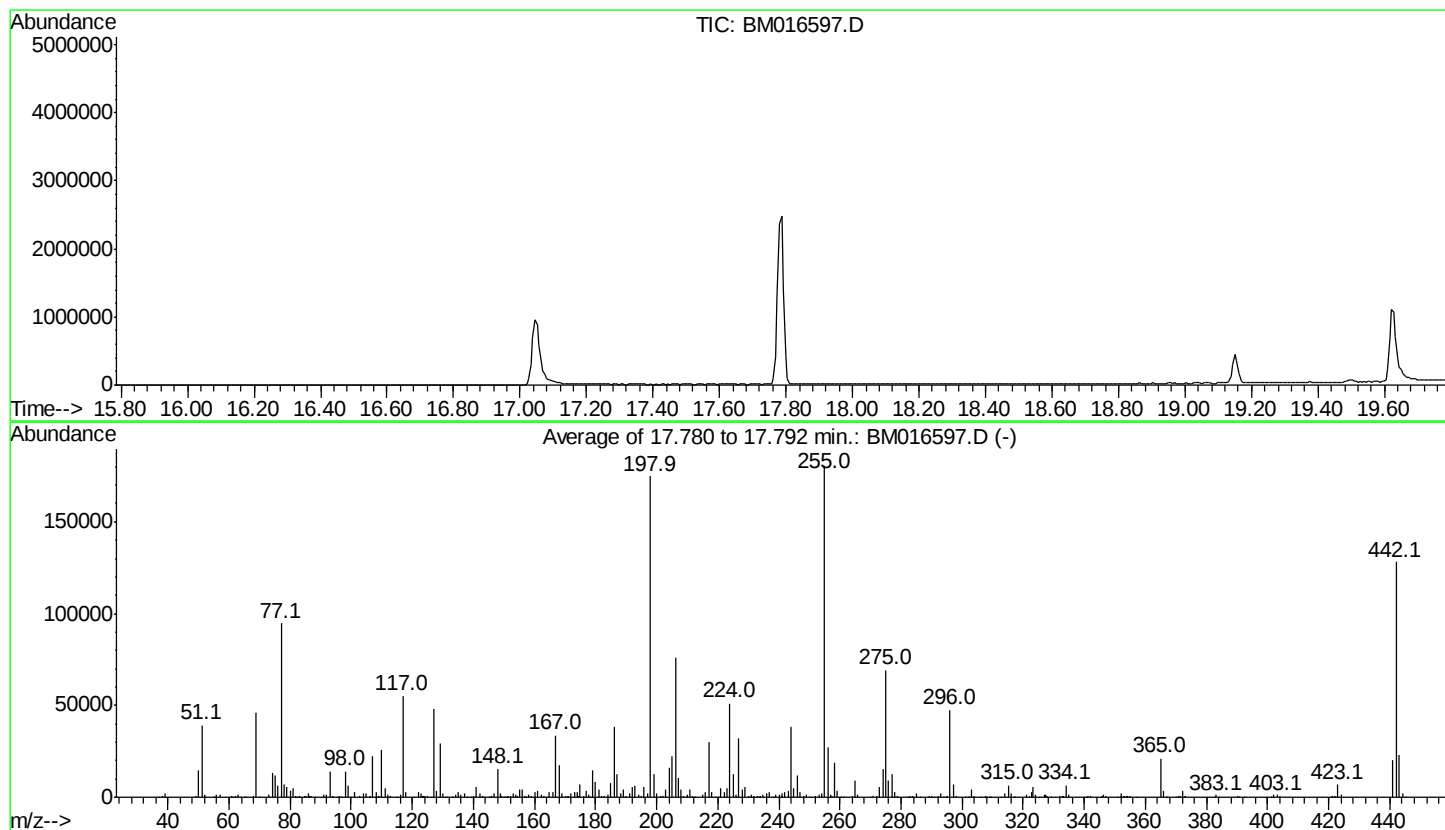

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	39104	PASS
68	69	0.00	2	1.9	892	PASS
69	198	0.00	100	26.4	46096	PASS
70	69	0.00	2	0.8	356	PASS
127	198	10	80	27.6	48269	PASS
197	198	0.00	2	1.2	2181	PASS
198	198	100	100	100.0	174922	PASS
199	198	5	9	7.0	12272	PASS
275	198	10	60	39.6	69272	PASS
365	198	1	100	12.1	21197	PASS
441	198	0.01	100	11.6	20360	PASS
442	198	50	100	73.2	128000	PASS
443	442	15	24	18.0	23016	PASS