


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082718\
 Data File : BM016617.D
 Acq On : 27 Aug 2018 22:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 27 13:01:22 2018

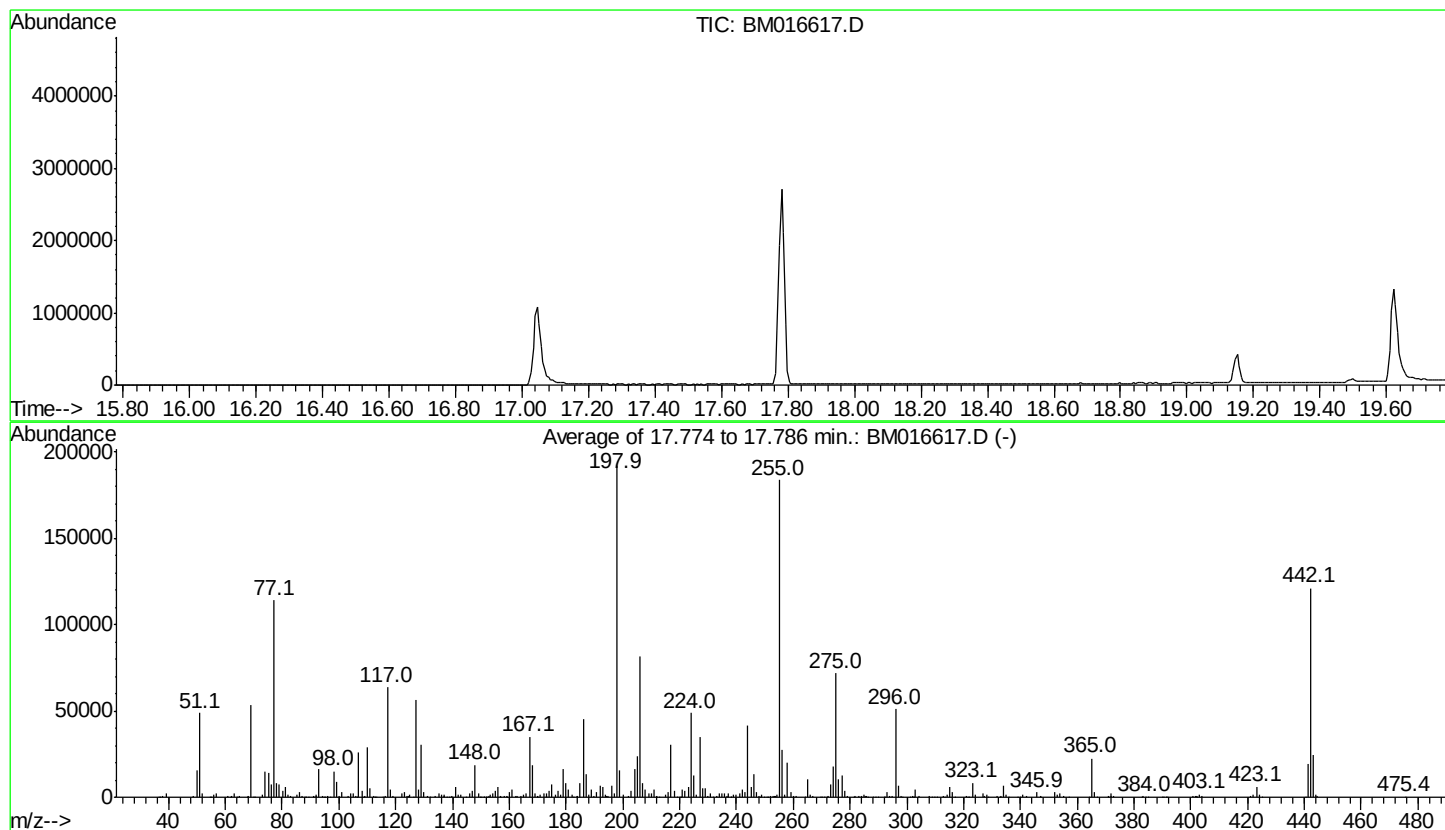

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	48642	PASS
68	69	0.00	2	2.1	1113	PASS
69	198	0.00	100	27.8	53346	PASS
70	69	0.00	2	0.3	184	PASS
127	198	10	80	29.2	56088	PASS
197	198	0.00	2	1.1	2071	PASS
198	198	100	100	100.0	191872	PASS
199	198	5	9	8.0	15271	PASS
275	198	10	60	37.4	71717	PASS
365	198	1	100	11.8	22570	PASS
441	198	0.01	100	10.1	19410	PASS
442	198	50	100	63.1	121104	PASS
443	442	15	24	19.9	24154	PASS