

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082720\
 Data File : BM027277.D
 Acq On : 27 Aug 2020 15:32
 Operator : JU/CG
 Sample : L3776-10DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4Y09DL

Quant Time: Aug 27 16:11:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 27 10:53:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	137110	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	520459	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	355995	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	784868	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	773683	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	689068	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	6.78	99	6390	0.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	18630	2.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	18431	2.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	11501	1.29	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	9905	2.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	9466	1.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.65	166	82937	2.94	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	85504	2.56	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
58) Fluorene-d10	15.23	176	68693	2.82	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	17.07	188	116253	3.12	ng/ul	0.00
79) Pyrene-d10	19.37	212	136124	3.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	112855	2.94	ng/ul	0.00


Target Compounds				Ovalue
32) Caprolactam	11.29	113	103749	36.332 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082720\
Data File : BM027277.D
Acq On : 27 Aug 2020 15:32
Operator : JU/CG
Sample : L3776-10DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4Y09DL

Quant Time: Aug 27 16:11:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 27 10:53:34 2020
Response via : Initial Calibration

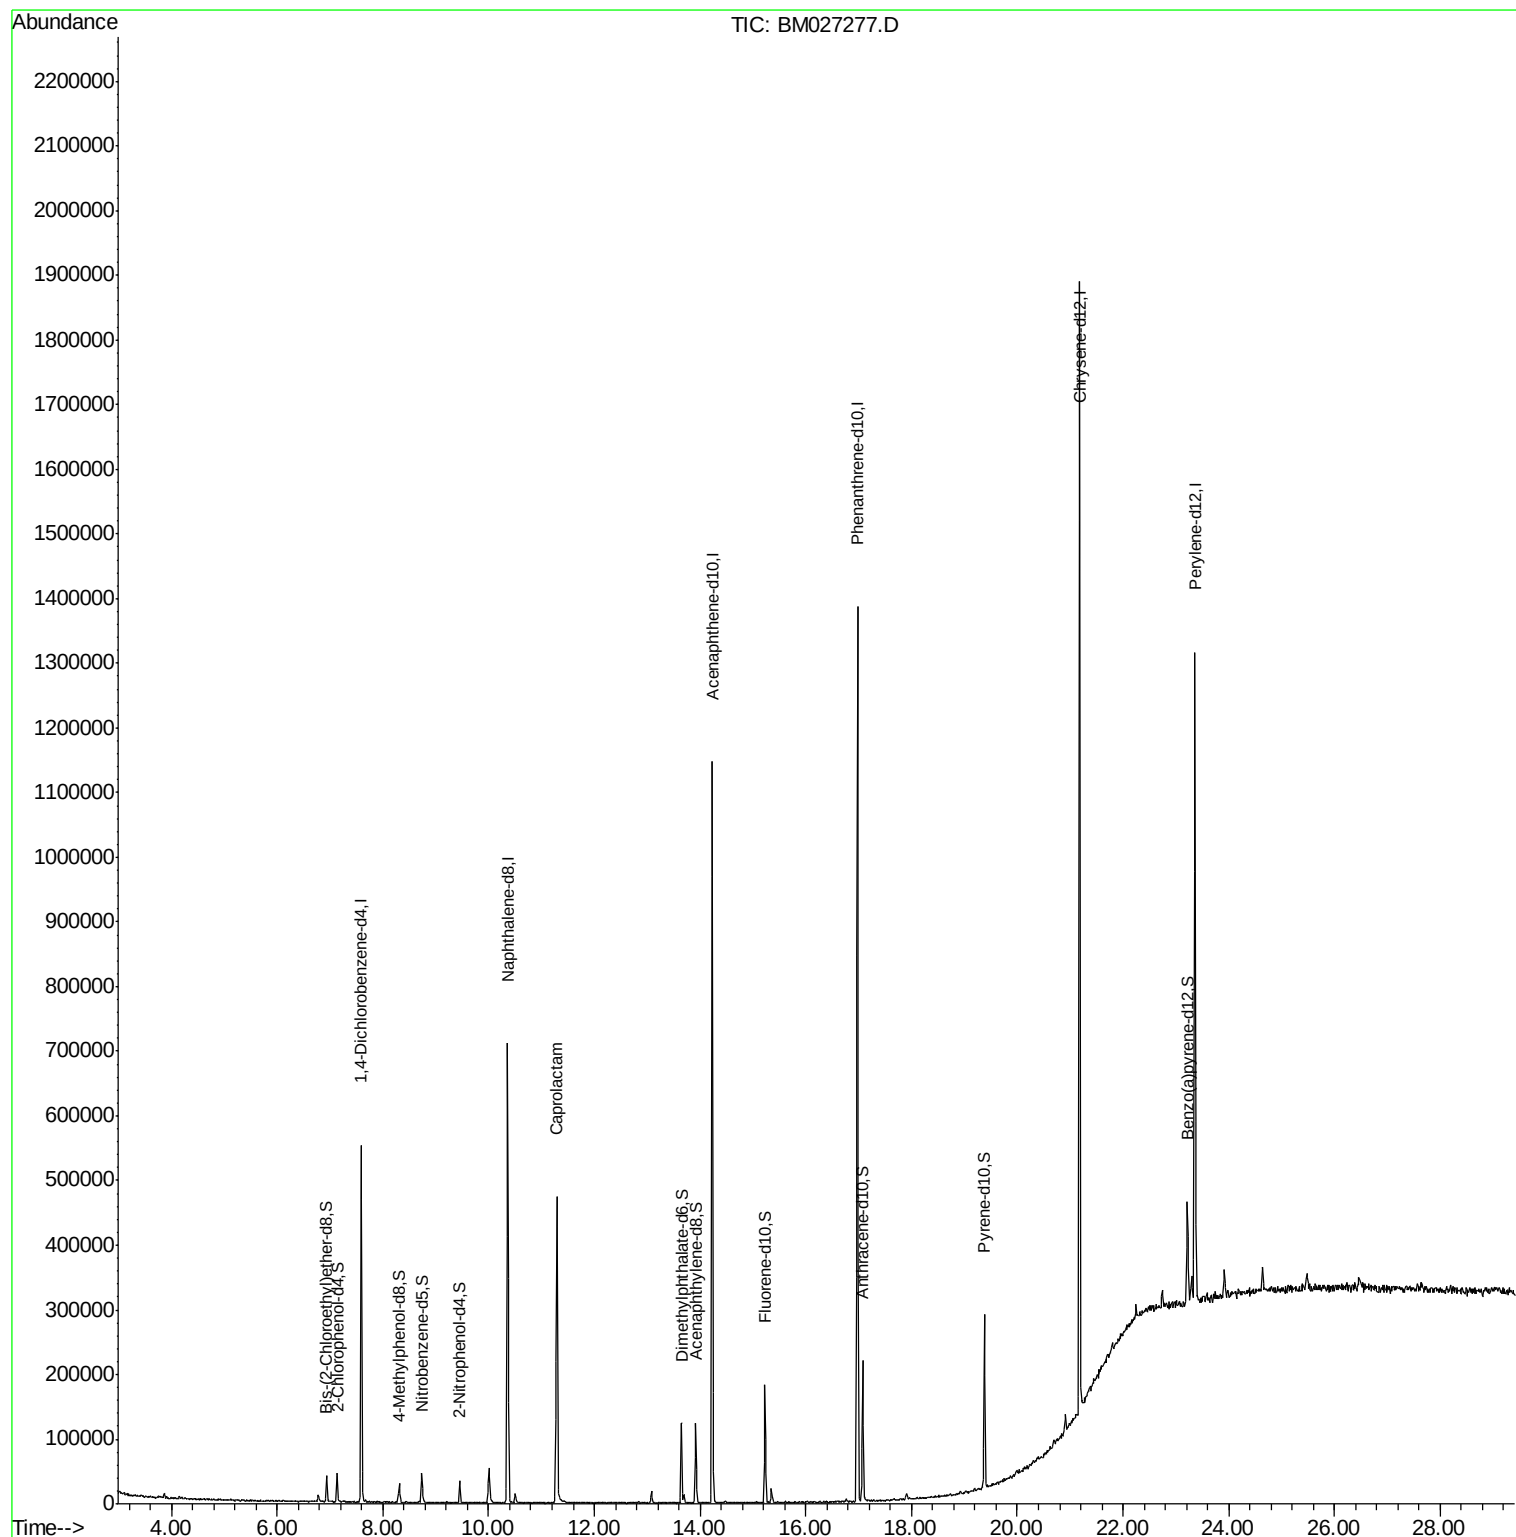

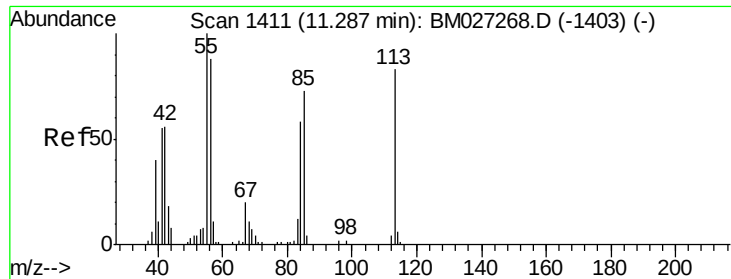

#32
 Caprolactam
 Concen: 36.332 ng/ul
 RT: 11.29 min Scan# 1412
 Delta R.T. 0.01 min
 Lab File: BM027277.D
 Acq: 27 Aug 2020 15:32

Instrument :
 BNA_M
 ClientSampleId :
 F4Y09DL

Tot Ion:113 Resp: 103749
 Ion Ratio Lower Upper
 113 100
 55 116.2 94.0 141.0
 56 103.1 82.4 123.6

