

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
 Data File : BM022389.D
 Acq On : 28 Aug 2019 18:51
 Operator : HP/JU
 Sample : PB122291BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	17	18	21	rBV2	1528	1331	0.14%	0.017%
2	3.122	21	23	28	rBV2	4671	6270	0.68%	0.080%
3	3.240	39	43	44	rVB3	1121	1024	0.11%	0.013%
4	3.322	54	57	60	rBV4	944	1196	0.13%	0.015%
5	3.387	67	68	71	rBV2	987	1059	0.11%	0.013%
6	3.605	103	105	108	rVB2	945	1035	0.11%	0.013%
7	3.640	108	111	113	rBV2	998	1389	0.15%	0.018%
8	6.734	632	637	651	rBV	103367	191896	20.74%	2.442%
9	6.899	659	665	676	rBV	73412	124823	13.49%	1.588%
10	7.075	689	695	703	rBV	131374	212793	23.00%	2.708%
11	7.534	767	773	783	rBV	86299	136950	14.80%	1.743%
12	8.257	891	896	909	rBV	141437	247783	26.79%	3.153%
13	8.710	967	973	983	rBV	123417	208886	22.58%	2.658%
14	8.775	983	984	991	rVB	1787	1919	0.21%	0.024%
15	9.422	1088	1094	1105	rVB	110501	191940	20.75%	2.443%
16	9.951	1179	1184	1207	rBV	129342	280773	30.35%	3.573%
17	10.310	1238	1245	1254	rBB	127020	208776	22.57%	2.657%
18	10.481	1269	1274	1292	rBV	107940	257588	27.85%	3.278%
19	11.933	1519	1521	1525	rBB2	1557	1912	0.21%	0.024%
20	13.622	1802	1808	1820	rBV	317583	470452	50.86%	5.987%
21	13.886	1847	1853	1863	rBV	376517	534091	57.74%	6.797%
22	14.192	1900	1905	1913	rBB2	211434	307802	33.27%	3.917%
23	14.486	1950	1955	1980	rBV3	35231	127002	13.73%	1.616%
24	14.645	1980	1982	1985	rVB	1250	1174	0.13%	0.015%
25	15.198	2070	2076	2088	rBV	444416	683581	73.90%	8.699%
26	15.280	2088	2090	2092	rVB	1391	1190	0.13%	0.015%
27	15.374	2101	2106	2116	rBV	63353	119806	12.95%	1.525%
28	15.439	2116	2117	2125	rVB	4532	5069	0.55%	0.065%
29	15.680	2155	2158	2162	rBV	541	982	0.11%	0.012%
30	16.027	2216	2217	2223	rBV	442	975	0.11%	0.012%
31	16.957	2370	2375	2386	rBV2	279468	391123	42.28%	4.977%
32	17.063	2386	2393	2411	rVB	520462	781098	84.44%	9.940%
33	18.374	2613	2616	2619	rBV	911	1481	0.16%	0.019%
34	18.527	2638	2642	2643	rBV	918	940	0.10%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
 Data File : BM022389.D
 Acq On : 28 Aug 2019 18:51
 Operator : HP/JU
 Sample : PB122291BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	18.592	2649	2653	2654	rBV	1288	1156	0.12%	0.015%
36	18.680	2664	2668	2670	rBV2	918	1133	0.12%	0.014%
37	18.810	2688	2690	2692	rVB	1785	1343	0.15%	0.017%
38	18.898	2701	2705	2707	rVB2	800	1205	0.13%	0.015%
39	18.939	2709	2712	2715	rBV2	1042	1494	0.16%	0.019%
40	19.004	2719	2723	2725	rBV2	4587	5299	0.57%	0.067%
41	19.257	2762	2766	2771	rBV2	2958	4595	0.50%	0.058%
42	19.321	2775	2777	2779	rBV2	1112	976	0.11%	0.012%
43	19.368	2779	2785	2795	rBV	597109	925045	100.00%	11.772%
44	19.639	2829	2831	2833	rBV3	1216	971	0.10%	0.012%
45	19.768	2850	2853	2855	rBV3	1843	1956	0.21%	0.025%
46	19.927	2879	2880	2882	rBV	1523	1202	0.13%	0.015%
47	20.233	2931	2932	2935	rBV3	1683	1394	0.15%	0.018%
48	21.180	3088	3093	3100	rBV	259037	382860	41.39%	4.872%
49	23.227	3434	3441	3451	rVB	349276	679612	73.47%	8.649%
50	23.368	3459	3465	3478	rVB	167936	341660	36.93%	4.348%


Sum of corrected areas: 7858010

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
Data File : BM022389.D
Acq On : 28 Aug 2019 18:51
Operator : HP/JU
Sample : PB122291BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

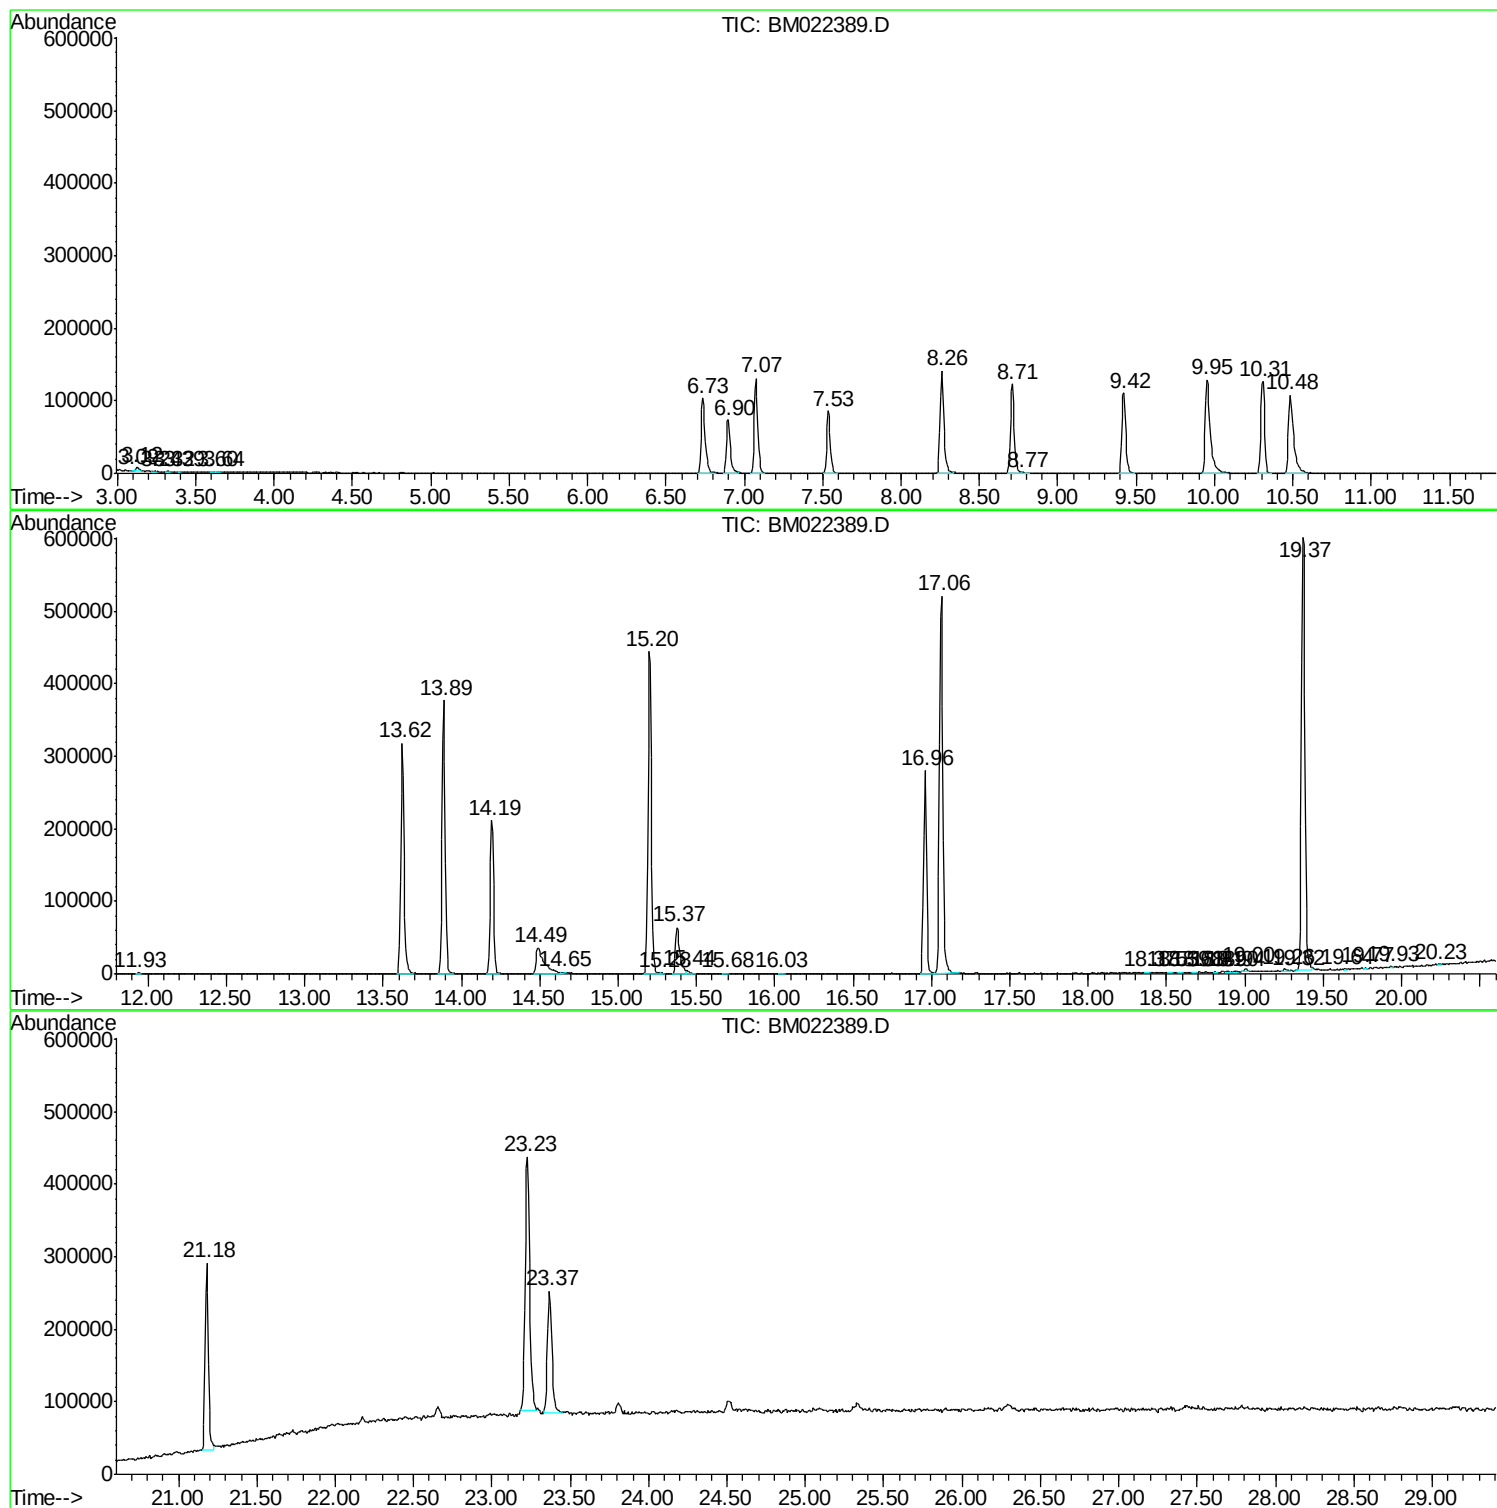

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082819\
Data File : BM022389.D
Acq On : 28 Aug 2019 18:51
Operator : HP/JU
Sample : PB122291BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082819\
Data File : BM022389.D
Acq On : 28 Aug 2019 18:51
Operator : HP/JU
Sample : PB122291BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc