

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
 Data File : BM022390.D
 Acq On : 28 Aug 2019 19:27
 Operator : HP/JU
 Sample : PB122641BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	32	rVB2	5873	8439	1.00%	0.110%
2	3.546	91	95	99	rBV3	625	1137	0.14%	0.015%
3	3.805	138	139	144	rVB2	894	940	0.11%	0.012%
4	4.293	219	222	225	rBV	1035	1039	0.12%	0.014%
5	4.558	263	267	270	rVB2	806	953	0.11%	0.012%
6	4.599	270	274	277	rBV	585	975	0.12%	0.013%
7	5.128	360	364	366	rBV	686	1060	0.13%	0.014%
8	6.499	592	597	598	rBV	512	854	0.10%	0.011%
9	6.734	632	637	649	rBV	104908	188706	22.44%	2.458%
10	6.899	659	665	676	rBV	72706	126786	15.08%	1.651%
11	7.075	690	695	703	rBV	131136	208549	24.80%	2.716%
12	7.534	766	773	782	rBB	85023	136141	16.19%	1.773%
13	8.257	891	896	907	rBV	140467	242355	28.82%	3.156%
14	8.328	907	908	913	rVB	1593	1479	0.18%	0.019%
15	8.710	967	973	987	rBV	125451	210868	25.08%	2.746%
16	9.422	1087	1094	1104	rBB2	111148	192010	22.83%	2.501%
17	9.951	1179	1184	1202	rBV	132129	277243	32.97%	3.611%
18	10.063	1202	1203	1207	rVB2	2117	1587	0.19%	0.021%
19	10.310	1238	1245	1252	rBV	126921	208514	24.80%	2.716%
20	10.487	1268	1275	1289	rBV	110422	254697	30.29%	3.317%
21	10.640	1298	1301	1304	rVB	724	861	0.10%	0.011%
22	11.939	1518	1522	1528	rBB2	1877	2449	0.29%	0.032%
23	13.622	1802	1808	1823	rBV	325130	470520	55.95%	6.128%
24	13.886	1847	1853	1862	rBV2	371646	531353	63.19%	6.920%
25	14.192	1900	1905	1915	rBB	209616	303076	36.04%	3.947%
26	14.492	1950	1956	1978	rBV2	34649	124217	14.77%	1.618%
27	14.657	1982	1984	1989	rVV	1735	3145	0.37%	0.041%
28	15.198	2070	2076	2095	rBV	445763	681965	81.10%	8.882%
29	15.375	2101	2106	2116	rBV2	61190	113839	13.54%	1.483%
30	15.439	2116	2117	2125	rVB2	4462	5692	0.68%	0.074%
31	16.957	2370	2375	2386	rVB2	278329	374605	44.55%	4.879%
32	17.057	2386	2392	2418	rVB2	495977	757530	90.08%	9.866%
33	18.386	2613	2618	2619	rBV	781	990	0.12%	0.013%
34	18.839	2694	2695	2699	rBV2	1712	1793	0.21%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
 Data File : BM022390.D
 Acq On : 28 Aug 2019 19:27
 Operator : HP/JU
 Sample : PB122641BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	18.904	2703	2706	2708	rBV	1037	1152	0.14%	0.015%
36	18.963	2715	2716	2718	rBV2	1115	1037	0.12%	0.014%
37	19.004	2720	2723	2725	rBV2	3377	3919	0.47%	0.051%
38	19.257	2763	2766	2770	rBV	3004	4722	0.56%	0.061%
39	19.374	2780	2786	2796	rBV	548766	840929	100.00%	10.952%
40	19.568	2817	2819	2820	rBV	983	1002	0.12%	0.013%
41	19.657	2832	2834	2835	rBV2	960	968	0.12%	0.013%
42	19.810	2857	2860	2861	rBV3	1400	1670	0.20%	0.022%
43	20.262	2935	2937	2939	rBV3	2524	1917	0.23%	0.025%
44	21.180	3088	3093	3103	rBV	238103	346300	41.18%	4.510%
45	23.227	3434	3441	3453	rVB	356992	681691	81.06%	8.878%
46	23.368	3459	3465	3478	rVB2	164675	327636	38.96%	4.267%
47	23.809	3537	3540	3544	rVB4	21711	29059	3.46%	0.378%


Sum of corrected areas: 7678369

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
Data File : BM022390.D
Acq On : 28 Aug 2019 19:27
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

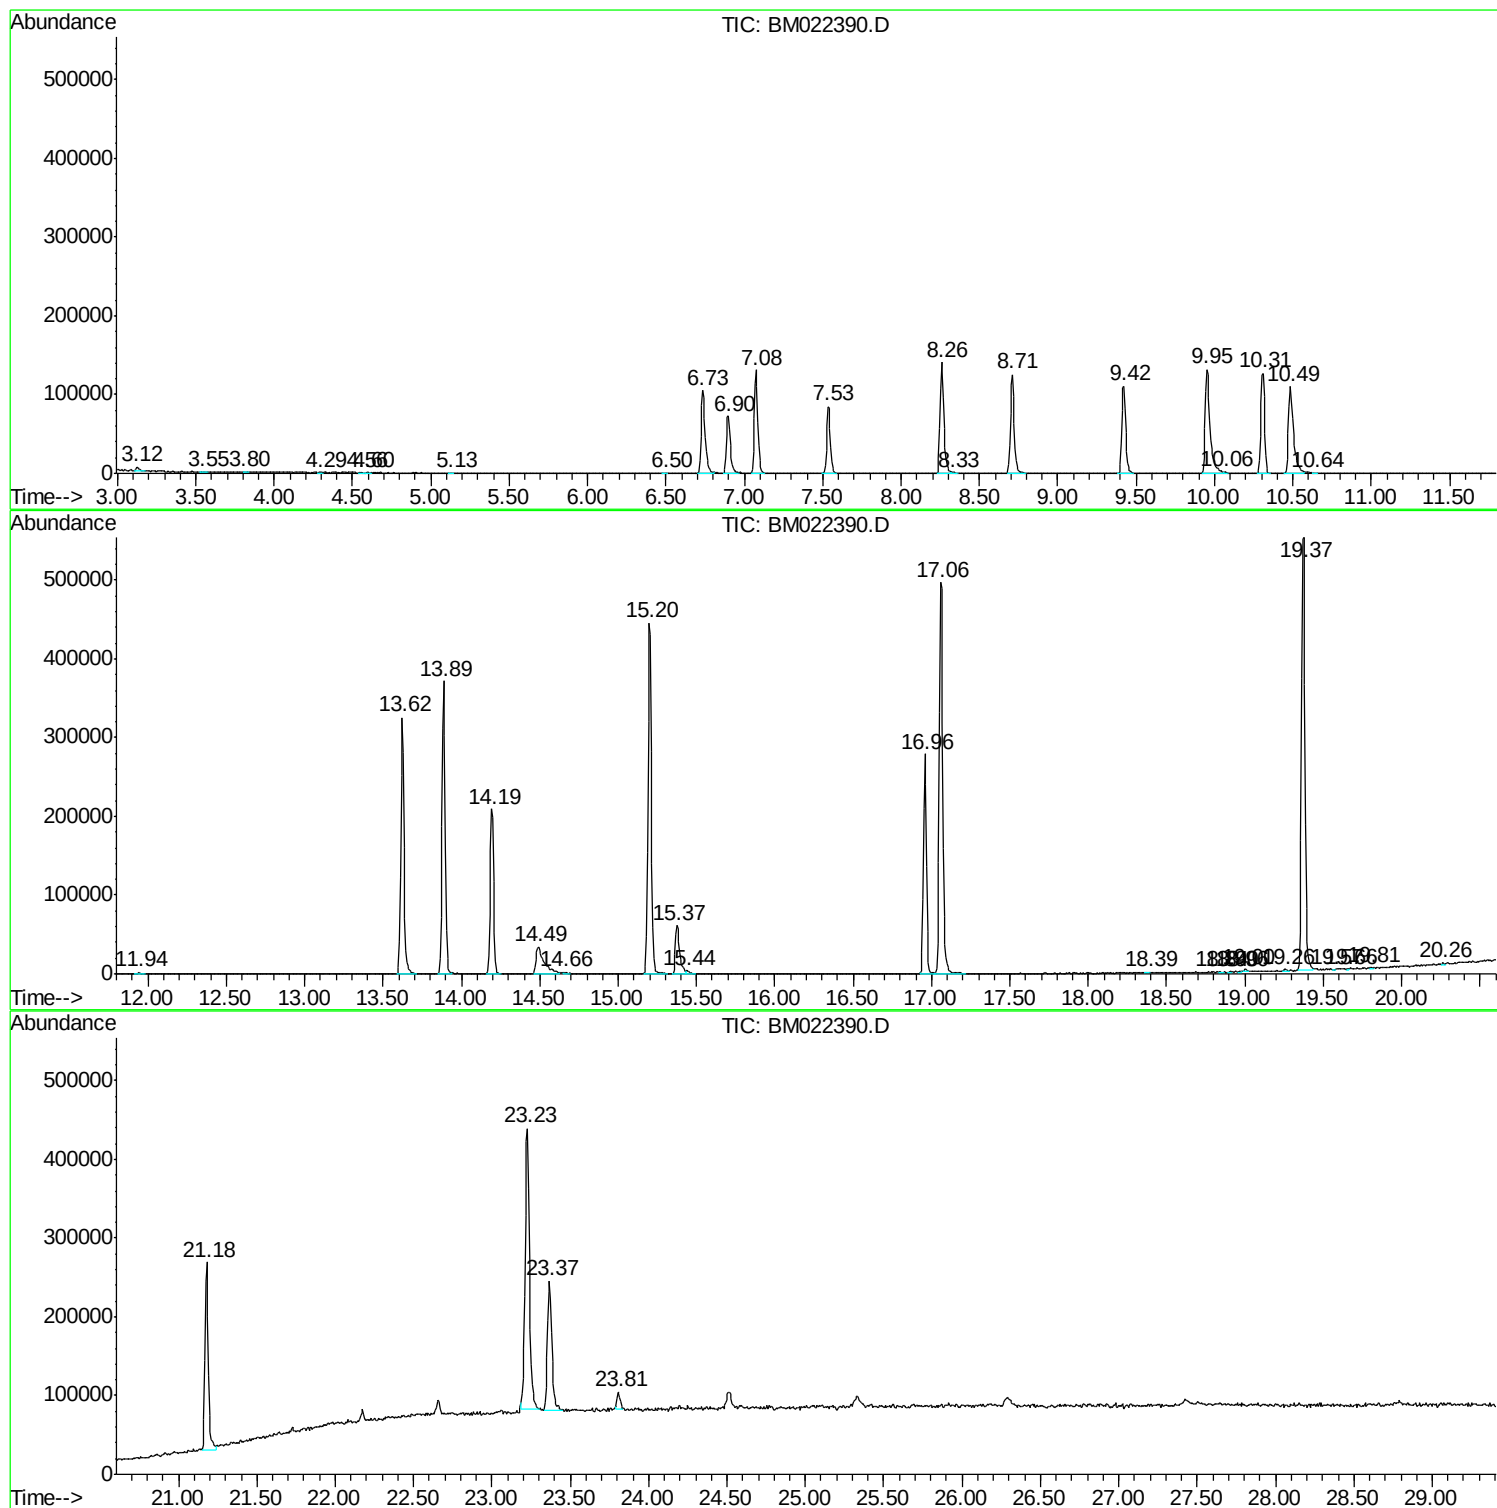

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082819\
Data File : BM022390.D
Acq On : 28 Aug 2019 19:27
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082819\
Data File : BM022390.D
Acq On : 28 Aug 2019 19:27
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc