

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
 Data File : BM022394.D
 Acq On : 28 Aug 2019 22:29
 Operator : HP/JU
 Sample : PB122603BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	3	5	9	rVB	8192	7527	2.35%	0.504%
2	3.722	121	125	128	rBV2	659	1109	0.35%	0.074%
3	3.775	131	134	137	rVV2	502	661	0.21%	0.044%
4	3.975	166	168	171	rBV2	613	798	0.25%	0.053%
5	4.157	197	199	202	rBV	529	652	0.20%	0.044%
6	4.257	211	216	219	rBV	659	1020	0.32%	0.068%
7	4.328	225	228	230	rBV	673	668	0.21%	0.045%
8	4.416	239	243	244	rBV2	549	718	0.22%	0.048%
9	4.487	253	255	260	rBV	647	588	0.18%	0.039%
10	4.775	301	304	307	rVB2	497	629	0.20%	0.042%
11	5.034	345	348	351	rBV	786	1047	0.33%	0.070%
12	5.475	420	423	424	rBV	460	546	0.17%	0.037%
13	5.563	435	438	440	rBV	499	681	0.21%	0.046%
14	5.793	476	477	480	rBV	466	602	0.19%	0.040%
15	5.940	501	502	505	rBV	656	626	0.20%	0.042%
16	6.140	534	536	540	rBV	452	826	0.26%	0.055%
17	6.269	555	558	560	rBV	413	625	0.19%	0.042%
18	6.363	573	574	576	rBV	553	445	0.14%	0.030%
19	6.534	602	603	606	rBV	700	621	0.19%	0.042%
20	7.004	681	683	685	rBB	457	470	0.15%	0.031%
21	7.275	727	729	732	rBB	416	498	0.16%	0.033%
22	7.381	745	747	749	rBV	424	513	0.16%	0.034%
23	7.534	768	773	790	rBB	71746	127153	39.64%	8.506%
24	8.098	867	869	872	rBB	444	546	0.17%	0.037%
25	8.698	970	971	975	rBV	360	575	0.18%	0.038%
26	10.310	1239	1245	1262	rBV	74947	166939	52.05%	11.168%
27	11.939	1519	1522	1523	rBV	386	502	0.16%	0.034%
28	14.198	1898	1906	1918	rBV2	140560	252569	78.74%	16.897%
29	14.333	1926	1929	1930	rBB	609	463	0.14%	0.031%
30	14.404	1939	1941	1943	rBV	346	455	0.14%	0.030%
31	14.557	1964	1967	1969	rBB	342	445	0.14%	0.030%
32	14.645	1981	1982	1985	rBV	355	455	0.14%	0.030%
33	14.786	2003	2006	2009	rBB	431	517	0.16%	0.035%
34	14.845	2013	2016	2018	rBB	364	471	0.15%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
 Data File : BM022394.D
 Acq On : 28 Aug 2019 22:29
 Operator : HP/JU
 Sample : PB122603BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	14.974	2036	2038	2041	rBV	390	640	0.20%	0.043%
36	15.068	2052	2054	2057	rBB	469	522	0.16%	0.035%
37	15.104	2057	2060	2062	rBV	374	591	0.18%	0.040%
38	15.145	2064	2067	2068	rBV	495	515	0.16%	0.034%
39	15.463	2119	2121	2124	rBB	468	545	0.17%	0.036%
40	15.498	2125	2127	2129	rBV	414	502	0.16%	0.034%
41	15.521	2129	2131	2133	rVB	461	473	0.15%	0.032%
42	15.715	2163	2164	2168	rBB	440	503	0.16%	0.034%
43	15.792	2175	2177	2181	rBB	456	530	0.17%	0.035%
44	15.927	2196	2200	2202	rVB	520	755	0.24%	0.051%
45	16.010	2211	2214	2215	rBV	442	535	0.17%	0.036%
46	16.151	2236	2238	2240	rVB	490	454	0.14%	0.030%
47	16.210	2245	2248	2251	rBV	458	834	0.26%	0.056%
48	16.257	2255	2256	2259	rVB	495	450	0.14%	0.030%
49	16.580	2309	2311	2312	rBV	569	480	0.15%	0.032%
50	16.968	2371	2377	2398	rBV	154126	301478	93.99%	20.168%
51	17.168	2410	2411	2415	rVB	681	671	0.21%	0.045%
52	18.527	2639	2642	2644	rBV2	1013	956	0.30%	0.064%
53	18.662	2661	2665	2668	rVB2	1092	1241	0.39%	0.083%
54	18.686	2668	2669	2671	rBV2	680	479	0.15%	0.032%
55	18.709	2671	2673	2674	rBV	657	537	0.17%	0.036%
56	18.751	2677	2680	2681	rVB	994	758	0.24%	0.051%
57	18.862	2698	2699	2701	rVB	1123	610	0.19%	0.041%
58	18.904	2702	2706	2709	rVV	1034	1341	0.42%	0.090%
59	18.927	2709	2710	2713	rVB2	1481	1090	0.34%	0.073%
60	18.956	2713	2715	2717	rBV	1041	1175	0.37%	0.079%
61	19.133	2741	2745	2747	rBV2	1516	2496	0.78%	0.167%
62	19.403	2789	2791	2794	rBV2	1737	1357	0.42%	0.091%
63	21.180	3088	3093	3103	rBV	205397	320751	100.00%	21.458%
64	23.368	3460	3465	3478	rVB2	137424	278570	86.85%	18.636%


Sum of corrected areas: 1494799

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082819\
Data File : BM022394.D
Acq On : 28 Aug 2019 22:29
Operator : HP/JU
Sample : PB122603BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

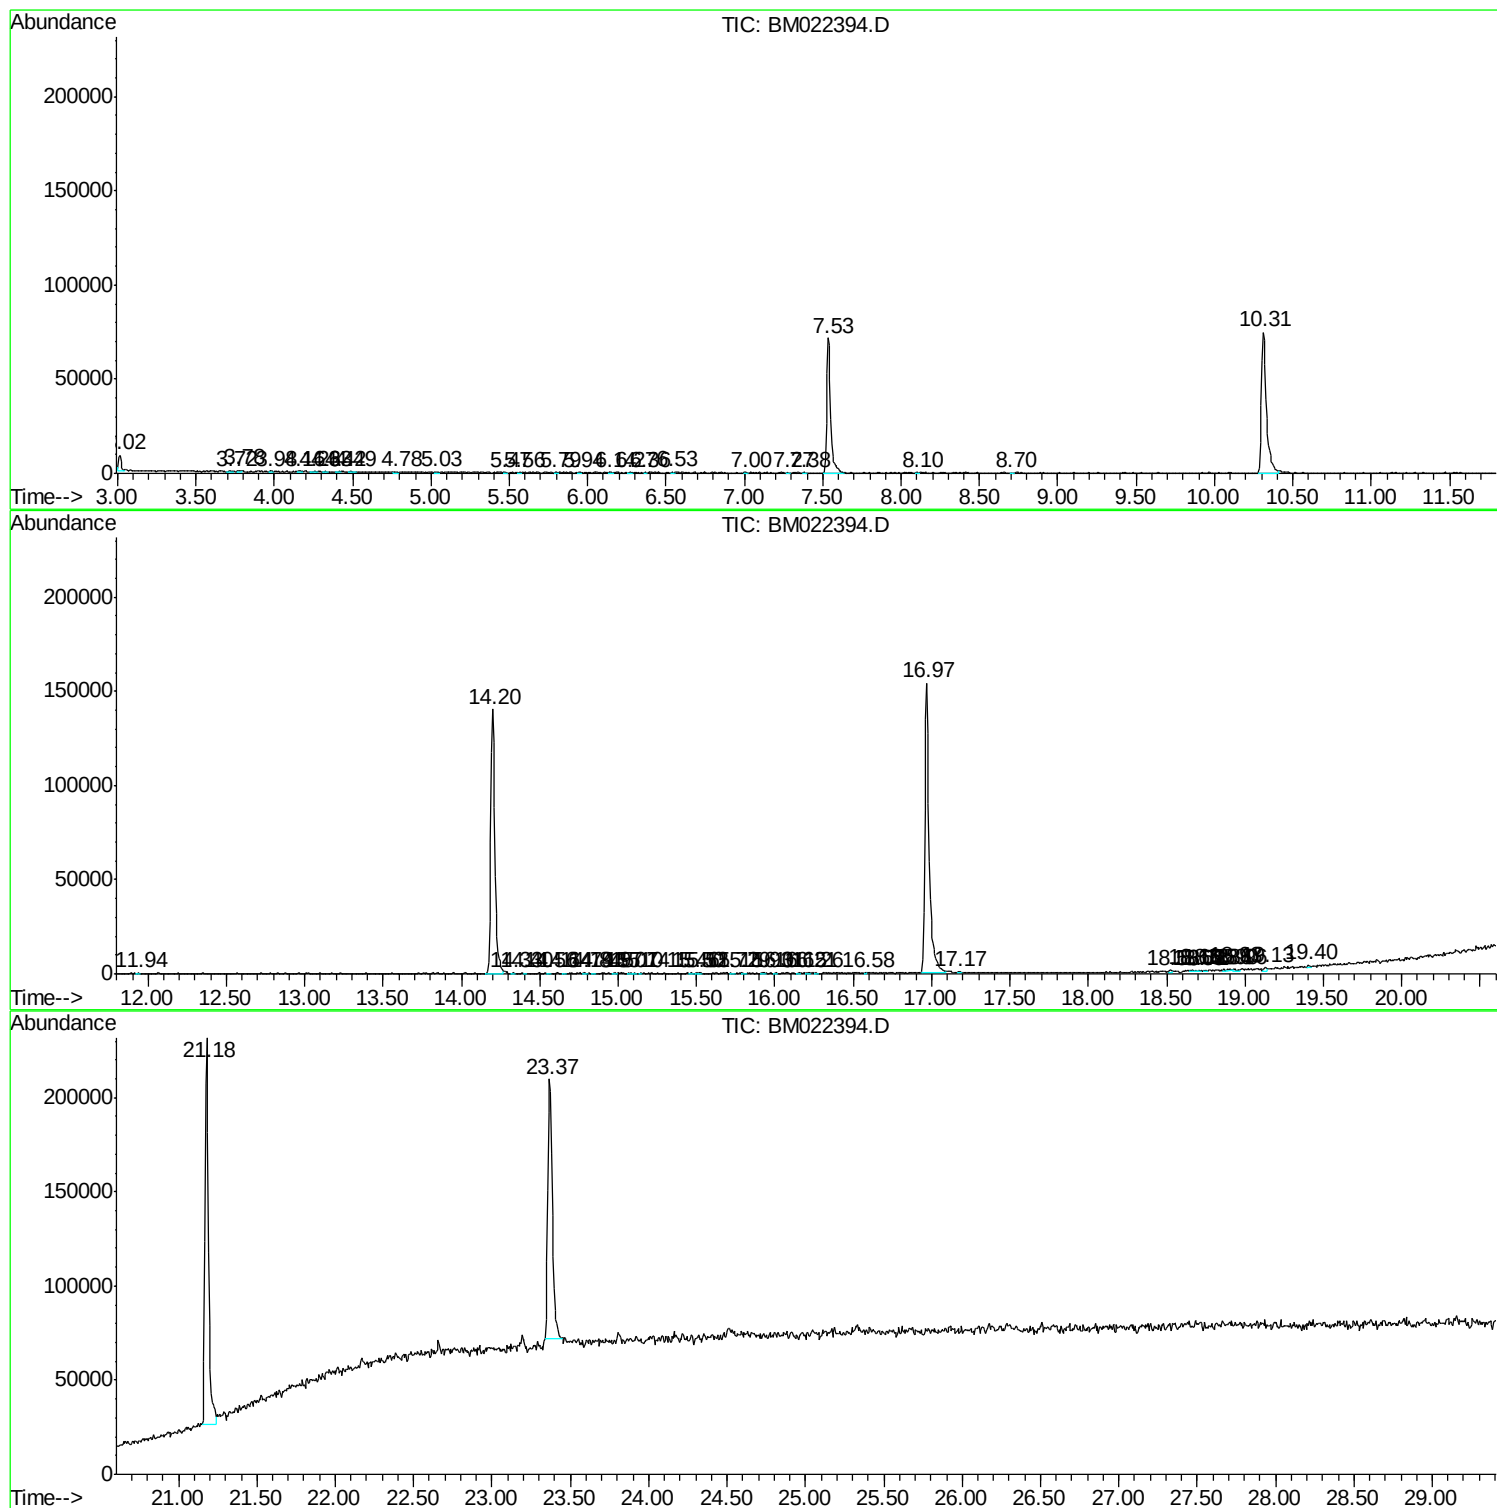

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082819\
Data File : BM022394.D
Acq On : 28 Aug 2019 22:29
Operator : HP/JU
Sample : PB122603BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082819\
Data File : BM022394.D
Acq On : 28 Aug 2019 22:29
Operator : HP/JU
Sample : PB122603BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc