

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031935.D
 Acq On : 28 Aug 2021 16:53
 Operator : CG/JU
 Sample : SSTD02020
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 28 23:55:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	80602	20.000	ng/u1	0.00
20) Naphthalene-d8	10.269	136	352124	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.151	164	268790	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.904	188	610850	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.109	240	702641	20.000	ng/u1	0.00
88) Perylene-d12	23.250	264	764172	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	14722	7.137	ng/uL	0.00
4) Pyridine-d5	3.522	84	100509	18.633	ng/u1	0.00
7) Phenol-d5	6.704	99	130659	18.552	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.869	67	78916	17.396	ng/u1	0.00
11) 2-Chlorophenol-d4	7.051	132	109109	20.192	ng/u1	0.00
15) 4-Methylphenol-d8	8.222	113	114289	20.249	ng/u1	0.00
21) Nitrobenzene-d5	8.663	128	56411	21.539	ng/u1	0.00
24) 2-Nitrophenol-d4	9.369	143	66048	23.049	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.904	165	131251	23.801	ng/u1	0.00
31) 4-Chloroaniline-d4	10.422	131	185330	23.665	ng/u1	0.00
46) Dimethylphthalate-d6	13.574	166	445293	23.663	ng/u1	0.00
49) Acenaphthylene-d8	13.839	160	529197	22.263	ng/u1	0.00
54) 4-Nitrophenol-d4	14.386	143	76400	23.329	ng/u1	0.00
60) Fluorene-d10	15.151	176	389100	23.482	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200	84173	21.490	ng/u1	0.00
73) Anthracene-d10	17.004	188	632717	22.227	ng/u1	0.00
81) Pyrene-d10	19.309	212	718494	18.541	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.115	264	873463	22.144	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.163	88	15920	7.486	ng/uL#	87
5) Pyridine	3.540	79	100998	17.175	ng/u1	94
6) Benzaldehyde	6.681	77	33942	9.366	ng/u1	97
8) Phenol	6.728	94	133452	18.487	ng/u1	95
10) Bis(2-Chloroethyl)ether	6.957	93	104951	18.665	ng/u1	92
12) 2-Chlorophenol	7.081	128	109277	20.188	ng/u1	94
13) 2-Methylphenol	7.957	108	103460	19.715	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.040	45	138988	15.011	ng/u1#	93
16) Acetophenone	8.334	105	184864	20.812	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.316	70	96920	21.966	ng/u1	95
18) 4-Methylphenol	8.287	108	115039	19.978	ng/u1	99
19) Hexachloroethane	8.557	117	46412	20.376	ng/u1	88
22) Nitrobenzene	8.704	77	141903	21.073	ng/u1	98
23) Isophorone	9.228	82	260833	22.195	ng/u1	97
25) 2-Nitrophenol	9.404	139	68628	22.338	ng/u1	96
26) 2,4-Dimethylphenol	9.469	107	139733	21.931	ng/u1	95
27) Bis(2-Chloroethoxy)met...	9.710	93	154041	20.713	ng/u1	99
29) 2,4-Dichlorophenol	9.928	162	125710	23.503	ng/u1	96
30) Naphthalene	10.316	128	379484	21.431	ng/u1	99
32) 4-Chloroaniline	10.445	127	185515	23.613	ng/u1	98
33) Hexachlorobutadiene	10.592	225	82382	22.658	ng/u1	98
34) Caprolactam	11.239	113	19818	12.809	ng/u1	86
35) 4-Chloro-3-methylphenol	11.575	107	133124	24.559	ng/u1	98
36) 2-Methylnaphthalene	11.939	142	299351	23.711	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031935.D
 Acq On : 28 Aug 2021 16:53
 Operator : CG/JU
 Sample : SSTD02020
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 28 23:55:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.163	142	306034	23.912	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.316	216	167245	20.512	ng/ul	99
40) Hexachlorocyclopentadiene	12.280	237	79135	15.967	ng/ul	99
41) 2,4,6-Trichlorophenol	12.569	196	112571	21.885	ng/ul	97
42) 2,4,5-Trichlorophenol	12.645	196	123909	22.727	ng/ul	99
43) 1,1'-Biphenyl	12.975	154	409883	20.928	ng/ul	95
44) 2-Chloronaphthalene	13.010	162	321734	20.990	ng/ul	99
45) 2-Nitroaniline	13.239	65	93483	21.705	ng/ul	100
47) Dimethylphthalate	13.627	163	434705	23.580	ng/ul	100
48) 2,6-Dinitrotoluene	13.751	165	88738	24.992	ng/ul	96
50) Acenaphthylene	13.869	152	487250	21.942	ng/ul	97
51) 3-Nitroaniline	14.080	138	63183	17.032	ng/ul	99
52) Acenaphthene	14.216	153	348982	21.543	ng/ul	97
53) 2,4-Dinitrophenol	14.298	184	52309	24.723	ng/ul	95
55) 4-Nitrophenol	14.404	109	71286	25.646	ng/ul	84
56) Dibenzofuran	14.557	168	514762	22.567	ng/ul	99
57) 2,4-Dinitrotoluene	14.545	165	131319	26.528	ng/ul#	82
58) 2,3,4,6-Tetrachlorophenol	14.786	232	112490	24.814	ng/ul	99
59) Diethylphthalate	15.004	149	449687	24.577	ng/ul	98
61) Fluorene	15.210	166	436458	23.231	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.210	204	223046	23.589	ng/ul	100
63) 4-Nitroaniline	15.257	138	48292	13.666	ng/ul#	86
66) 4,6-Dinitro-2-methylph...	15.310	198	82426	21.798	ng/ul	98
67) N-Nitrosodiphenylamine	15.433	169	385737	21.182	ng/ul	98
68) 4-Bromophenyl-phenylether	16.104	248	135065	20.994	ng/ul	95
69) Hexachlorobenzene	16.210	284	155761	21.333	ng/ul	98
70) Atrazine	16.398	200	139898	21.570	ng/ul	97
71) Pentachlorophenol	16.563	266	92316	20.806	ng/ul	97
72) Phenanthrene	16.951	178	721600	22.138	ng/ul	100
74) Anthracene	17.039	178	740158	22.101	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	12.933	216	169875	17.938	ng/uL	98
76) Pentachlorobenzene	14.469	250	179701	19.392	ng/uL	98
77) Carbazole	17.321	167	659158	22.642	ng/ul	100
78) Di-n-butylphthalate	17.892	149	797551	23.771	ng/ul	99
80) Fluoranthene	18.974	202	883572	18.491	ng/ul#	95
82) Pyrene	19.339	202	920474	18.587	ng/ul	96
83) Butylbenzylphthalate	20.262	149	378930	22.384	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.039	252	311707	24.311	ng/ul	97
85) Benzo(a)anthracene	21.098	228	961259	21.881	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.045	149	612173	24.530	ng/ul#	97
87) Chrysene	21.145	228	922592	21.344	ng/ul	100
89) Di-n-octyl phthalate	21.897	149	1076812	22.690	ng/ul	100
90) Benzo(b)fluoranthene	22.615	252	1034384	21.013	ng/ul	98
91) Benzo(k)fluoranthene	22.656	252	1049249	21.929	ng/ul	98
93) Benzo(a)pyrene	23.156	252	951901	21.852	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	25.356	276	1204177	22.227	ng/ul	95
95) Dibenzo(a,h)anthracene	25.362	278	1006372	22.155	ng/ul	97
96) Benzo(g,h,i)perylene	25.997	276	993756	22.879	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031935.D
 Acq On : 28 Aug 2021 16:53
 Operator : CG/JU
 Sample : SST02020
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 28 23:55:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration




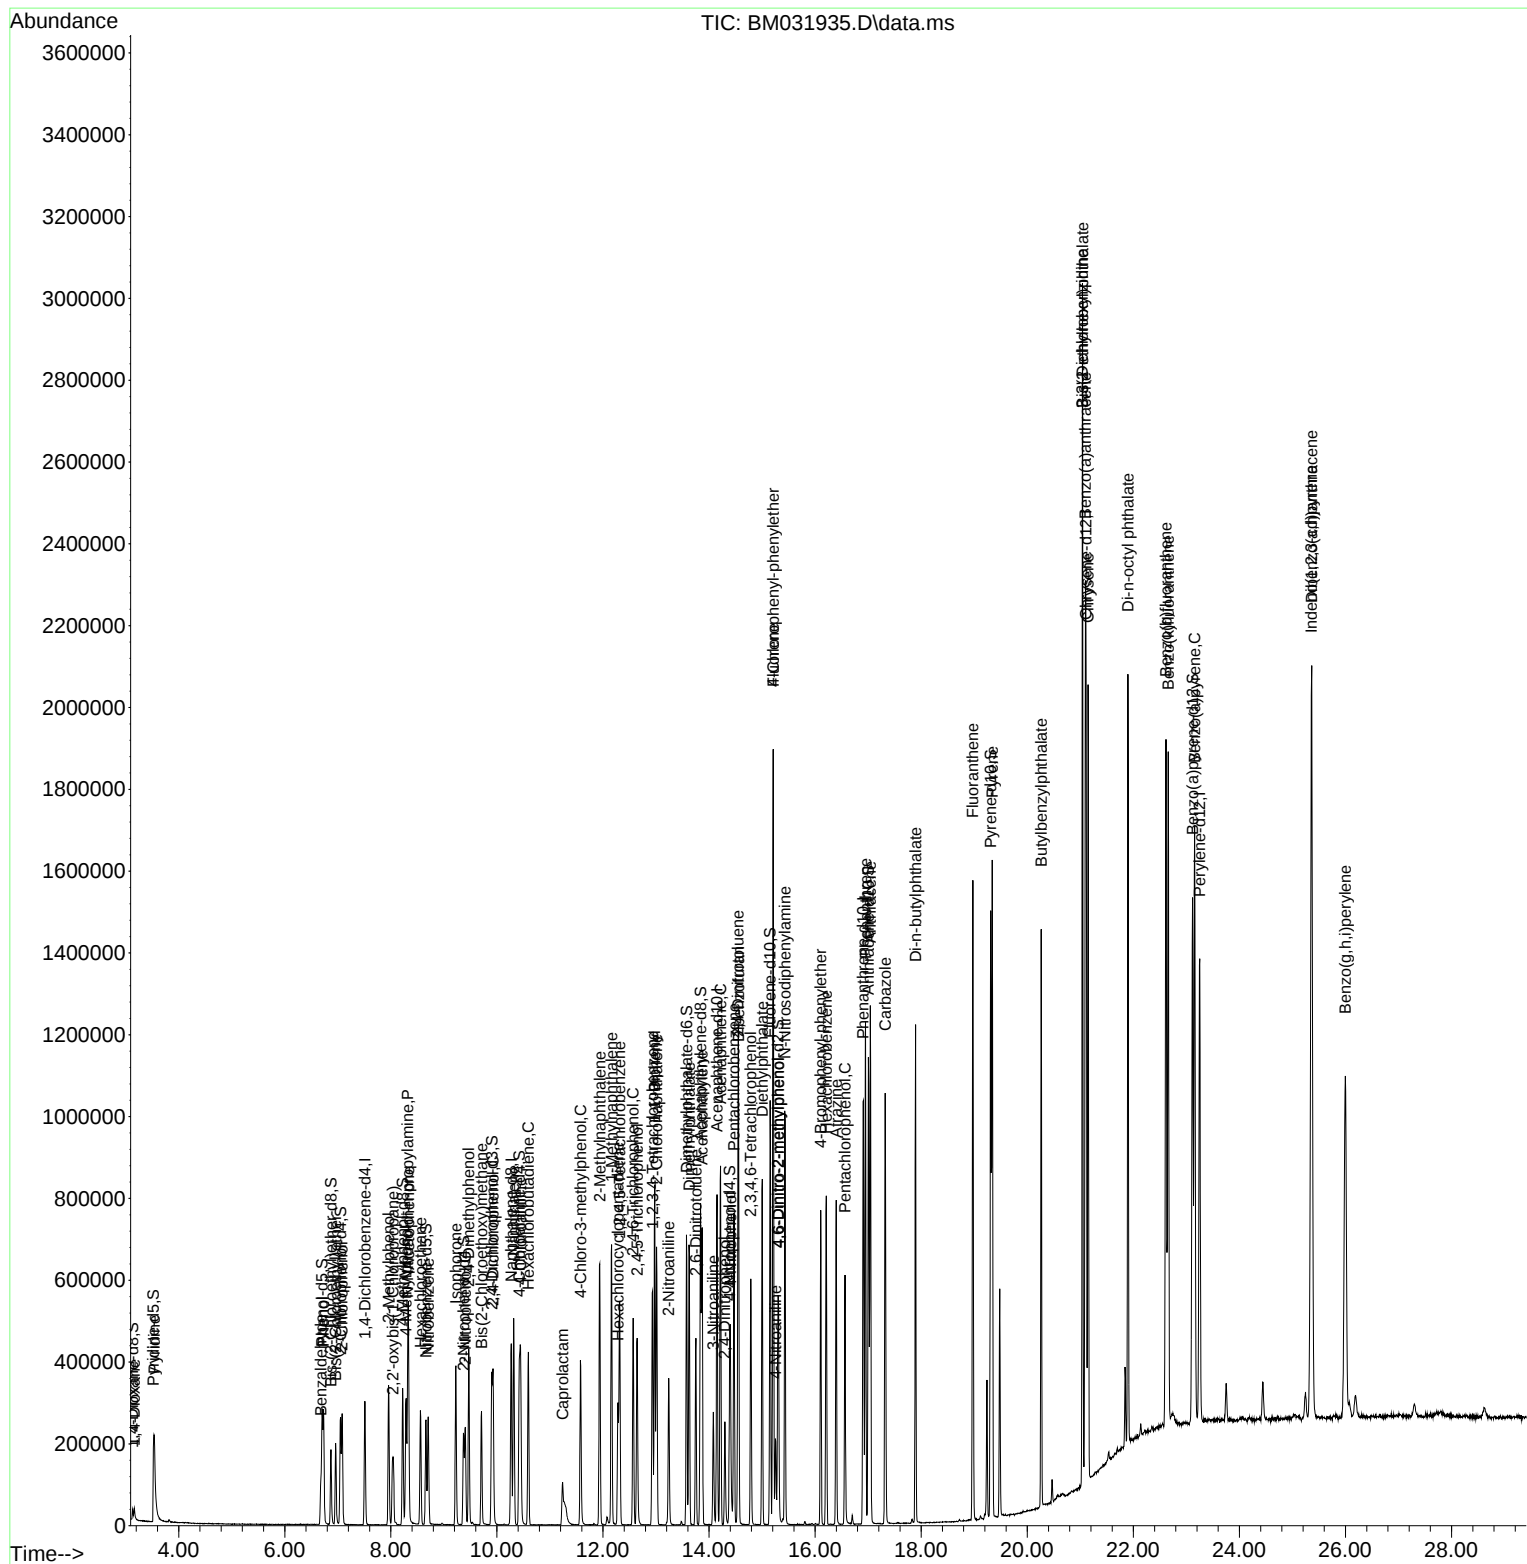




#2
1,4-Dioxane
Concen: 7.486 ng/uL
RT: 3.163 min Scan# 13
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion: 88 Resp: 15920
Ion Ratio Lower Upper
88 100
43 30.0 31.5 47.3#
58 69.5 64.1 96.1



#5
Pyridine
Concen: 17.175 ng/uL
RT: 3.540 min Scan# 77
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion: 79 Resp: 100998
Ion Ratio Lower Upper
79 100
52 81.3 69.9 104.9
51 38.6 33.8 50.6









#6
Benzaldehyde
Concen: 9.366 ng/ul
RT: 6.681 min Scan# 611
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:	77	Resp:	33942
Ion	Ratio	Lower	Upper
77	100		
105	96.9	82.2	123.4
106	93.5	75.0	112.4



#8
Phenol
Concen: 18.487 ng/ul
RT: 6.728 min Scan# 619
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:	94	Resp:	133452
Ion	Ratio	Lower	Upper
94	100		
65	29.7	24.2	36.4
66	44.3	31.4	47.0









#10
 Bis(2-Chloroethyl)ether
 Concen: 18.665 ng/ul
 RT: 6.957 min Scan# 658
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53




Instrument :
 BNA_M
 ClientSampled :


Tgt Ion: 93 Resp: 104951
 Ion Ratio Lower Upper
 93 100
 63 74.7 68.0 102.0
 95 32.1 25.8 38.6

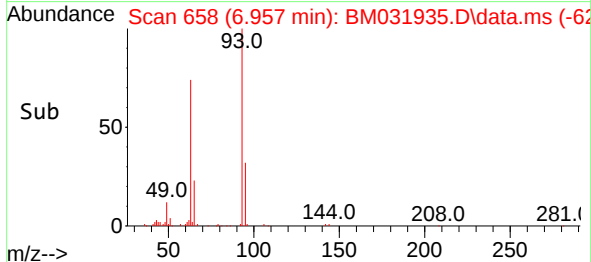

#12
 2-Chlorophenol
 Concen: 20.188 ng/ul
 RT: 7.081 min Scan# 679
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53

Tgt Ion:128 Resp: 109277
 Ion Ratio Lower Upper
 128 100
 64 44.3 39.2 58.8
 130 34.3 25.3 37.9









#13
2-Methylphenol
Concen: 19.715 ng/ul
RT: 7.957 min Scan# 828
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:108 Resp: 103460
Ion Ratio Lower Upper
108 100
107 89.1 70.6 105.8



#14
2,2'-oxybis(1-Chloropropane)
Concen: 15.011 ng/ul
RT: 8.040 min Scan# 842
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion: 45 Resp: 138988
Ion Ratio Lower Upper
45 100
77 15.7 10.2 15.4#
79 12.7 7.8 11.8#









#16
Acetophenone
Concen: 20.812 ng/ul
RT: 8.334 min Scan# 892
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
105	100		
77	78.3	63.7	95.5
51	28.9	25.4	38.0



#17
N-Nitroso-di-n-propylamine
Concen: 21.966 ng/ul
RT: 8.316 min Scan# 889
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion	Ratio	Lower	Upper
70	100		
42	61.6	53.4	80.0
101	9.5	7.4	11.0
130	21.9	16.8	25.2









#18
4-Methylphenol
Concen: 19.978 ng/ul
RT: 8.287 min Scan# 884
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:108 Resp: 115039
Ion Ratio Lower Upper
108 100
107 109.8 87.0 130.6

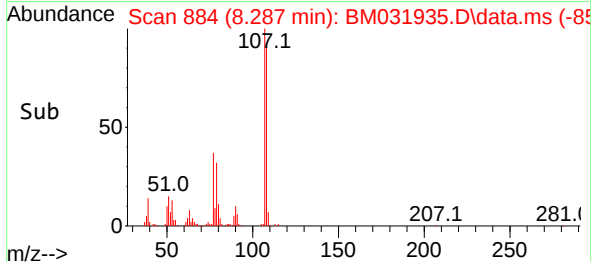

#19
Hexachloroethane
Concen: 20.376 ng/ul
RT: 8.557 min Scan# 930
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:117 Resp: 46412
Ion Ratio Lower Upper
117 100
201 113.5 80.1 120.1
199 71.9 50.8 76.2









#22
Nitrobenzene
Concen: 21.073 ng/ul
RT: 8.704 min Scan# 955
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion: 77 Resp: 141903
Ion Ratio Lower Upper
77 100
123 45.0 34.8 52.2
65 13.3 10.4 15.6

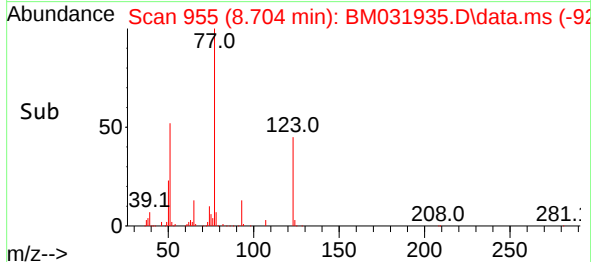

#23
Isophorone
Concen: 22.195 ng/ul
RT: 9.228 min Scan# 1044
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion: 82 Resp: 260833
Ion Ratio Lower Upper
82 100
95 7.5 5.3 7.9
138 18.2 13.6 20.4









#25
2-Nitrophenol
Concen: 22.338 ng/ul
RT: 9.404 min Scan# 1074
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:139 Resp: 68628
Ion Ratio Lower Upper
139 100
65 52.8 43.7 65.5
109 34.1 24.0 36.0



#26
2,4-Dimethylphenol
Concen: 21.931 ng/ul
RT: 9.469 min Scan# 1085
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:107 Resp: 139733
Ion Ratio Lower Upper
107 100
121 48.3 41.0 61.6
122 80.1 68.2 102.2






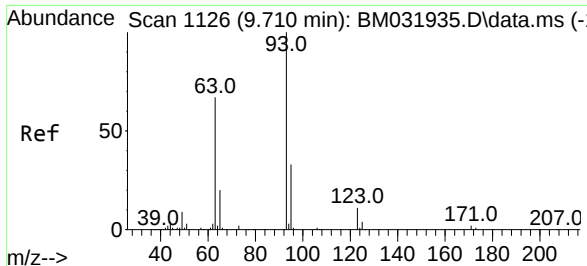


#27

Bis(2-Chloroethoxy)methane
Concen: 20.713 ng/ul
RT: 9.710 min Scan# 1126
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Instrument :
BNA_M
ClientSampled :




Tgt Ion:	93	Resp:	154041
Ion	Ratio	Lower	Upper
93	100		
95	32.5	25.9	38.9
123	11.3	8.5	12.7

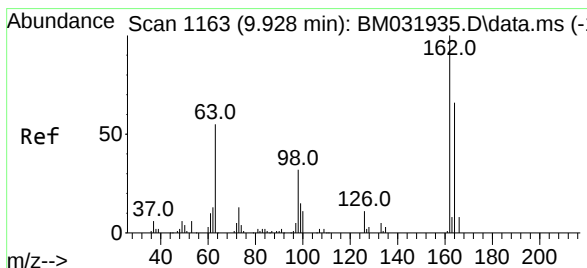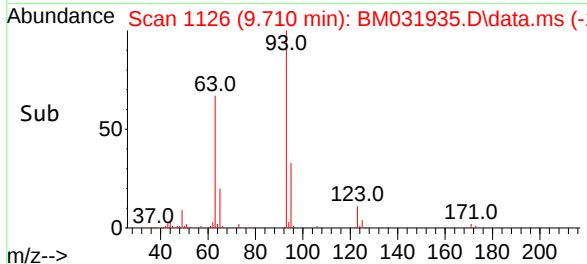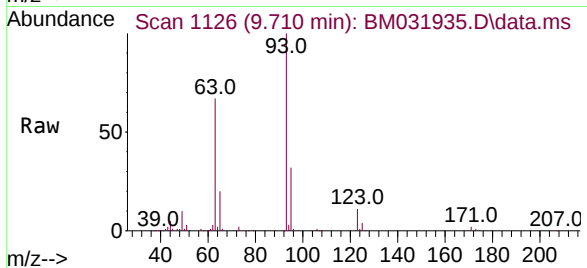


#29

2,4-Dichlorophenol
Concen: 23.503 ng/ul
RT: 9.928 min Scan# 1163
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:	162	Resp:	125710
Ion	Ratio	Lower	Upper
162	100		
164	67.1	51.6	77.4
98	31.9	28.2	42.4


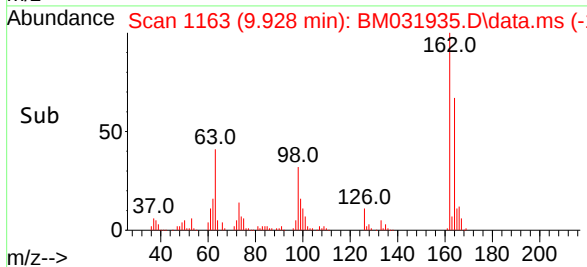

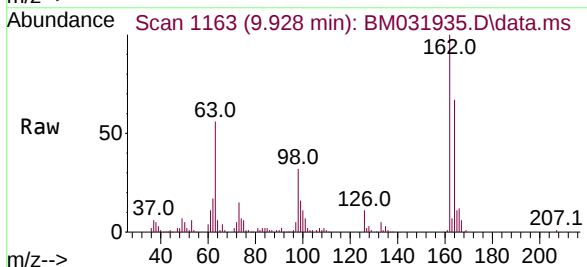




#30
Naphthalene
Concen: 21.431 ng/ul
RT: 10.316 min Scan# 1229
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:128 Resp: 379484
Ion Ratio Lower Upper
128 100
129 10.8 9.0 13.4
127 12.8 10.6 15.8

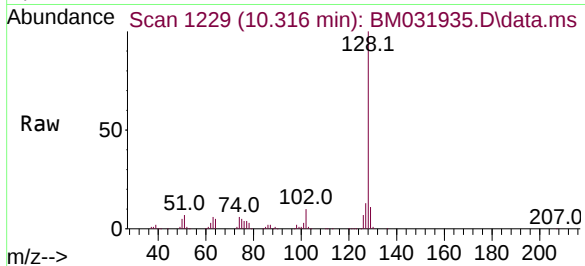

#32
4-Chloroaniline
Concen: 23.613 ng/ul
RT: 10.445 min Scan# 1251
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:127 Resp: 185515
Ion Ratio Lower Upper
127 100
129 32.8 25.6 38.4




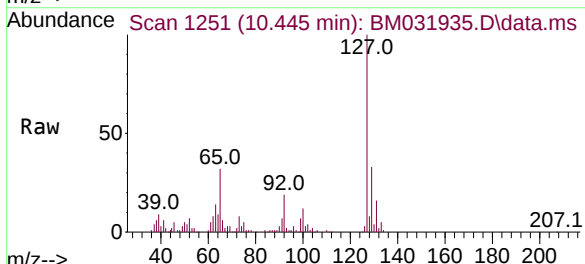




#33
Hexachlorobutadiene
Concen: 22.658 ng/ul
RT: 10.592 min Scan# 1276
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:225 Resp: 82382
Ion Ratio Lower Upper
225 100
223 60.6 50.7 76.1
227 63.0 50.7 76.1

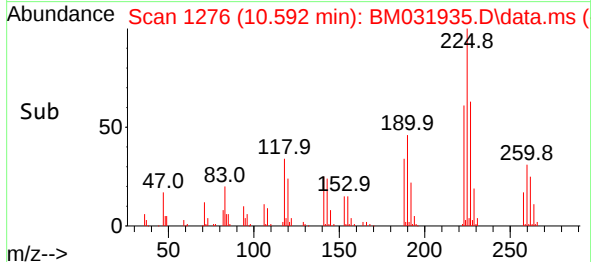

#34
Caprolactam
Concen: 12.809 ng/ul
RT: 11.239 min Scan# 1386
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:113 Resp: 19818
Ion Ratio Lower Upper
113 100
55 161.3 155.2 232.8
56 126.3 101.9 152.9









#35
4-Chloro-3-methylphenol
Concen: 24.559 ng/ul
RT: 11.575 min Scan# 1443
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:	107	Resp:	133124
Ion Ratio	Lower	Upper	
107	100		
144	28.2	22.3	33.5
142	84.3	65.6	98.4

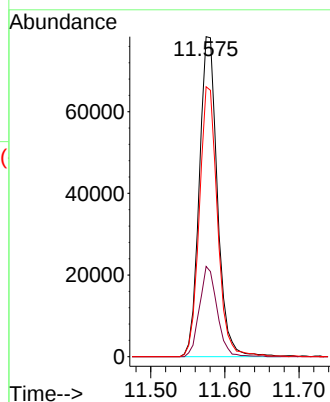

#36
2-Methylnaphthalene
Concen: 23.711 ng/ul
RT: 11.939 min Scan# 1505
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:	142	Resp:	299351
Ion Ratio	Lower	Upper	
142	100		
141	90.4	70.6	105.8









#37
1-Methylnaphthalene
Concen: 23.912 ng/ul
RT: 12.163 min Scan# 1543
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:142 Resp: 306034
Ion Ratio Lower Upper
142 100
141 91.6 72.8 109.2
116 4.0 3.1 4.7

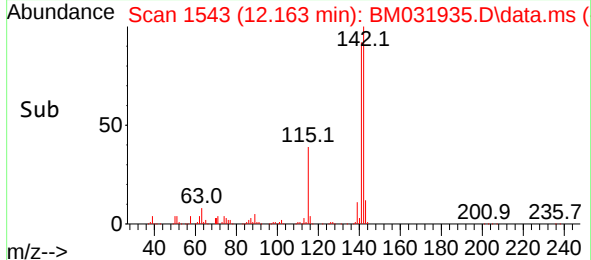

#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.512 ng/ul
RT: 12.316 min Scan# 1569
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:216 Resp: 167245
Ion Ratio Lower Upper
216 100
214 77.5 62.2 93.4
179 21.3 16.6 24.8
108 15.8 13.5 20.3



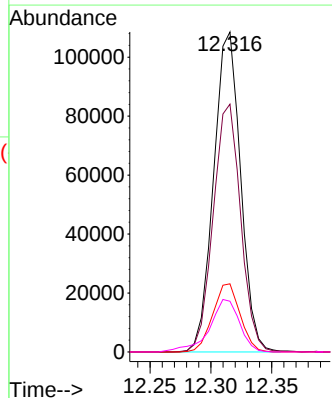





#40
Hexachlorocyclopentadiene
Concen: 15.967 ng/ul
RT: 12.280 min Scan# 1563
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion	Ratio	Lower	Upper
237	100		
235	61.2	49.0	73.4
272	11.8	11.0	16.4



#41
2,4,6-Trichlorophenol
Concen: 21.885 ng/ul
RT: 12.569 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion	Ratio	Lower	Upper
196	100		
198	95.5	78.8	118.2
200	31.6	26.0	39.0









#42
2,4,5-Trichlorophenol
Concen: 22.727 ng/ul
RT: 12.645 min Scan# 1625
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:196 Resp: 123909
Ion Ratio Lower Upper
196 100
198 95.7 76.1 114.1
200 30.8 25.4 38.2



#43
1,1'-Biphenyl
Concen: 20.928 ng/ul
RT: 12.975 min Scan# 1681
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:154 Resp: 409883
Ion Ratio Lower Upper
154 100
153 37.7 32.3 48.5
76 10.6 10.6 15.8









#44
2-Chloronaphthalene
Concen: 20.990 ng/ul
RT: 13.010 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:162 Resp: 321734
Ion Ratio Lower Upper
162 100
164 33.6 26.2 39.4
127 36.2 29.4 44.0

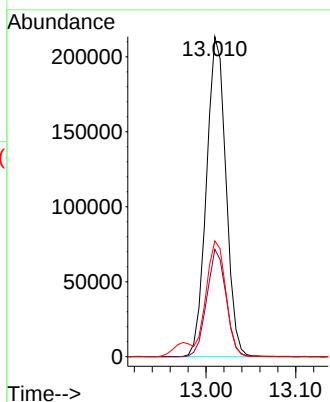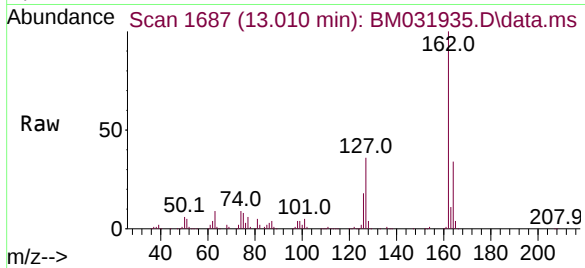

#45
2-Nitroaniline
Concen: 21.705 ng/ul
RT: 13.239 min Scan# 1726
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53


Tgt Ion: 65 Resp: 93483
Ion Ratio Lower Upper
65 100
92 67.0 53.9 80.9
138 104.5 83.3 124.9

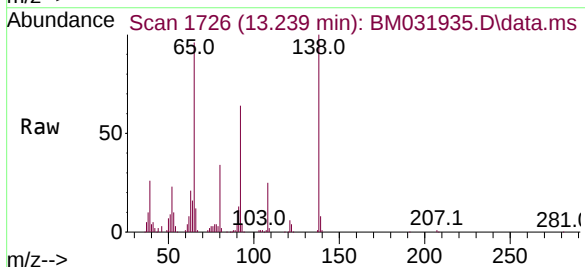






#47
Dimethylphthalate
Concen: 23.580 ng/ul
RT: 13.627 min Scan# 1792
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53


Instrument :
BNA_M
ClientSampled :





Tgt Ion:163 Resp: 434705
Ion Ratio Lower Upper
163 100
194 4.2 3.2 4.8
164 10.2 8.2 12.4

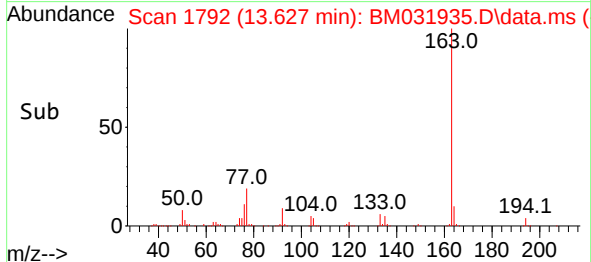


#48
2,6-Dinitrotoluene
Concen: 24.992 ng/ul
RT: 13.751 min Scan# 1813
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53



Tgt Ion:165 Resp: 88738
Ion Ratio Lower Upper
165 100
89 58.2 48.6 72.8
121 19.6 18.1 27.1









#50
Acenaphthylene
Concen: 21.942 ng/ul
RT: 13.869 min Scan# 1833
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:152 Resp: 487250
Ion Ratio Lower Upper
152 100
151 18.0 16.2 24.2
153 12.7 10.2 15.4



#51
3-Nitroaniline
Concen: 17.032 ng/ul
RT: 14.080 min Scan# 1869
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53


Tgt Ion:138 Resp: 63183
Ion Ratio Lower Upper
138 100
108 10.4 7.4 11.2
92 119.4 96.5 144.7








#52
Acenaphthene
Concen: 21.543 ng/ul
RT: 14.216 min Scan# 1892
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53


Instrument :
BNA_M
ClientSampled :





Tgt Ion:153 Resp: 348982
Ion Ratio Lower Upper
153 100
152 46.5 37.4 56.2
154 90.7 69.4 104.0




#53
2,4-Dinitrophenol
Concen: 24.723 ng/ul
RT: 14.298 min Scan# 1906
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53



Tgt Ion:184 Resp: 52309
Ion Ratio Lower Upper
184 100
63 68.0 56.9 85.3
154 67.0 49.0 73.6









#55
4-Nitrophenol
Concen: 25.646 ng/ul
RT: 14.404 min Scan# 1924
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:109 Resp: 71286
Ion Ratio Lower Upper
109 100
139 107.3 100.3 150.5
65 111.3 104.6 156.8

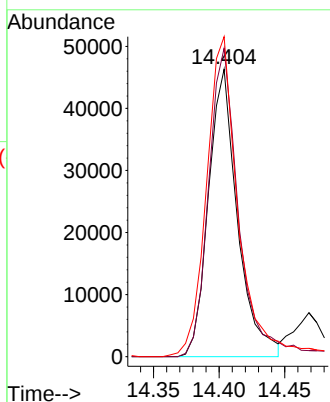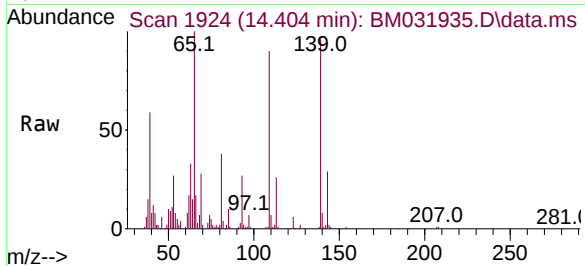

#56
Dibenzofuran
Concen: 22.567 ng/ul
RT: 14.557 min Scan# 1950
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:168 Resp: 514762
Ion Ratio Lower Upper
168 100
139 37.6 29.5 44.3




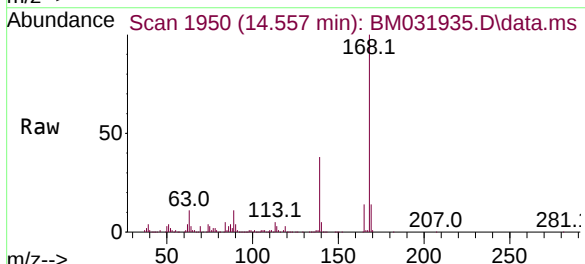




#57
2,4-Dinitrotoluene
Concen: 26.528 ng/ul
RT: 14.545 min Scan# 1948
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:165 Resp: 131319
Ion Ratio Lower Upper
165 100
63 59.7 37.6 56.4#
182 2.9 1.8 2.8#

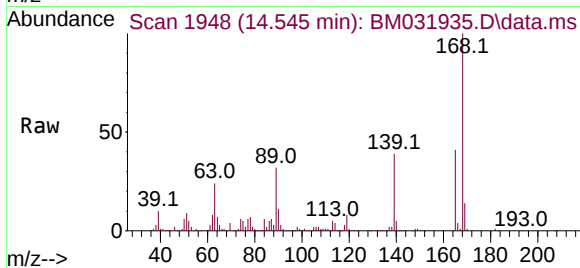

#58
2,3,4,6-Tetrachlorophenol
Concen: 24.814 ng/ul
RT: 14.786 min Scan# 1989
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:232 Resp: 112490
Ion Ratio Lower Upper
232 100
131 43.5 35.0 52.6
130 2.0 1.7 2.5
166 30.2 24.4 36.6




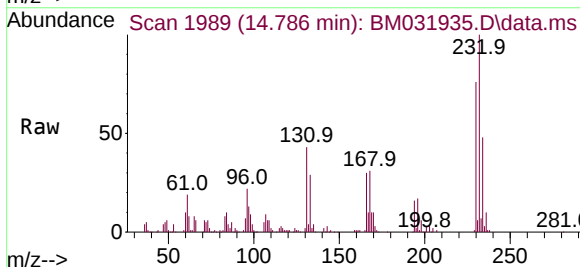




#59
Diethylphthalate
Concen: 24.577 ng/ul
RT: 15.004 min Scan# 2026
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:149 Resp: 449687
Ion Ratio Lower Upper
149 100
177 22.4 17.0 25.4
150 12.6 9.9 14.9

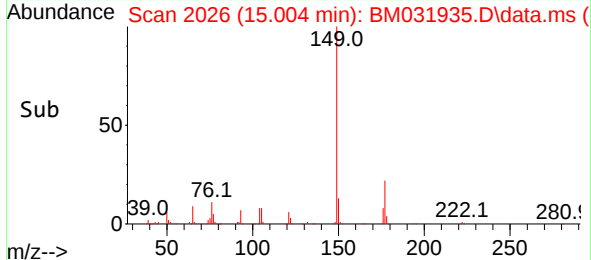

#61
Fluorene
Concen: 23.231 ng/ul
RT: 15.210 min Scan# 2061
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:166 Resp: 436458
Ion Ratio Lower Upper
166 100
165 95.1 78.4 117.6
167 13.3 10.6 15.8









#62
4-Chlorophenyl-phenylether
Concen: 23.589 ng/ul
RT: 15.210 min Scan# 2061
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:204 Resp: 223046
Ion Ratio Lower Upper
204 100
206 32.5 26.0 39.0
141 57.2 45.6 68.4

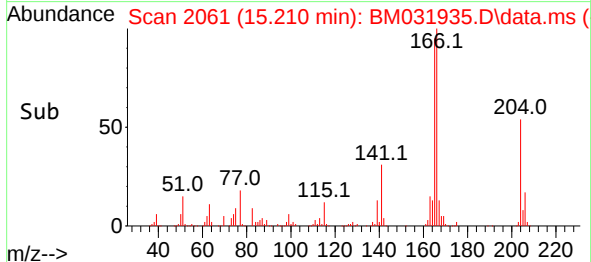

#63
4-Nitroaniline
Concen: 13.666 ng/ul
RT: 15.257 min Scan# 2069
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:138 Resp: 48292
Ion Ratio Lower Upper
138 100
92 51.3 41.5 62.3
108 95.8 61.4 92.2#









#66
 4,6-Dinitro-2-methylphenol
 Concen: 21.798 ng/ul
 RT: 15.310 min Scan# 2078
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53




Instrument :
 BNA_M
 ClientSampled :


Tgt Ion:198 Resp: 82426
 Ion Ratio Lower Upper
 198 100
 182 4.6 3.8 5.6
 77 26.3 20.1 30.1

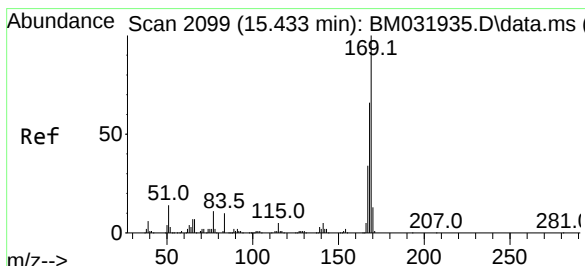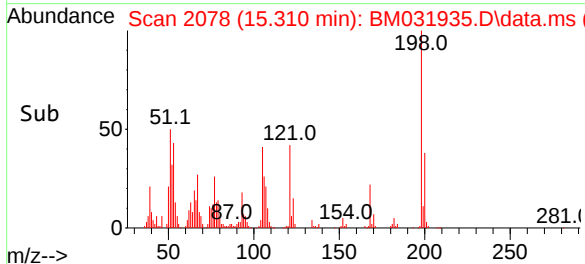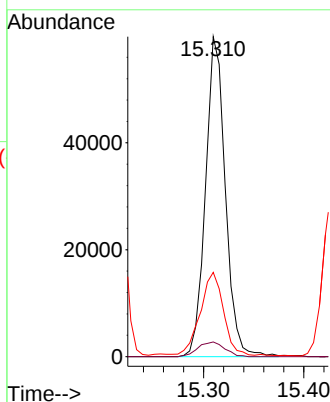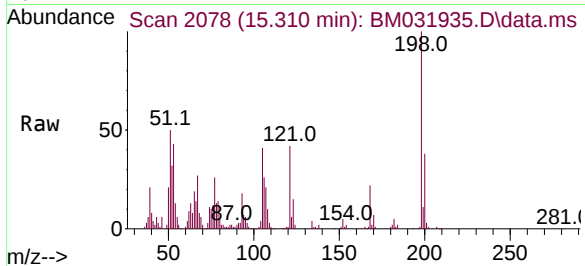

#67
 N-Nitrosodiphenylamine
 Concen: 21.182 ng/ul
 RT: 15.433 min Scan# 2099
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53

Tgt Ion:169 Resp: 385737
 Ion Ratio Lower Upper
 169 100
 168 65.8 53.8 80.6
 167 34.1 28.6 43.0


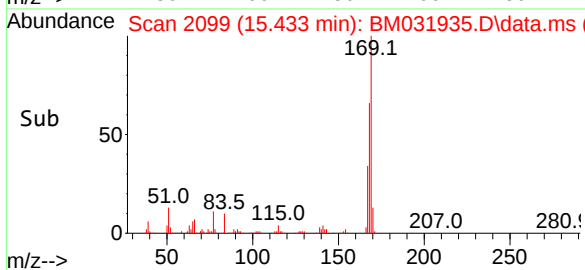

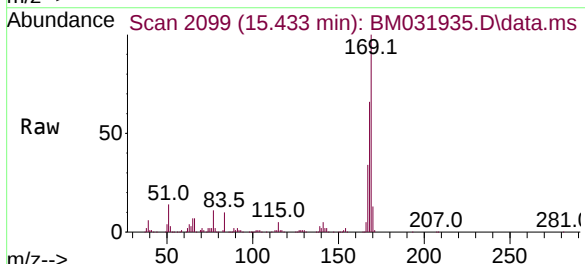




#68
4-Bromophenyl-phenylether
Concen: 20.994 ng/ul
RT: 16.104 min Scan# 2213
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:248	Resp: 135065
Ion Ratio	Lower Upper
248 100	
250 96.3	78.6 118.0
141 78.1	56.2 84.2

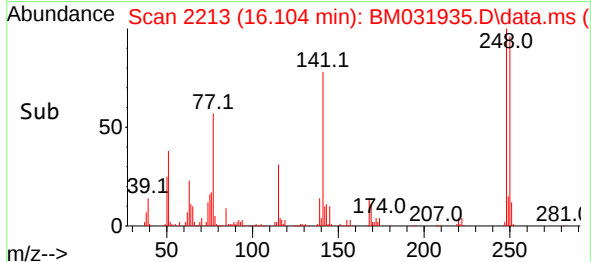

#69
Hexachlorobenzene
Concen: 21.333 ng/ul
RT: 16.210 min Scan# 2231
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:284	Resp: 155761
Ion Ratio	Lower Upper
284 100	
142 35.3	29.0 43.4
249 30.4	25.0 37.4









#70
Atrazine
Concen: 21.570 ng/ul
RT: 16.398 min Scan# 2263
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:200 Resp: 139898
Ion Ratio Lower Upper
200 100
173 25.9 18.7 28.1
215 47.7 38.9 58.3

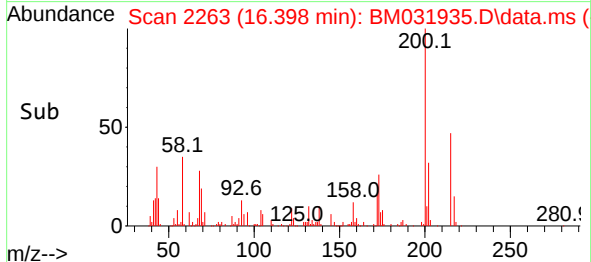

#71
Pentachlorophenol
Concen: 20.806 ng/ul
RT: 16.563 min Scan# 2291
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:266 Resp: 92316
Ion Ratio Lower Upper
266 100
264 62.5 48.2 72.4
268 62.6 51.6 77.4









#72
Phenanthrene
Concen: 22.138 ng/ul
RT: 16.951 min Scan# 2357
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:178 Resp: 721600
Ion Ratio Lower Upper
178 100
179 15.1 12.1 18.1
176 18.6 15.2 22.8



#74
Anthracene
Concen: 22.101 ng/ul
RT: 17.039 min Scan# 2372
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:178 Resp: 740158
Ion Ratio Lower Upper
178 100
179 15.2 12.1 18.1
176 18.2 15.2 22.8









#75
1,2,3,4-Tetrachlorobenzene
Concen: 17.938 ng/uL
RT: 12.933 min Scan# 1674
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:	216	Resp:	169875
Ion Ratio	Lower	Upper	
216	100		
214	79.2	61.9	92.9
218	47.5	39.5	59.3



#76
Pentachlorobenzene
Concen: 19.392 ng/uL
RT: 14.469 min Scan# 1935
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:	250	Resp:	179701
Ion Ratio	Lower	Upper	
250	100		
248	62.3	50.2	75.4
252	62.0	52.2	78.2









#77
 Carbazole
 Concen: 22.642 ng/ul
 RT: 17.321 min Scan# 2420
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53




Instrument :
 BNA_M
 ClientSampled :


Tgt Ion:	167	Resp:	659158
Ion	Ratio	Lower	Upper
167	100		
166	21.3	17.0	25.6
139	12.0	9.9	14.9



#78
 Di-n-butylphthalate
 Concen: 23.771 ng/ul
 RT: 17.892 min Scan# 2517
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53

Tgt Ion:	149	Resp:	797551
Ion	Ratio	Lower	Upper
149	100		
150	8.8	7.3	10.9
104	5.5	4.1	6.1









#80
 Fluoranthene
 Concen: 18.491 ng/u1
 RT: 18.974 min Scan# 2701
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53




Instrument :
 BNA_M
 ClientSampled :


Tgt Ion:202 Resp: 883572
 Ion Ratio Lower Upper
 202 100
 101 8.6 8.8 13.2#
 100 6.9 6.8 10.2



#82
 Pyrene
 Concen: 18.587 ng/u1
 RT: 19.339 min Scan# 2763
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53

Tgt Ion:202 Resp: 920474
 Ion Ratio Lower Upper
 202 100
 101 10.9 10.0 15.0
 100 9.0 8.5 12.7









#83
Butylbenzylphthalate
Concen: 22.384 ng/ul
RT: 20.262 min Scan# 2920
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:149 Resp: 378930
Ion Ratio Lower Upper
149 100
91 72.9 57.4 86.2
206 20.5 15.9 23.9

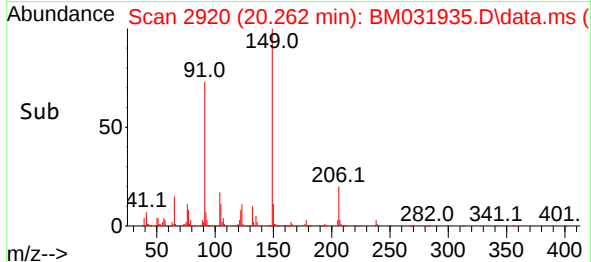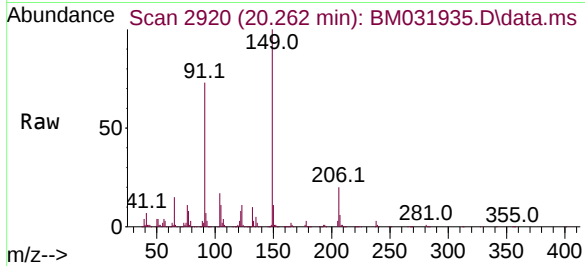

#84
3,3'-Dichlorobenzidine
Concen: 24.311 ng/ul
RT: 21.039 min Scan# 3052
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:252 Resp: 311707
Ion Ratio Lower Upper
252 100
254 64.5 49.9 74.9
126 10.3 8.9 13.3




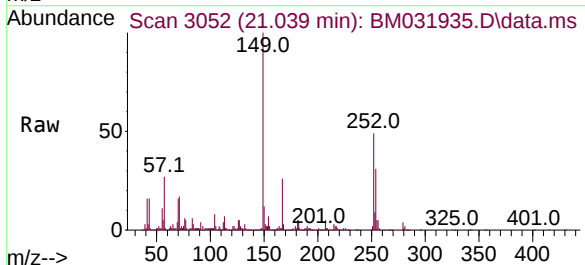




#85
Benzo(a)anthracene
Concen: 21.881 ng/ul
RT: 21.098 min Scan# 3062
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:228 Resp: 961259
Ion Ratio Lower Upper
228 100
229 19.1 16.0 24.0
226 26.2 22.2 33.2



#86
Bis(2-ethylhexyl)phthalate
Concen: 24.530 ng/ul
RT: 21.045 min Scan# 3053
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:149 Resp: 612173
Ion Ratio Lower Upper
149 100
167 27.2 20.7 31.1
279 4.8 3.0 4.4#









#87
Chrysene
Concen: 21.344 ng/ul
RT: 21.145 min Scan# 3070
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:228 Resp: 922592
Ion Ratio Lower Upper
228 100
226 29.4 23.6 35.4
229 19.6 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 22.690 ng/ul
RT: 21.897 min Scan# 3198
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:149 Resp: 1076812









#90
Benzo(b)fluoranthene
Concen: 21.013 ng/ul
RT: 22.615 min Scan# 3320
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:252 Resp: 1034384
Ion Ratio Lower Upper
252 100
253 22.9 17.8 26.6
125 8.3 7.7 11.5



#91
Benzo(k)fluoranthene
Concen: 21.929 ng/ul
RT: 22.656 min Scan# 3327
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:252 Resp: 1049249
Ion Ratio Lower Upper
252 100
253 21.5 17.4 26.2
125 8.2 7.9 11.9









#93
Benzo(a)pyrene
Concen: 21.852 ng/ul
RT: 23.156 min Scan# 3412
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53




Instrument :
BNA_M
ClientSampled :


Tgt Ion:252 Resp: 951901
Ion Ratio Lower Upper
252 100
253 21.7 17.5 26.3
125 8.7 8.6 13.0



#94
Indeno(1,2,3-cd)pyrene
Concen: 22.227 ng/ul
RT: 25.356 min Scan# 3786
Delta R.T. 0.000 min
Lab File: BM031935.D
Acq: 28 Aug 2021 16:53

Tgt Ion:276 Resp: 1204177
Ion Ratio Lower Upper
276 100
138 20.3 19.5 29.3
277 25.3 19.6 29.4









#95
 Dibenzo(a,h)anthracene
 Concen: 22.155 ng/ul
 RT: 25.362 min Scan# 3787
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53

Instrument :
 BNA_M
 ClientSampled :

Tgt Ion:278 Resp: 1006372

Ion	Ratio	Lower	Upper
278	100		
139	12.8	12.8	19.2
279	23.6	19.1	28.7

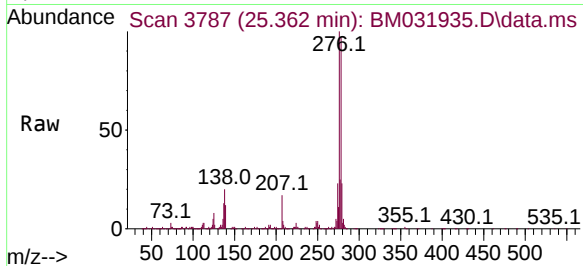

#96
 Benzo(g,h,i)perylene
 Concen: 22.879 ng/ul
 RT: 25.997 min Scan# 3895
 Delta R.T. 0.000 min
 Lab File: BM031935.D
 Acq: 28 Aug 2021 16:53

Tgt Ion:276 Resp: 993756

Ion	Ratio	Lower	Upper
276	100		
138	16.5	16.5	24.7
277	23.3	18.5	27.7

