

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031938.D
 Acq On : 28 Aug 2021 18:42
 Operator : CG/JU
 Sample : SSTD16023
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160020

Manual Integrations
 APPROVED

mohammad
 8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

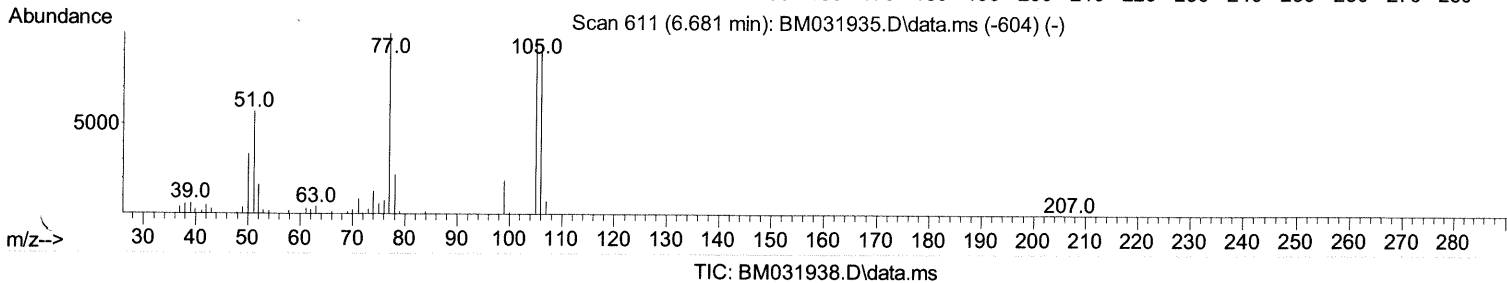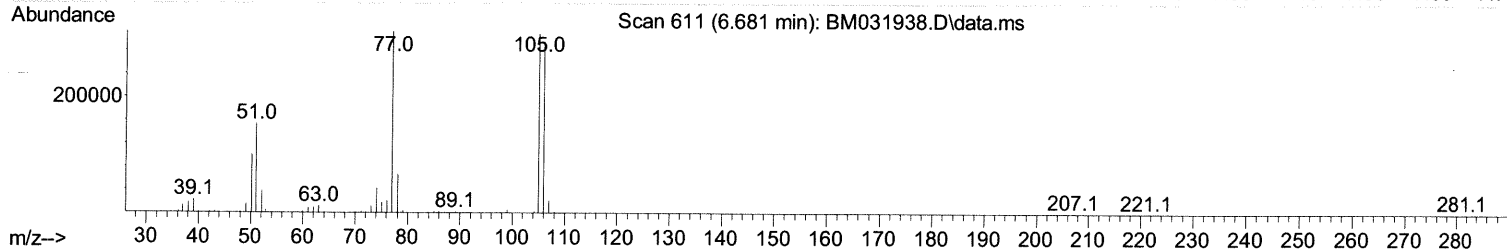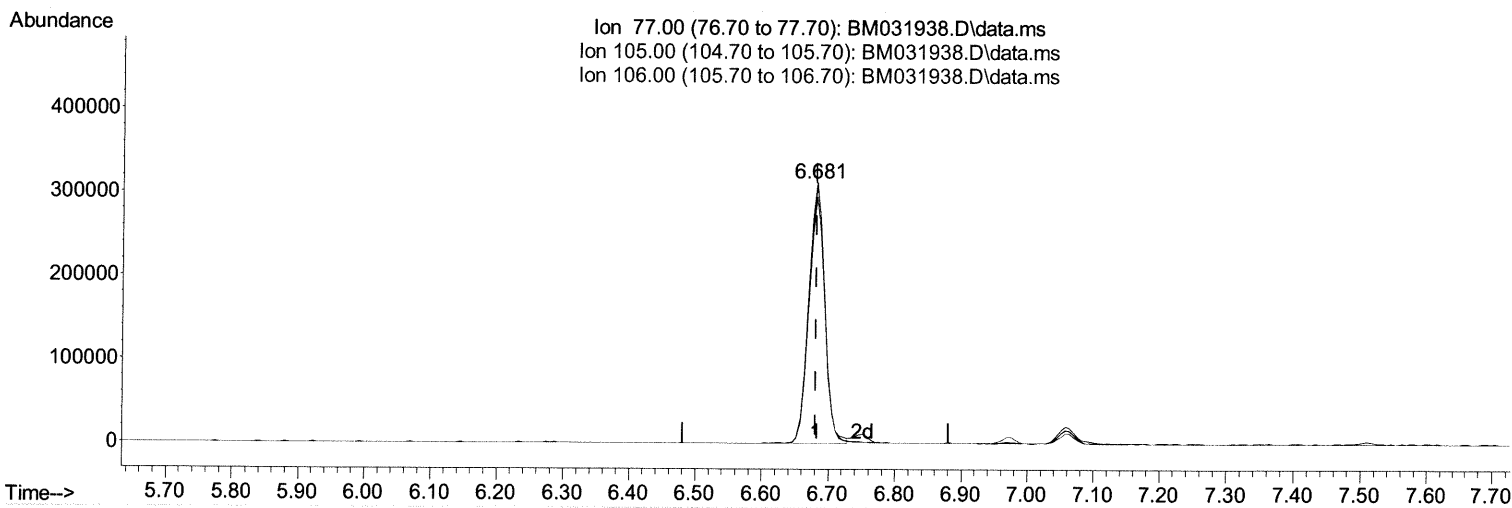

(6) Benzaldehyde

6.681min (+ 0.000) 117.98 ng/ul

response 523535

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	102.80	98.93
106.00	93.70	94.55
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031938.D
 Acq On : 28 Aug 2021 18:42
 Operator : CG/JU
 Sample : SSTD16023
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SSTD160020

Manual Integrations
APPROVED

mohammad
 8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

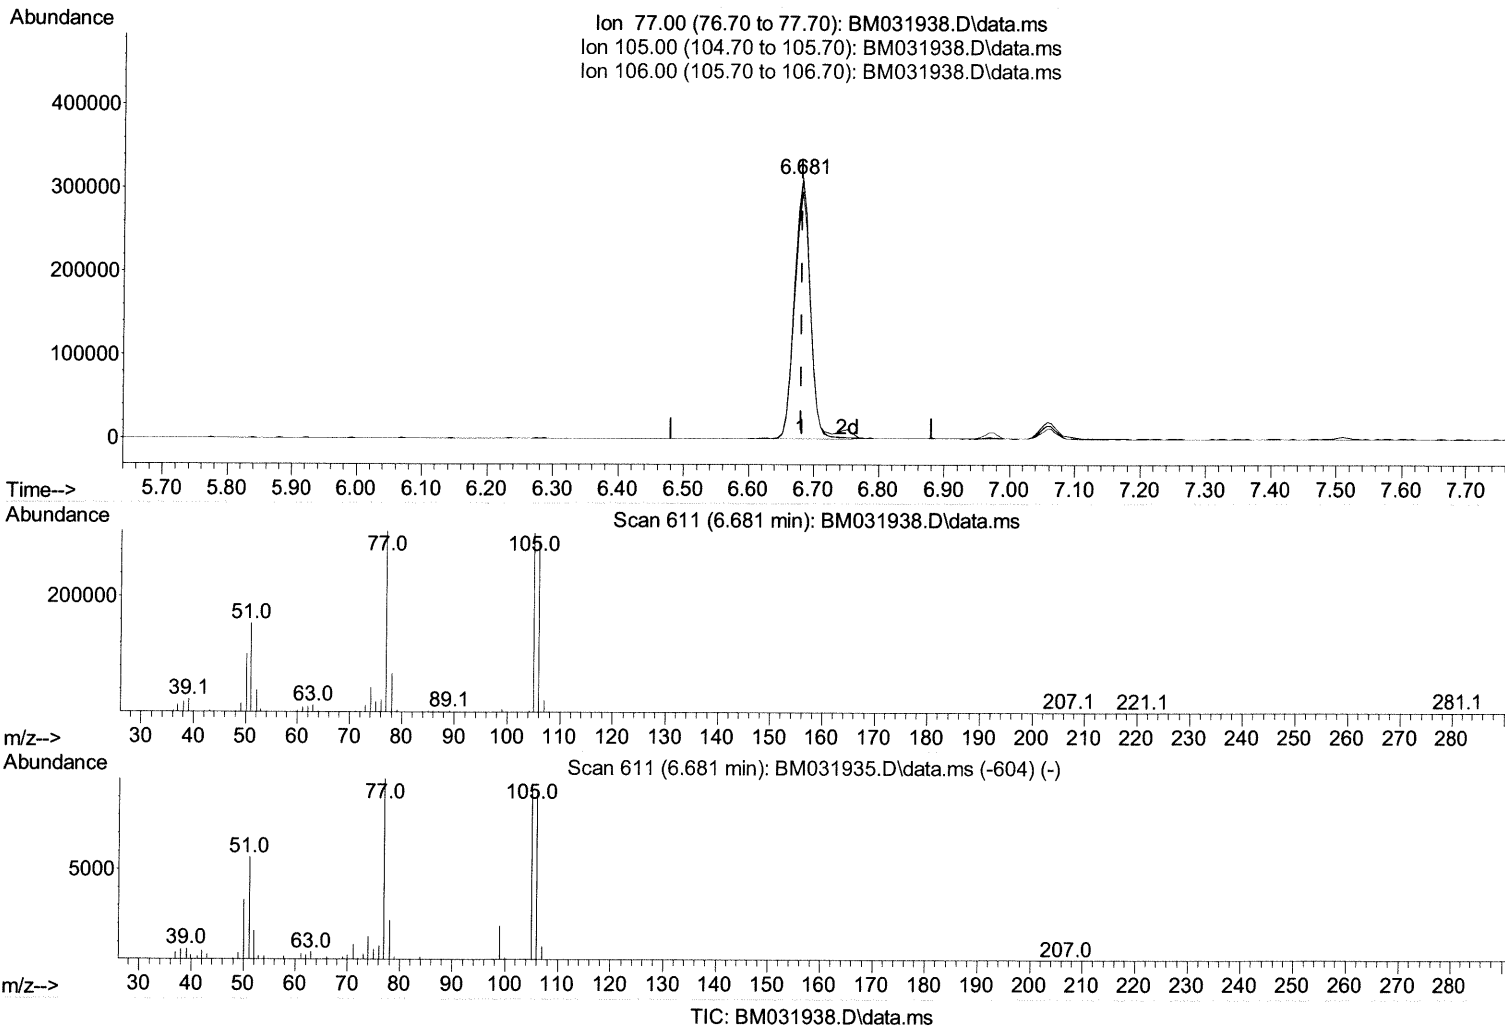

(6) Benzaldehyde

6.681min (+ 0.000) 121.77 ng/ul m 09/03/21 JU

response 540360

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	102.80	98.93
106.00	93.70	94.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031938.D
 Acq On : 28 Aug 2021 18:42
 Operator : CG/JU
 Sample : SSTD16023
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SSTD160020

Manual Integrations
APPROVED

mohammad
 8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 Qlast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

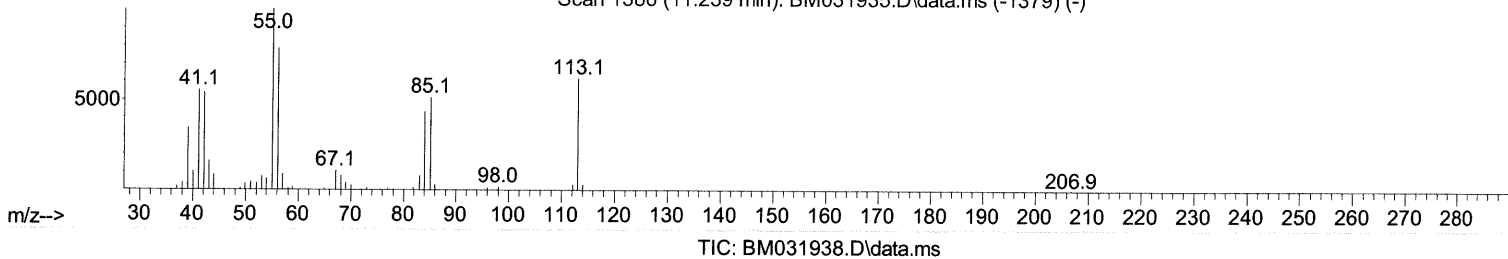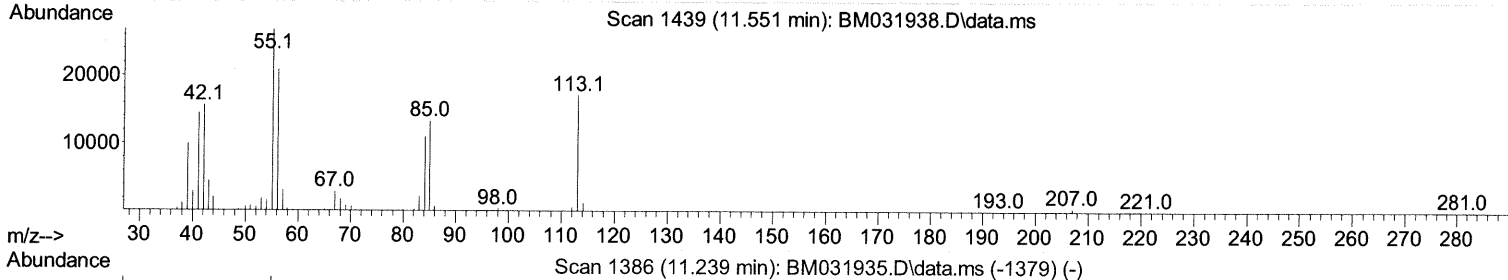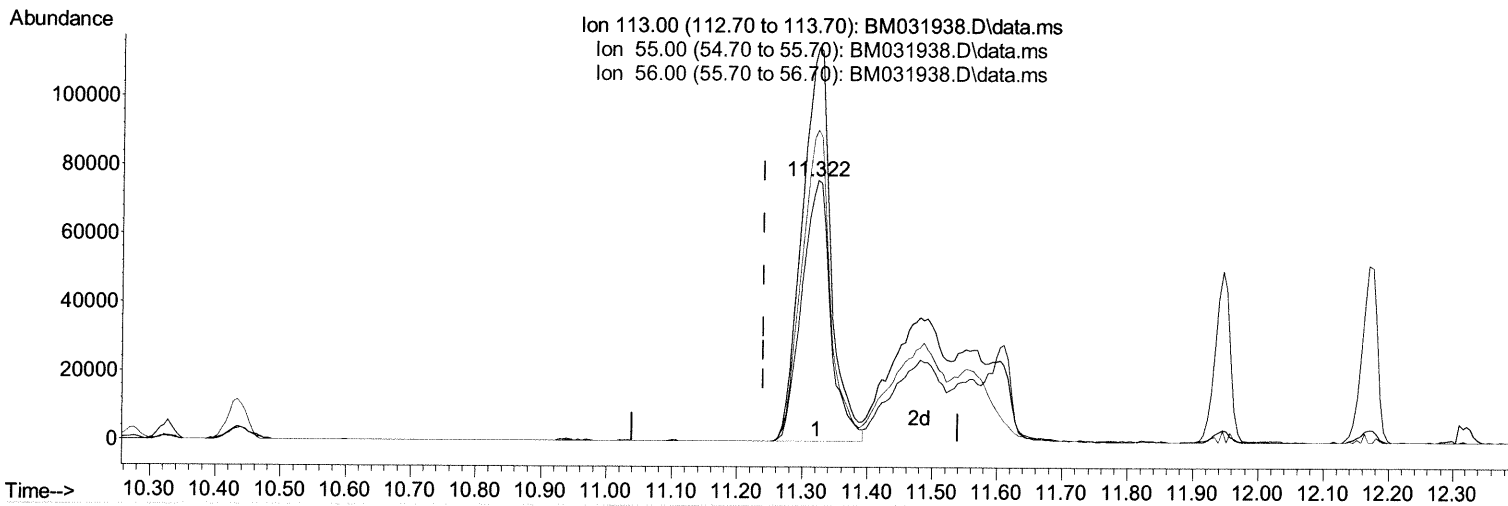

TIC: BM031938.D\data.ms

(34) Caprolactam

11.322min (+ 0.082) 117.02 ng/ul

response 233320

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	194.00	151.07#
56.00	127.40	119.48
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031938.D
 Acq On : 28 Aug 2021 18:42
 Operator : CG/JU
 Sample : SSTD16023
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160020

Manual Integrations
 APPROVED

mohammad
 8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

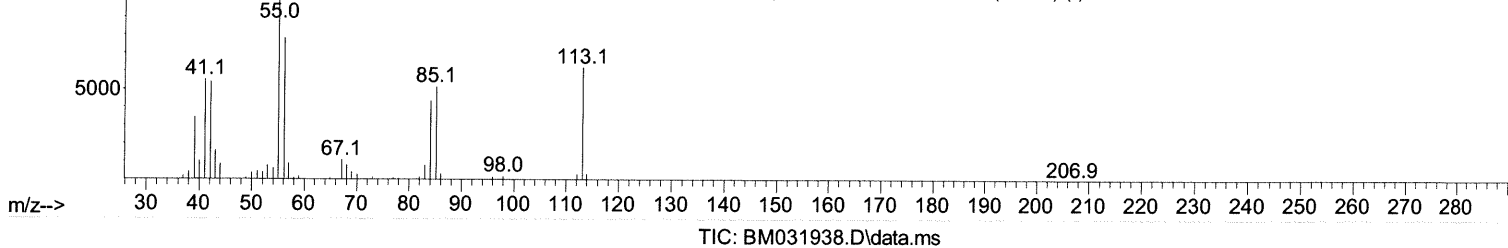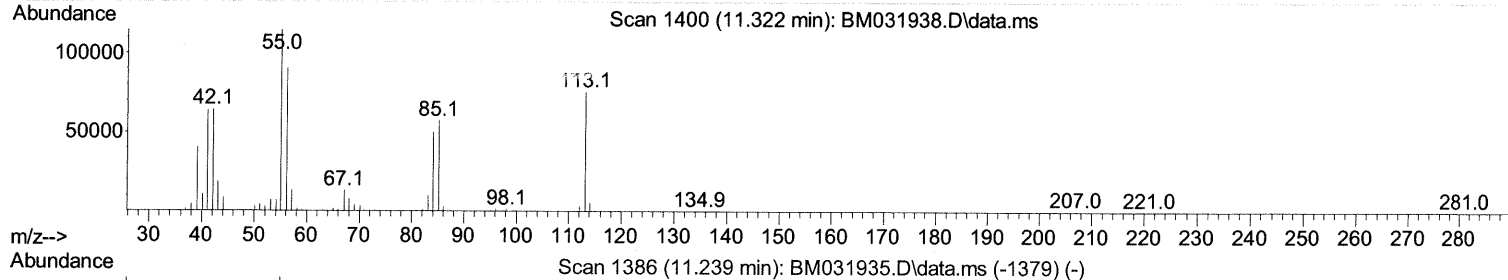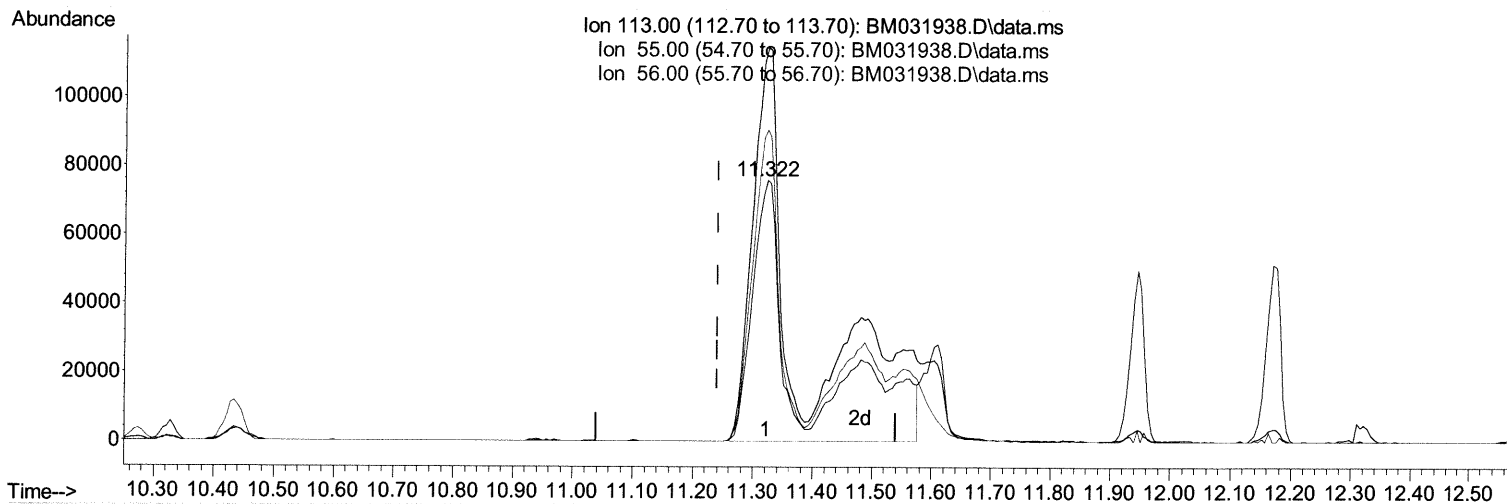

(34) Caprolactam

11.322min (+ 0.082) 206.15 ng/ul m 04/03/21 JU

response 411022

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	194.00	151.07#
56.00	127.40	119.48
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
Data File : BM031938.D
Acq On : 28 Aug 2021 18:42
Operator : CG/JU
Sample : SSTD16023
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD160020

Manual Integrations
APPROVED

mohammad
8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 28 23:51:00 2021
Response via : Initial Calibration

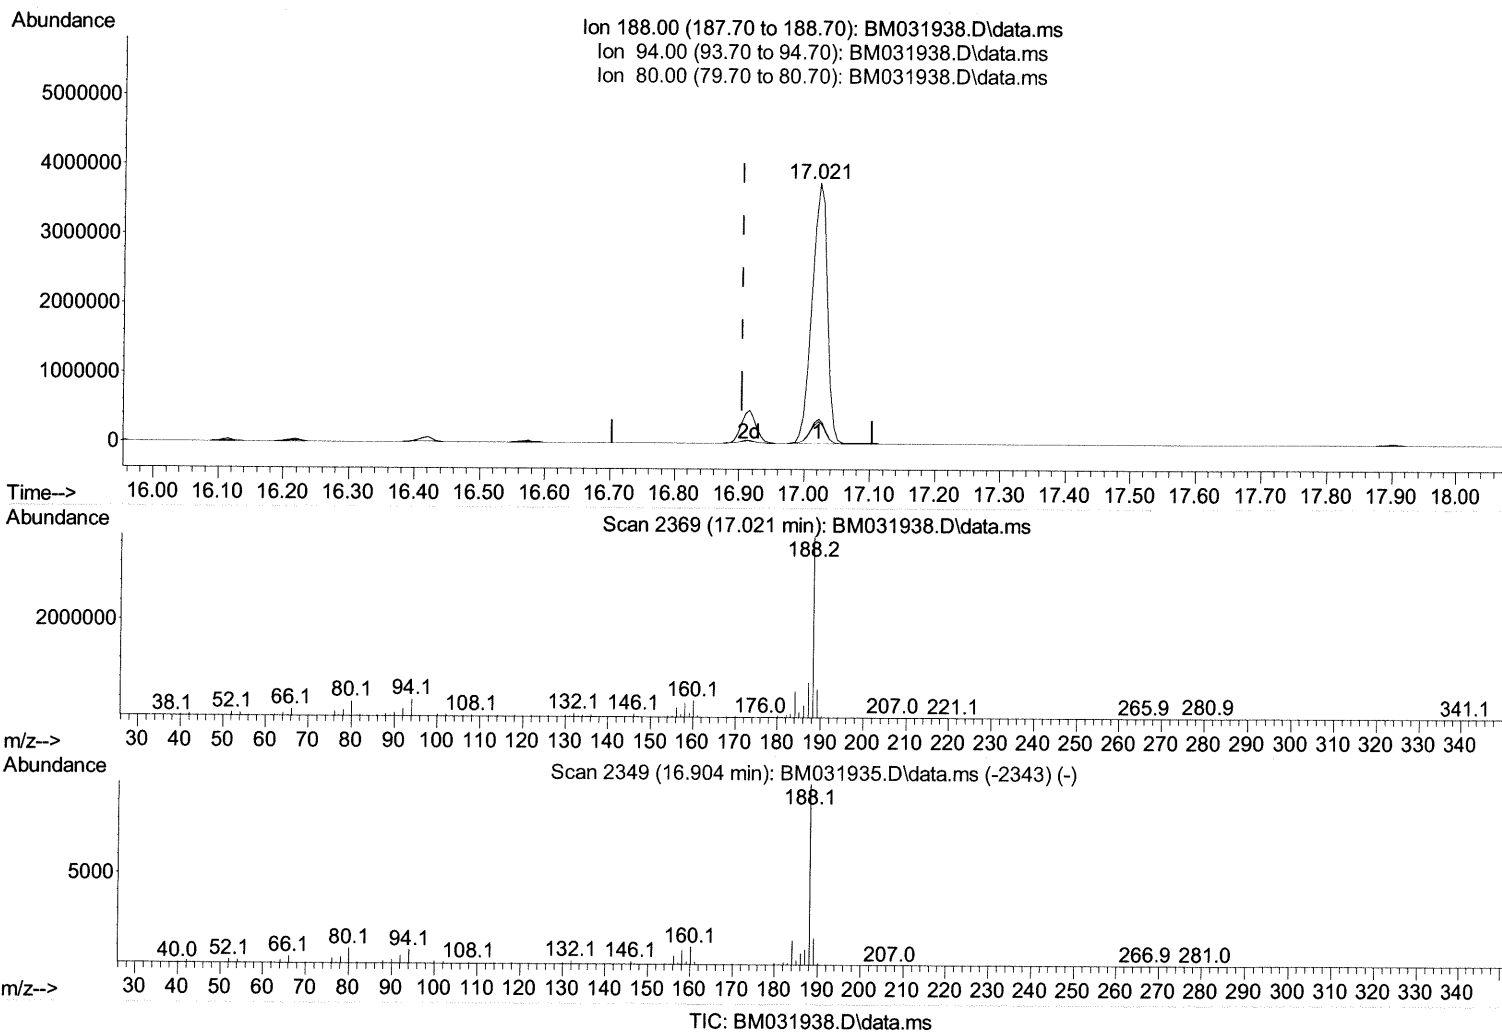

(64) Phenanthrene-d10 (I)

17.021min (+ 0.118) 20.00 ng/ul

response 6064031

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.60	9.24
80.00	10.20	8.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031938.D
 Acq On : 28 Aug 2021 18:42
 Operator : CG/JU
 Sample : SSTD16023
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160020

Manual Integrations
 APPROVED

mohammad
 8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

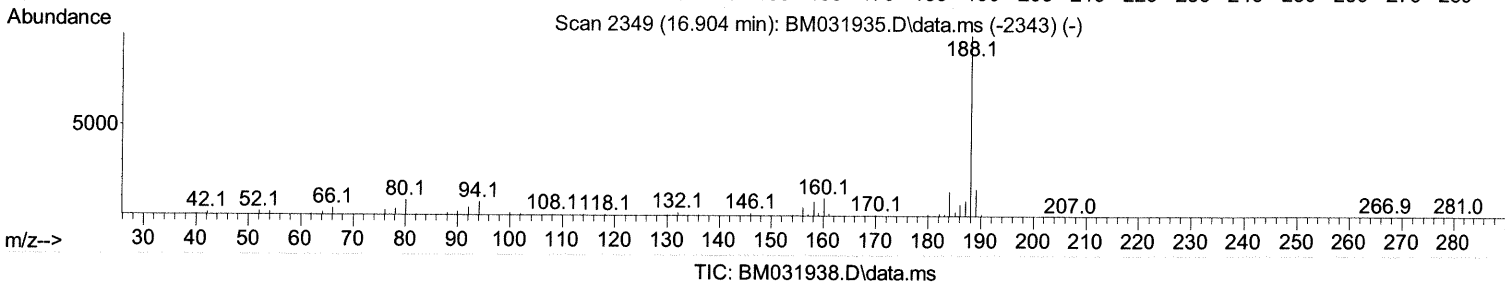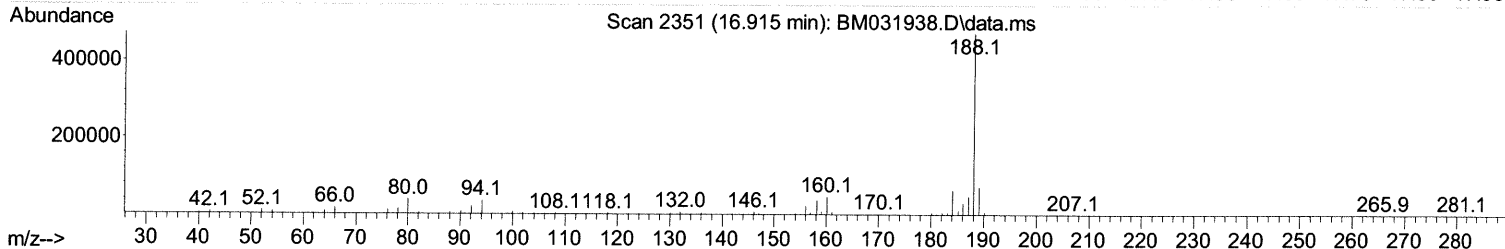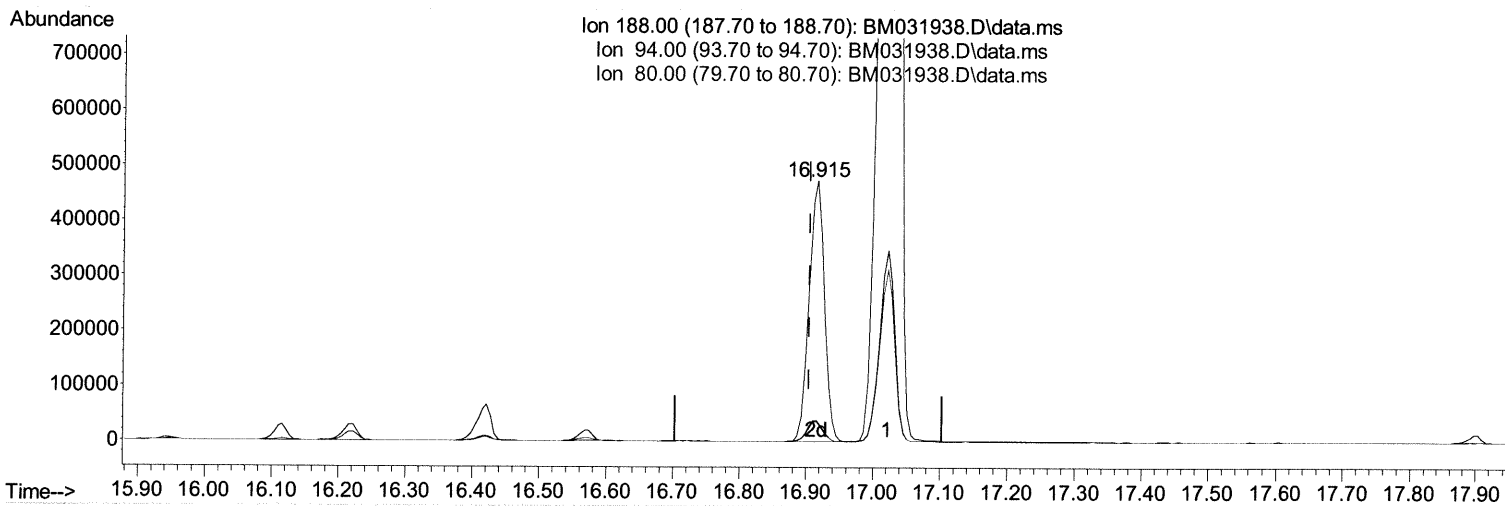

(64) Phenanthrene-d10 (I)

16.915min (+ 0.012) 20.00 ng/ul m 09/03/21 JU

response 749327

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.60	7.65#
80.00	10.20	8.15#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
 Data File : BM031938.D
 Acq On : 28 Aug 2021 18:42
 Operator : CG/JU
 Sample : SSTD16023
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160020

Manual Integrations
 APPROVED

mohammad
 8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 28 23:51:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	98700	20.000	ng/ul	0.00
20) Naphthalene-d8	10.275	136	453751	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.157	164	343342	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.915	188	749327m >	20.000	ng/ul >	0.0109/03/21 JU
79) Chrysene-d12	21.121	240	852099	20.000	ng/ul	0.01
88) Perylene-d12	23.256	264	772400	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/ul	
4) Pyridine-d5	3.516	84	1101891	166.819	ng/ul	0.00
7) Phenol-d5	6.722	99	1470214	170.474	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.881	67	779280	140.280	ng/ul	0.01
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/ul	
15) 4-Methylphenol-d8	8.245	113	1249233	180.749	ng/ul	0.02
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/ul	
31) 4-Chloroaniline-d4	10.434	131	1796521	178.023	ng/ul	0.01
46) Dimethylphthalate-d6	0.000	166	0d	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.000	ng/ul	
54) 4-Nitrophenol-d4	14.433	143	823698	196.908	ng/ul	0.05
60) Fluorene-d10	0.000	176	0d	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	15.327	200	952575	198.254	ng/ul	0.03
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
5) Pyridine	3.534	79	1096666	152.297	ng/ul	91
6) Benzaldehyde	6.681	77	540360m >	121.767	ng/ul >	09/03/21 JU
8) Phenol	6.751	94	1459683	165.129	ng/ul	97
10) Bis(2-Chloroethyl)ether	6.969	93	1053239	152.965	ng/ul	91
13) 2-Methylphenol	7.969	108	1123889	174.895	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.051	45	1297394	114.427	ng/ul#	89
16) Acetophenone	8.351	105	1867531	171.695	ng/ul	96
18) 4-Methylphenol	8.322	108	1242804	176.252	ng/ul	100
32) 4-Chloroaniline	10.463	127	1777565	175.579	ng/ul	100
34) Caprolactam	11.322	113	411022m >	206.154	ng/ul >	09/03/21 JU
40) Hexachlorocyclopentadiene	12.286	237	1063721	168.020	ng/ul	98
51) 3-Nitroaniline	14.104	138	826443	174.406	ng/ul	93
53) 2,4-Dinitrophenol	14.316	184	703440	260.276	ng/ul	92
55) 4-Nitrophenol	14.445	109	742978	209.259	ng/ul	87
63) 4-Nitroaniline	15.298	138	735599	162.959	ng/ul#	83
66) 4,6-Dinitro-2-methylph...	15.345	198	903154	194.707	ng/ul#	94
70) Atrazine	16.421	200	1206735	151.674	ng/ul	98
71) Pentachlorophenol	16.574	266	1066919	196.022	ng/ul	98
77) Carbazole	17.339	167	6260098	175.292	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.051	252	3126429	201.071	ng/ul	97
89) Di-n-octyl phthalate	21.909	149	9486825	197.773	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\
Data File : BM031938.D
Acq On : 28 Aug 2021 18:42
Operator : CG/JU
Sample : SSTD16023
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 28 23:56:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 28 23:51:00 2021
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SSTD160020

Manual Integrations
APPROVED

mohammad
8/30/2021 10:35:20 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082821\  
Data File : BM031938.D  
Acq On    : 28 Aug 2021  18:42  
Operator  : CG/JU  
Sample    : SSTD16023  
Misc      :  
ALS Vial  : 7    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
SSTD160020

Manual Integrations APPROVED

mohammad
8/30/2021 10:35:20 AM

Quant Time: Aug 28 23:56:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM082821.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 28 23:51:00 2021
Response via : Initial Calibration

