

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041527.D
 Acq On : 28 Aug 2023 18:26
 Operator : MA/JU
 Sample : PB155102BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK102

Quant Time: Aug 28 19:16:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	11119	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	31307	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	15310	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.506	188	27907	0.400	ng/ul	0.00
17) Chrysene-d12	21.694	240	9034	0.400	ng/ul	0.00
23) Perylene-d12	24.257	264	10779	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	106086	7.673	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	13235	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	15546	0.420	ng/ul	0.00
Target Compounds						Qvalue
20) Pyrene	19.896	202	4171	0.049	ng/ul#	1
26) Benzo(a)pyrene	24.094	252	6571	0.106	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041527.D
Acq On : 28 Aug 2023 18:26
Operator : MA/JU
Sample : PB155102BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK102

Quant Time: Aug 28 19:16:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

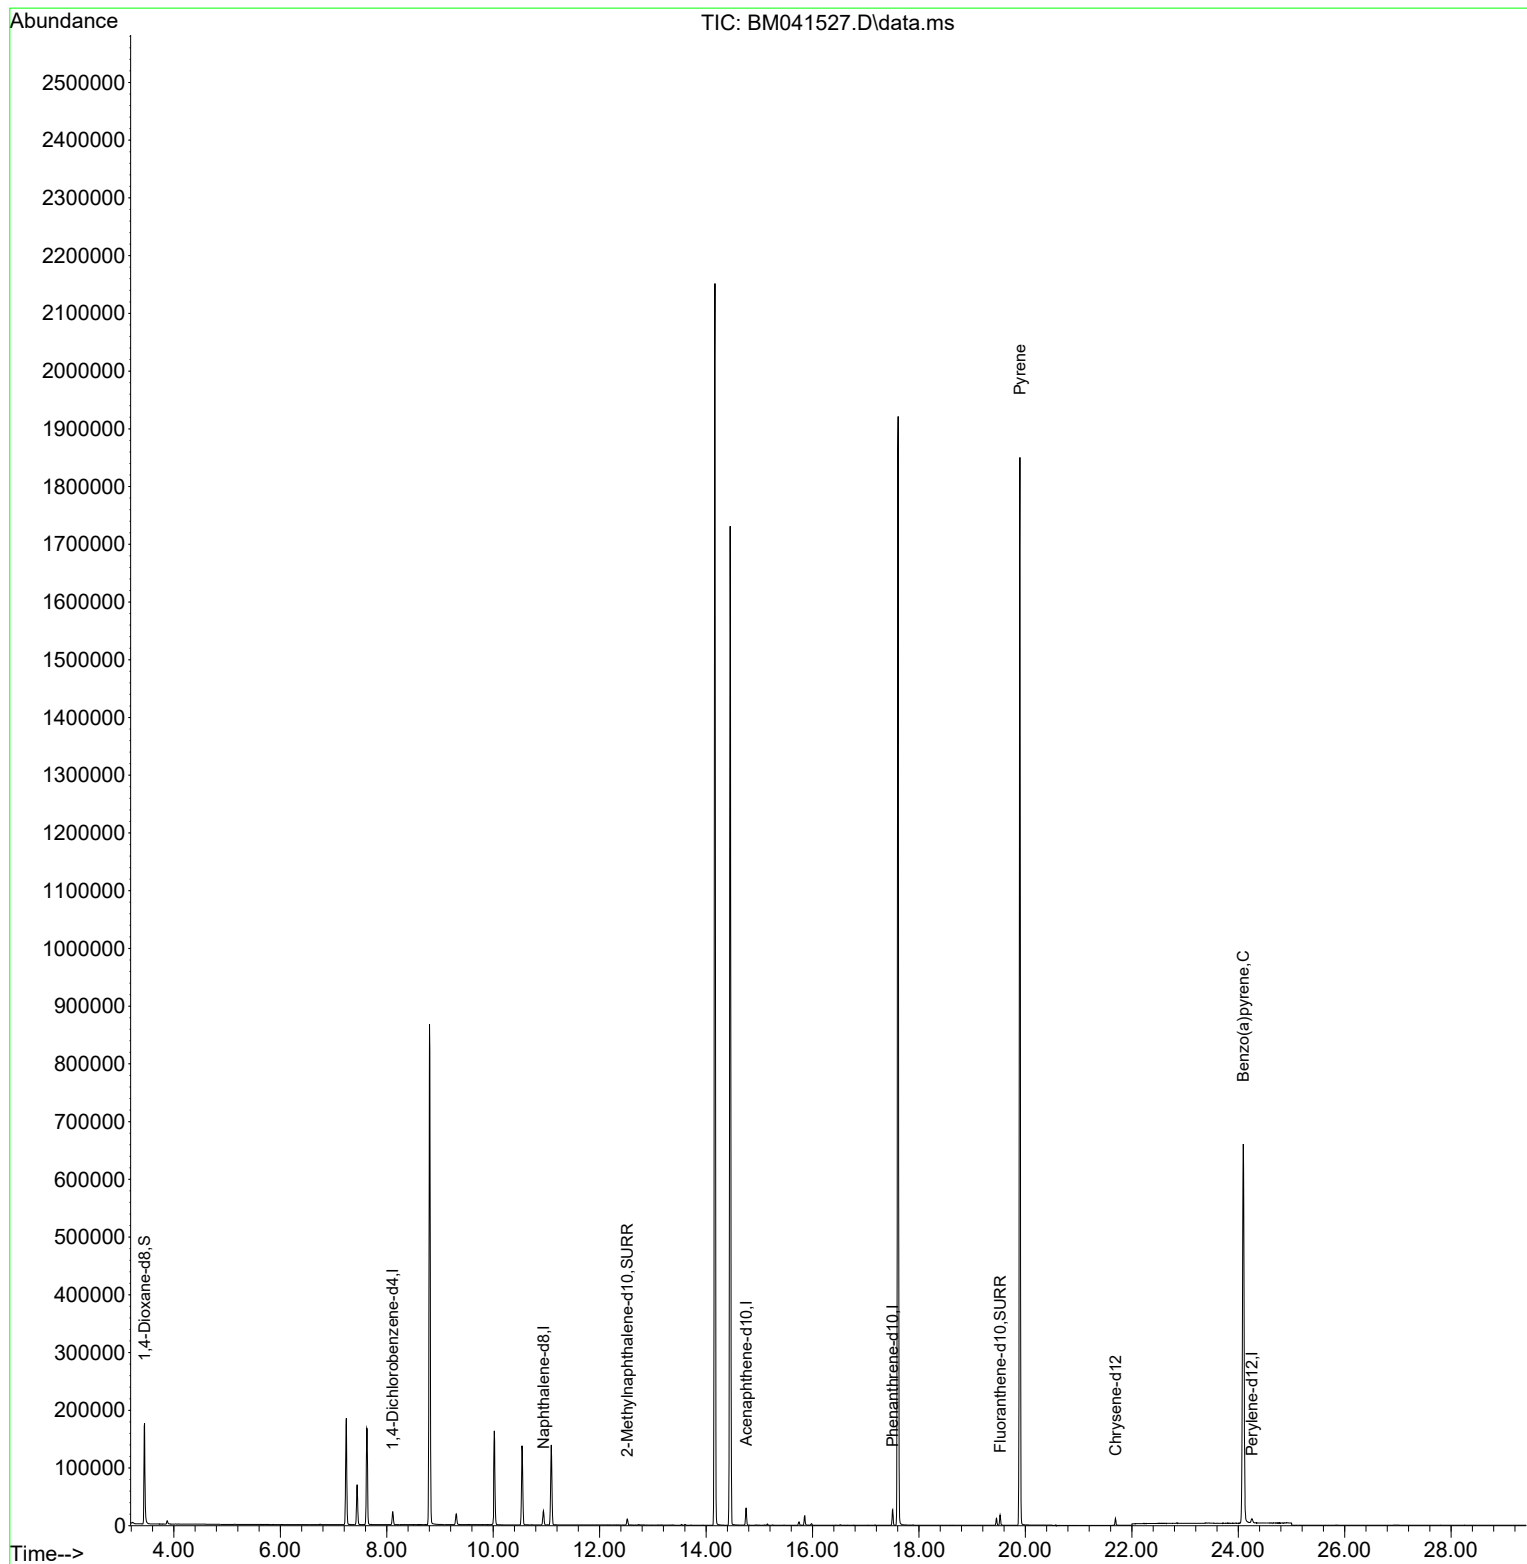

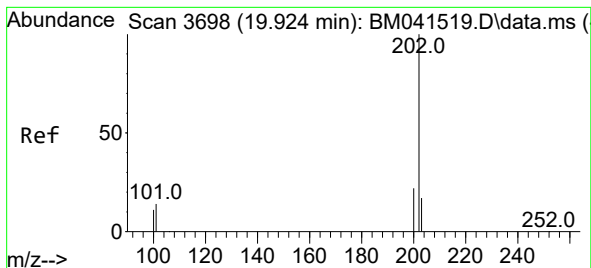

#20

Pyrene

Concen: 0.049 ng/ul

RT: 19.896 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM041527.D

Acq: 28 Aug 2023 18:26

Instrument :

BNA_M

ClientSampleId :

SBLK102





Tgt Ion:202 Resp: 4171

Ion Ratio Lower Upper

202 100

101 155.6 11.6 17.4#

100 1153.9 9.1 13.7#

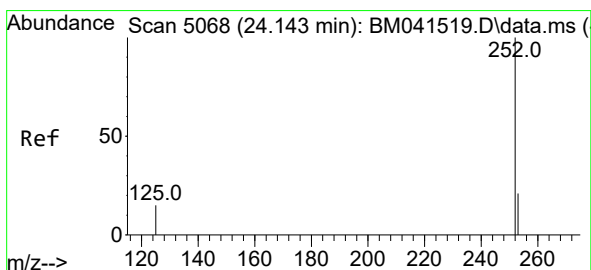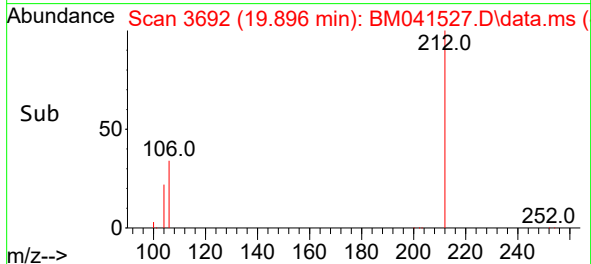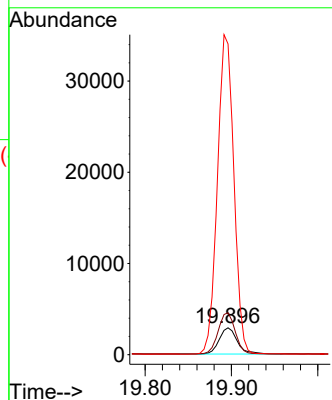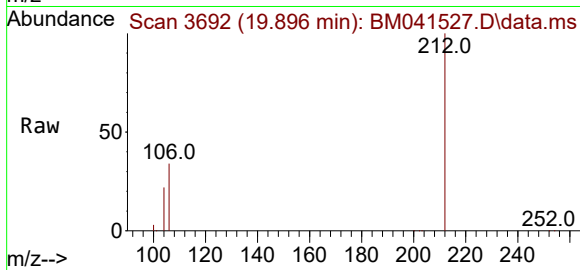

#26

Benzo(a)pyrene

Concen: 0.106 ng/ul

RT: 24.094 min Scan# 5051

Delta R.T. -0.050 min

Lab File: BM041527.D

Acq: 28 Aug 2023 18:26

Tgt Ion:252 Resp: 6571

Ion Ratio Lower Upper

252 100

253 39.7 20.0 30.0#

125 42.9 17.1 25.7#

