
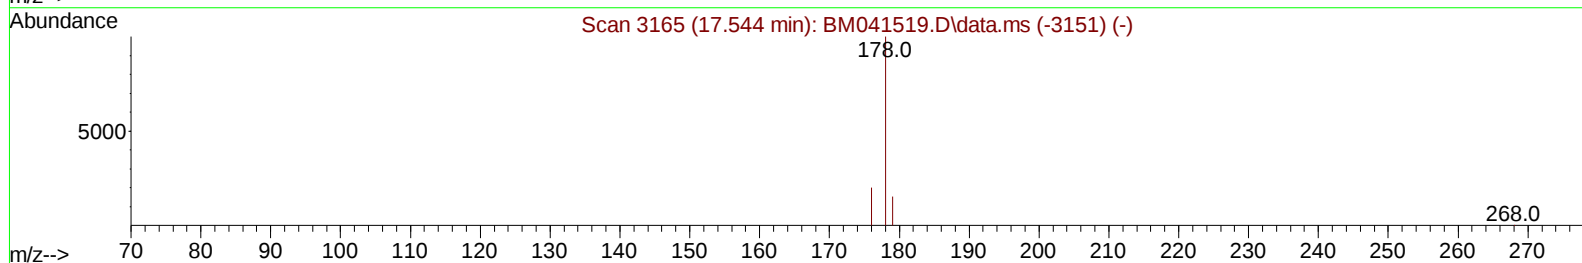
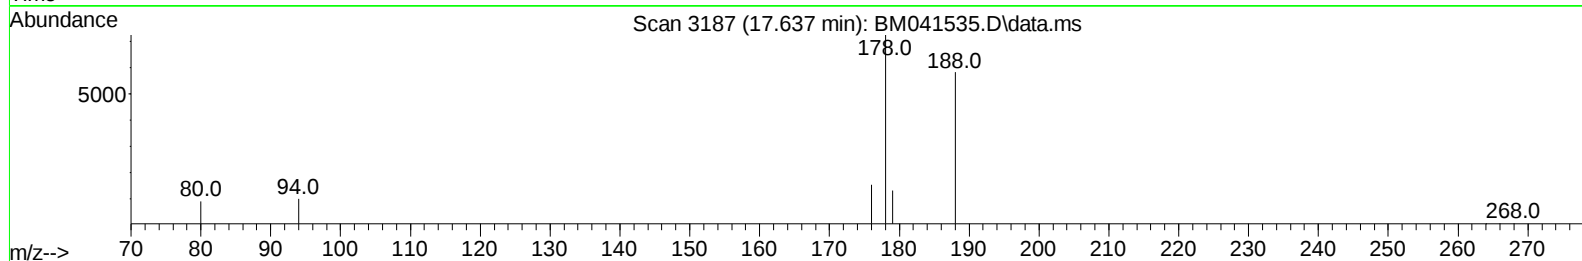


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041535.D
 Acq On : 28 Aug 2023 23:21
 Operator : MA/JU
 Sample : 04134-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 29 02:50:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

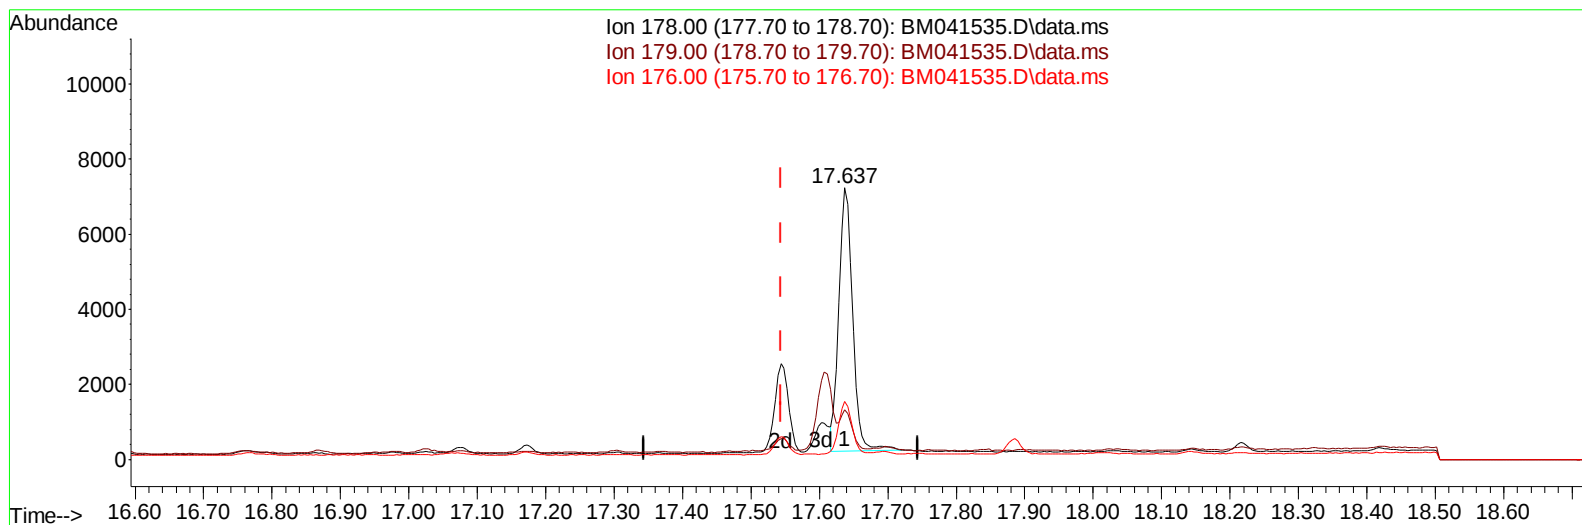

TIC: BM041535.D\data.ms

(15) Phenanthrene




17.637min (+ 0.093) 0.08 ng/u1

response 9904

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.70	18.29
176.00	20.40	21.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041535.D
Acq On : 28 Aug 2023 23:21
Operator : MA/JU
Sample : 04134-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 29 02:50:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

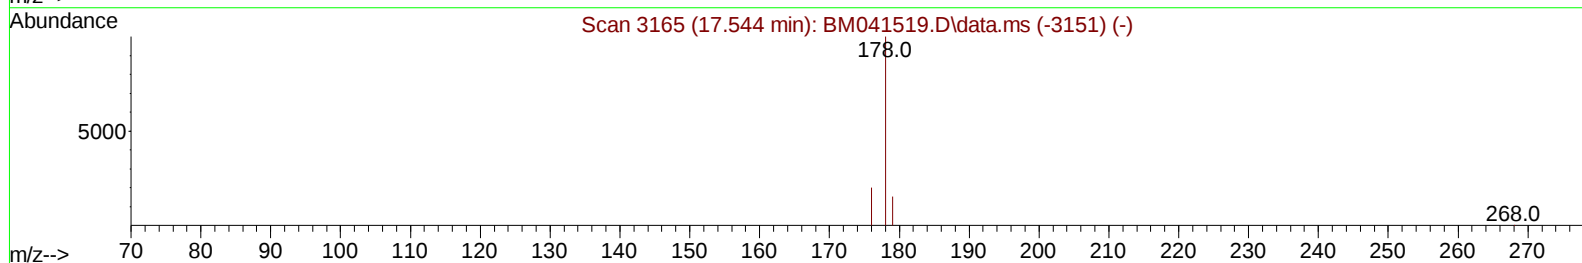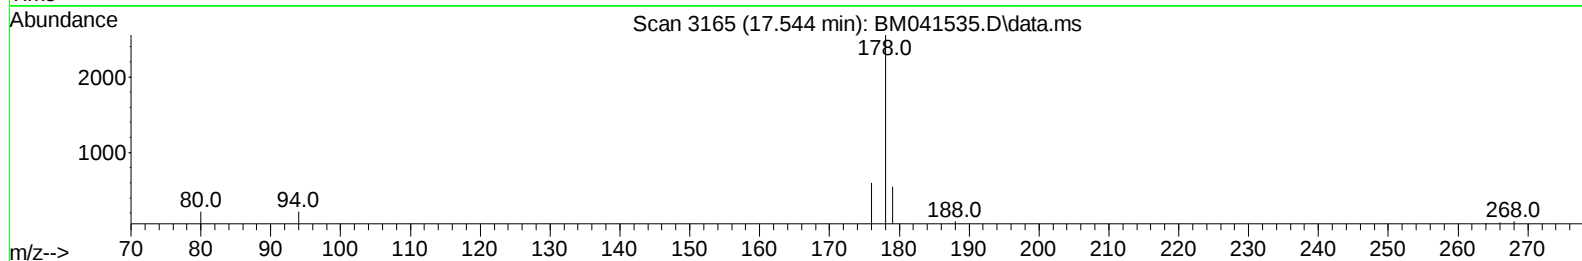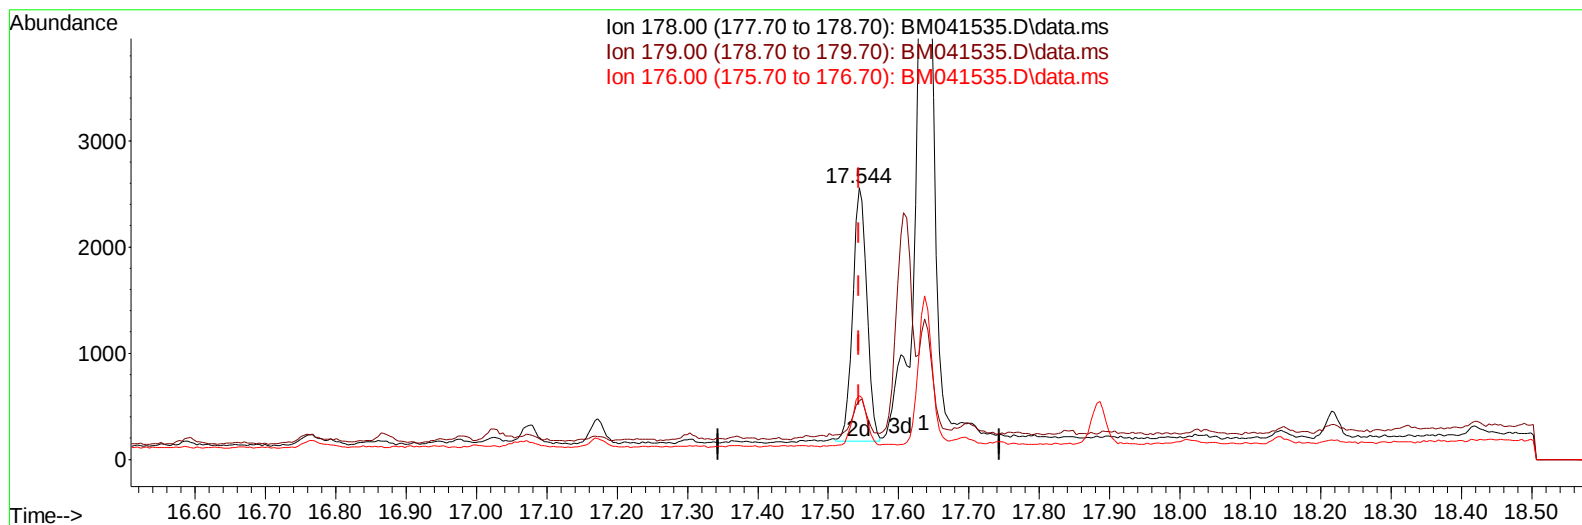

TIC: BM041535.D\data.ms

(15) Phenanthrene

17.544min (+ 0.000) 0.03 ng/ul m

response 3348

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.70	21.48#
176.00	20.40	23.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041535.D
 Acq On : 28 Aug 2023 23:21
 Operator : MA/JU
 Sample : 04134-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 29 02:50:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	10728	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	30047	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	15307	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	29063	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	11481	0.400	ng/ul	# 0.00
23) Perylene-d12	24.251	264	13279	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	74043	5.551	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	12792	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	20194	0.430	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.994	128	7376	0.077	ng/ul#	95
7) 2-Methylnaphthalene	12.588	142	2092	0.036	ng/ul	99
8) 1-Methylnaphthalene	12.808	142	1717	0.029	ng/ul	99
11) Acenaphthene	14.814	153	7636	0.108	ng/ul	99
12) Fluorene	15.800	166	14737	0.192	ng/ul	98
15) Phenanthrene	17.544	178	3348m	0.028	ng/ul	
16) Anthracene	17.637	178	10096	0.092	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041535.D
Acq On : 28 Aug 2023 23:21
Operator : MA/JU
Sample : 04134-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 29 02:50:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

