
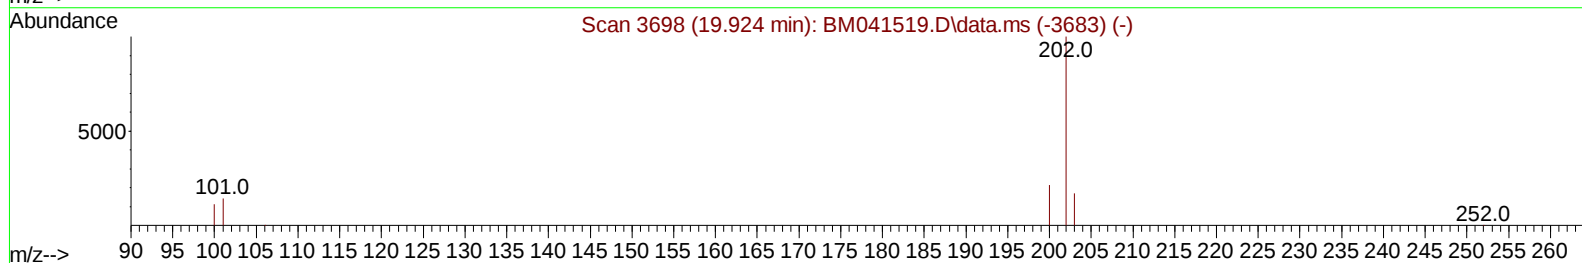
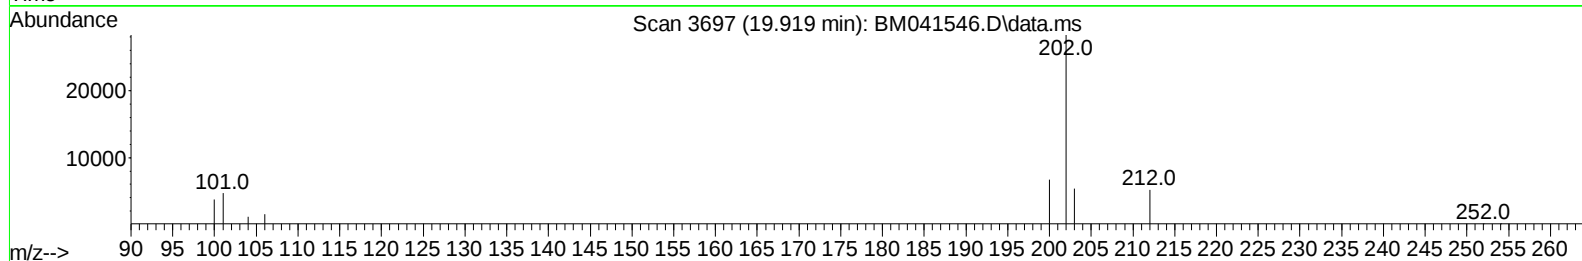


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041546.D
Acq On : 29 Aug 2023 06:40
Operator : MA/JU
Sample : 04134-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Aug 29 07:09:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

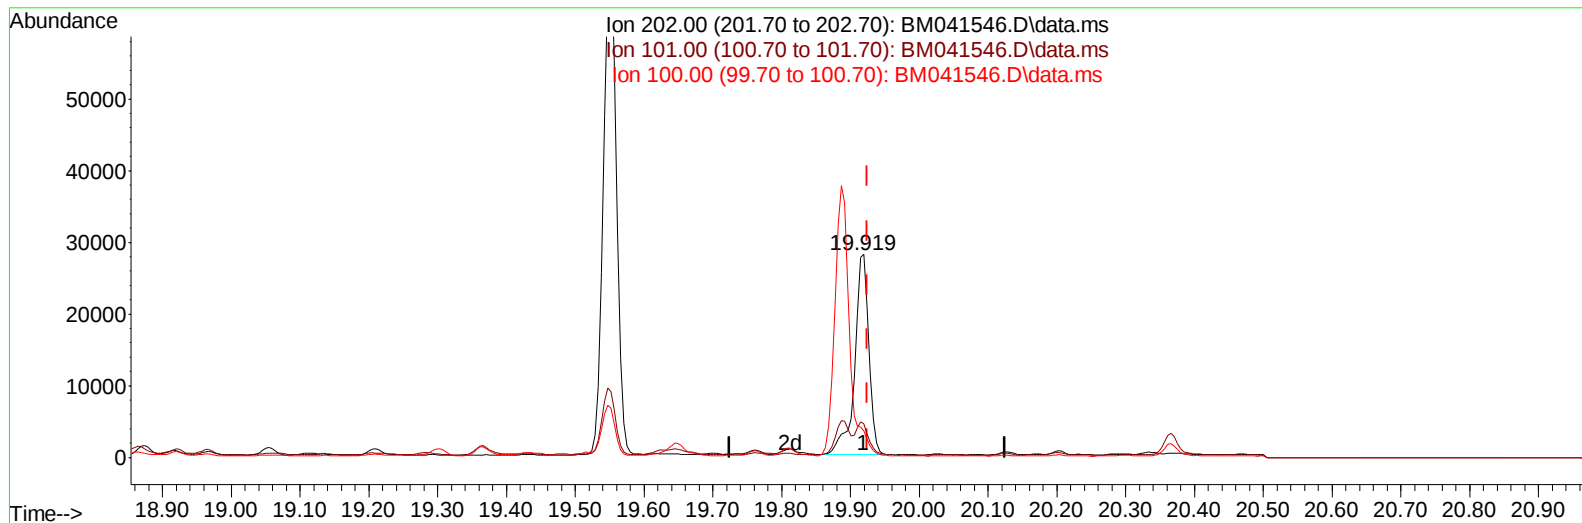

TIC: BM041546.D\data.ms

(20) Pyrene




19.919min (-0.005) 0.38 ng/u1

response 39836

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.50	16.51
100.00	11.40	13.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041546.D
Acq On : 29 Aug 2023 06:40
Operator : MA/JU
Sample : 04134-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Aug 29 07:09:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

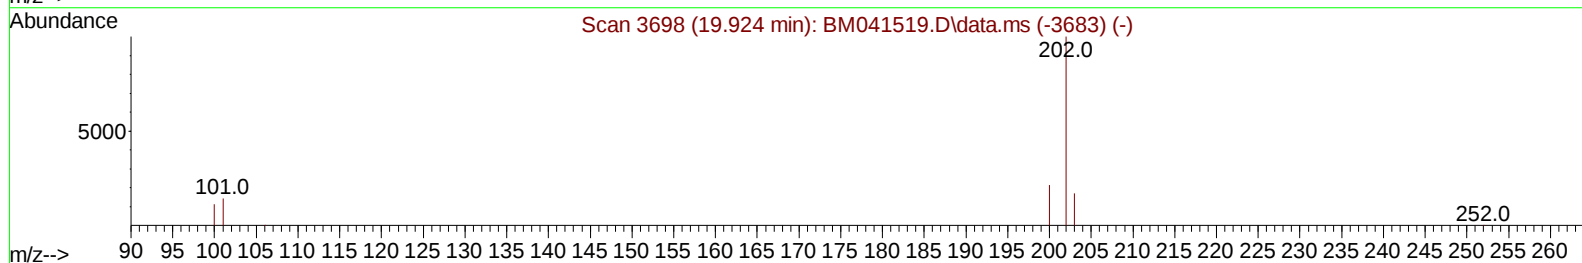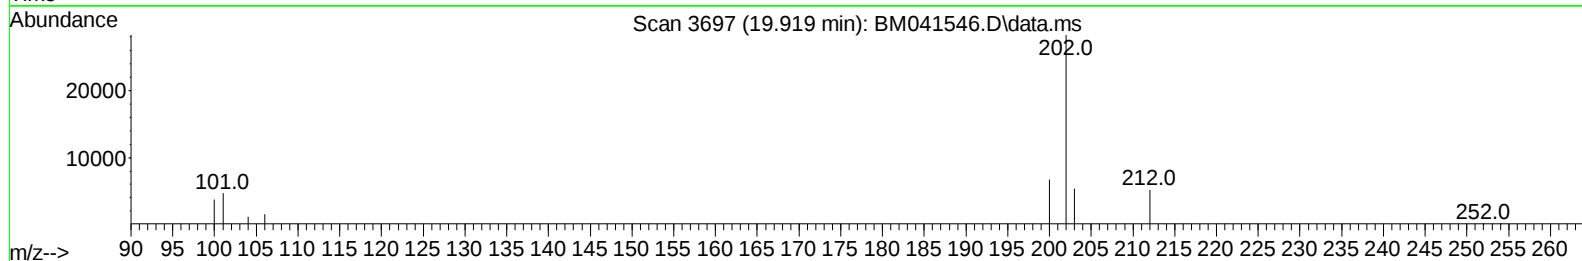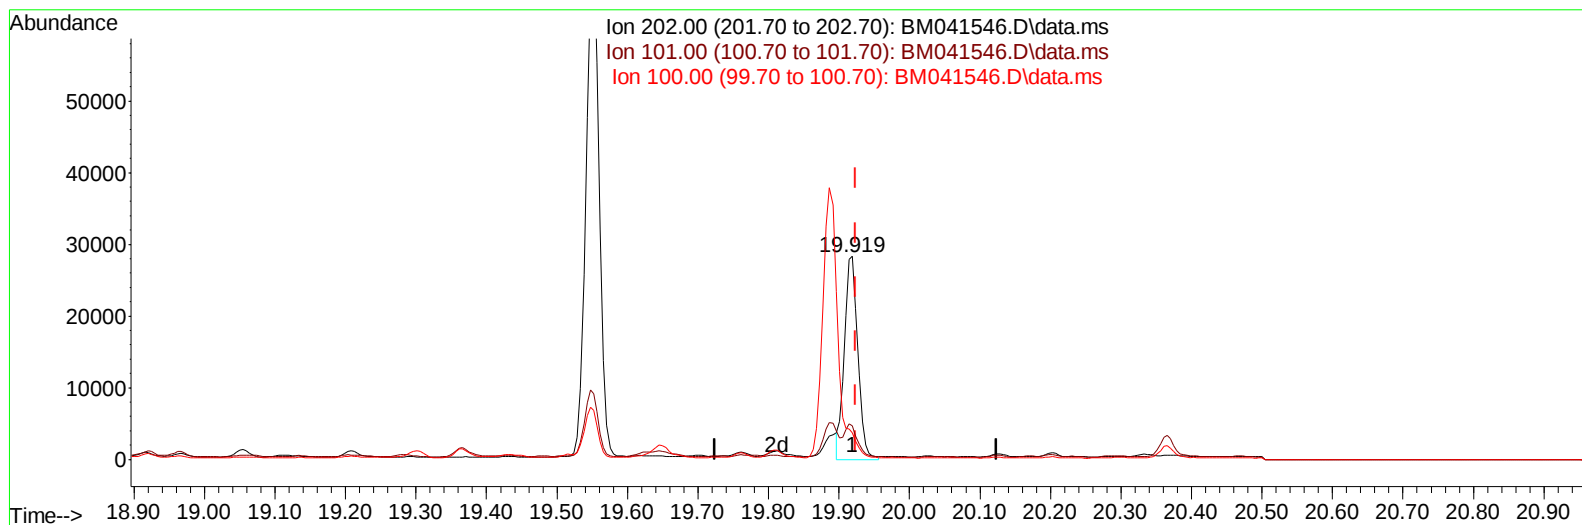

TIC: BM041546.D\data.ms

(20) Pyrene**19.919min (-0.005) 0.35 ng/ul m****response 37508**

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.50	16.51
100.00	11.40	13.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041546.D
 Acq On : 29 Aug 2023 06:40
 Operator : MA/JU
 Sample : 04134-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Quant Time: Aug 29 07:09:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	13562	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	37689	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	21815	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.502	188	34420	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	11320	0.400	ng/ul	0.00
23) Perylene-d12	24.245	264	12318	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	72476	4.298	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	13327	0.268	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	17632	0.381	ng/ul	0.00
Target Compounds				Qvalue		
5) Naphthalene	10.988	128	8640	0.072	ng/ul#	76
7) 2-Methylnaphthalene	12.588	142	418534	5.725	ng/ul	99
8) 1-Methylnaphthalene	12.808	142	787206	10.656	ng/ul	100
10) Acenaphthylene	14.476	152	91139	0.633	ng/ul#	93
11) Acenaphthene	14.814	153	2395257	23.683	ng/ul	96
12) Fluorene	15.795	166	1131235	10.360	ng/ul	99
14) Pentachlorophenol	17.126	266	466807	32.990	ng/ul	100
15) Phenanthrene	17.544	178	1788495	12.661	ng/ul	100
16) Anthracene	17.637	178	159866	1.233	ng/ul	98
19) Fluoranthene	19.552	202	92256	0.880	ng/ul	100
20) Pyrene	19.919	202	37508m	0.353	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041546.D
Acq On : 29 Aug 2023 06:40
Operator : MA/JU
Sample : 04134-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Aug 29 07:09:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

