
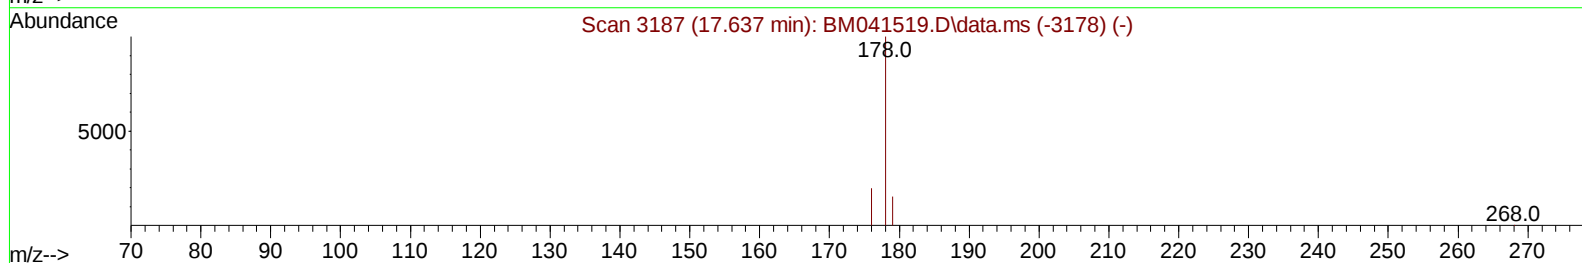
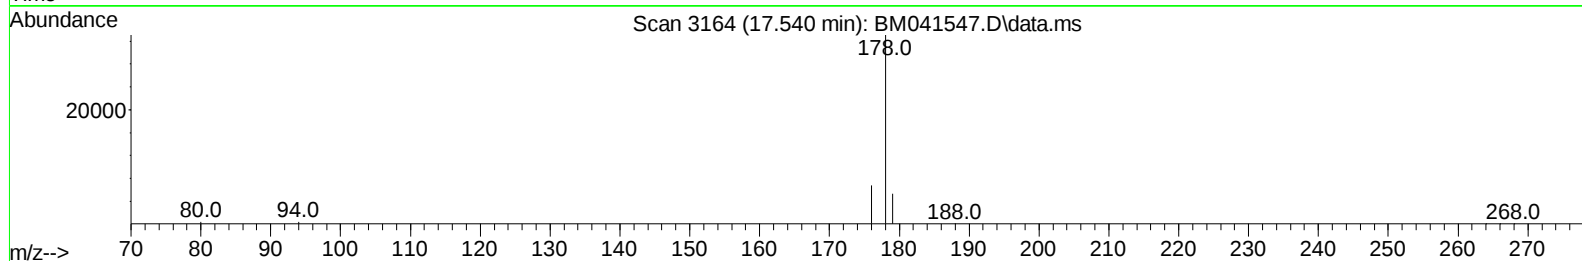


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041547.D
Acq On : 29 Aug 2023 07:16
Operator : MA/JU
Sample : 04134-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Aug 29 08:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

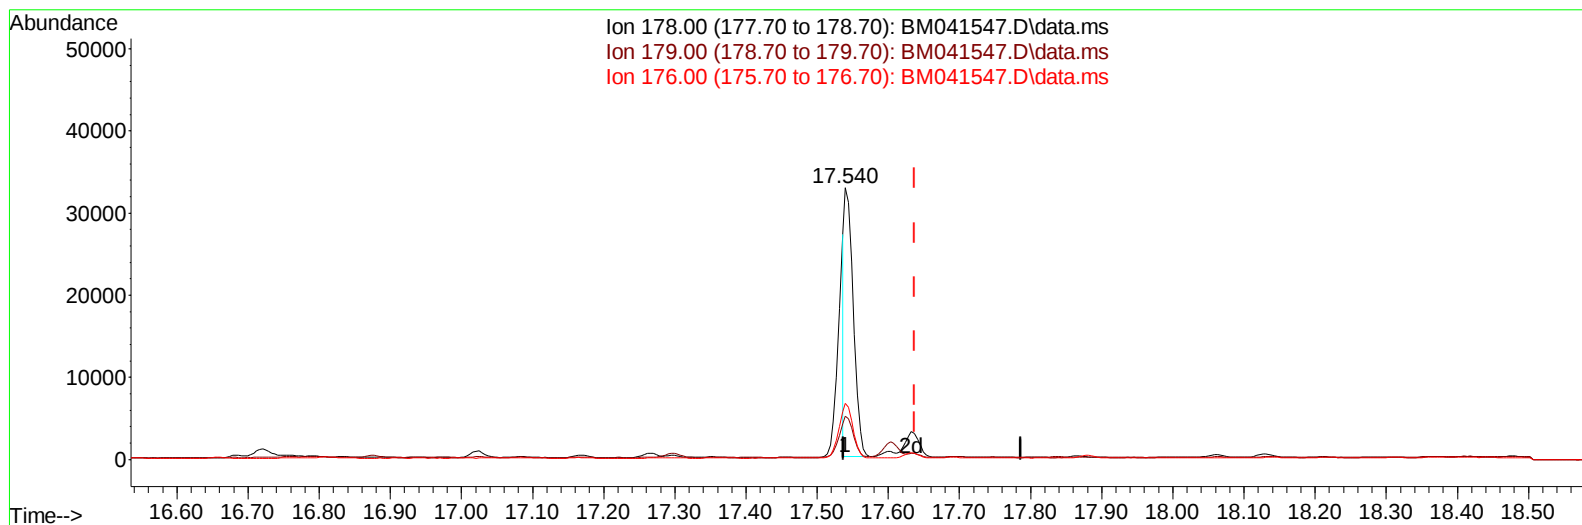




TIC: BM041547.D\data.ms

(16) Anthracene**17.540min (-0.097) 0.25 ng/u1****response 28858**

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	16.02
176.00	19.90	20.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041547.D
Acq On : 29 Aug 2023 07:16
Operator : MA/JU
Sample : 04134-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Aug 29 08:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

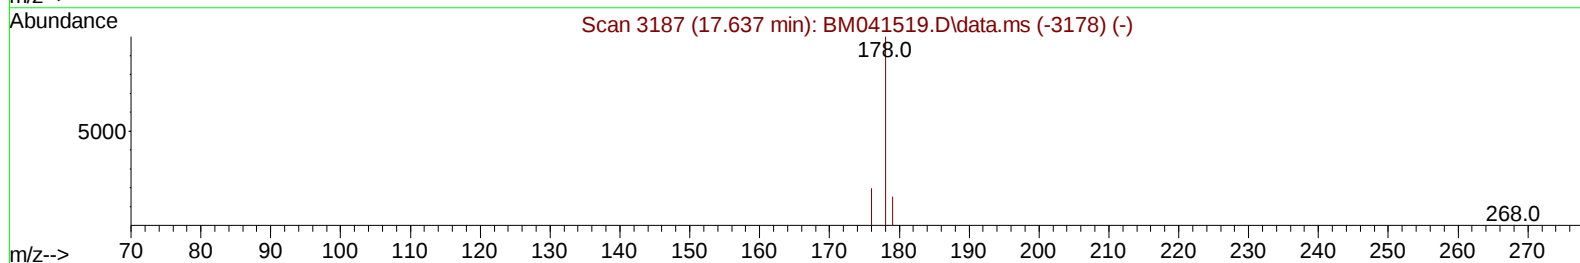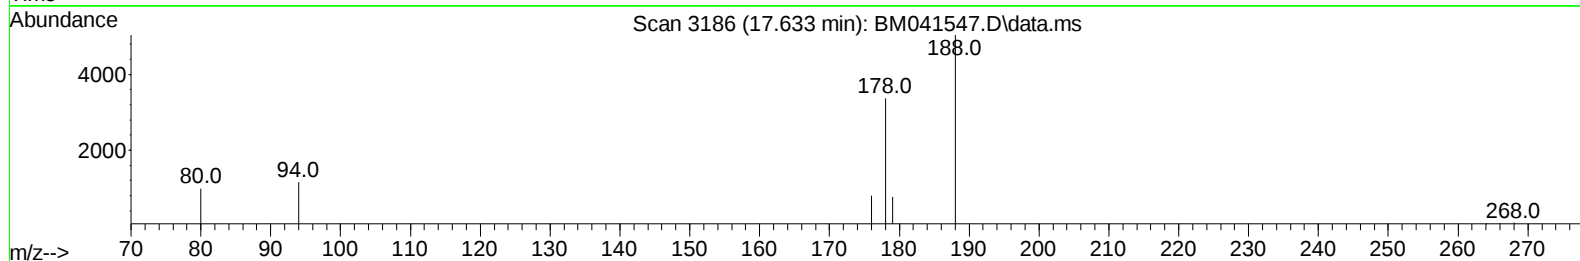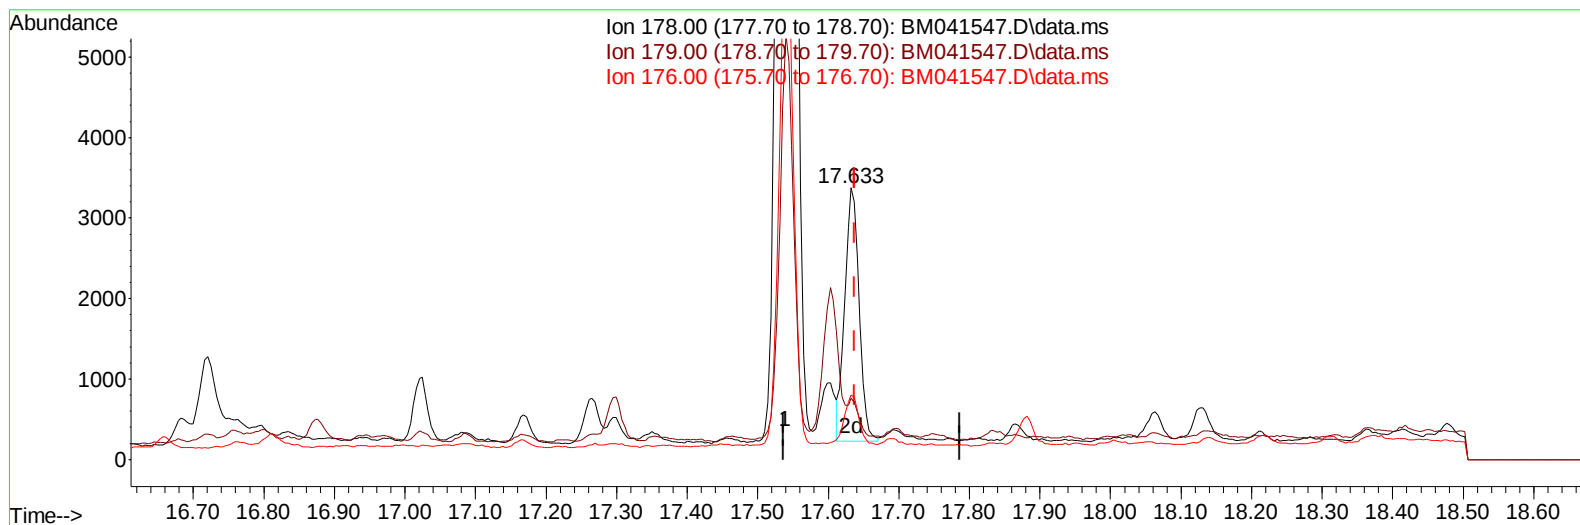

TIC: BM041547.D\data.ms

(16) Anthracene

17.633min (-0.004) 0.04 ng/ul m

response 4420

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	22.58#
176.00	19.90	23.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041547.D
 Acq On : 29 Aug 2023 07:16
 Operator : MA/JU
 Sample : 04134-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Aug 29 08:09:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	11185	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	32110	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.745	164	15762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.497	188	30076	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.685	240	10175	0.400	ng/ul	# 0.00
23) Perylene-d12	24.246	264	10563	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	62050	4.462	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	9639	0.227	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	15761	0.378	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.988	128	5509	0.054	ng/ul#	92
7) 2-Methylnaphthalene	12.588	142	14291	0.229	ng/ul	99
8) 1-Methylnaphthalene	12.803	142	11950	0.190	ng/ul	99
10) Acenaphthylene	14.476	152	2964	0.029	ng/ul#	83
11) Acenaphthene	14.809	153	38854	0.532	ng/ul	99
12) Fluorene	15.795	166	36927	0.468	ng/ul	100
14) Pentachlorophenol	17.122	266	664	0.054	ng/ul	100
15) Phenanthrene	17.540	178	44840	0.363	ng/ul	99
16) Anthracene	17.633	178	4420m	0.039	ng/ul	
19) Fluoranthene	19.547	202	2958	0.031	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041547.D
Acq On : 29 Aug 2023 07:16
Operator : MA/JU
Sample : 04134-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Aug 29 08:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

