

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082823\  
 Data File : BM041538.D  
 Acq On : 29 Aug 2023 01:11  
 Operator : MA/JU  
 Sample : 04113-11  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 EZYN8

Quant Time: Aug 29 02:50:36 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM082823.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 28 15:20:06 2023  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min)     |
|-----------------------------|--------|------|----------|-------|--------|--------------|
| -----                       |        |      |          |       |        |              |
| Internal Standards          |        |      |          |       |        |              |
| 1) 1,4-Dichlorobenzene-d4   | 8.110  | 152  | 11069    | 0.400 | ng/ul  | 0.00         |
| 4) Naphthalene-d8           | 10.944 | 136  | 33322    | 0.400 | ng/ul  | 0.00         |
| 9) Acenaphthene-d10         | 14.749 | 164  | 16102    | 0.400 | ng/ul  | 0.00         |
| 13) Phenanthrene-d10        | 17.502 | 188  | 28326    | 0.400 | ng/ul  | 0.00         |
| 17) Chrysene-d12            | 21.685 | 240  | 10182    | 0.400 | ng/ul  | 0.00         |
| 23) Perylene-d12            | 24.248 | 264  | 11874    | 0.400 | ng/ul  | -0.01        |
| System Monitoring Compounds |        |      |          |       |        |              |
| 3) 1,4-Dioxane-d8           | 3.448  | 96   | 44081    | 3.203 | ng/ul  | 0.00         |
| 6) 2-Methylnaphthalene-d10  | 12.517 | 152  | 15123    | 0.344 | ng/ul  | 0.00         |
| 18) Fluoranthene-d10        | 19.524 | 212  | 20325    | 0.488 | ng/ul  | 0.00         |
| Target Compounds            |        |      |          |       |        |              |
| 5) Naphthalene              | 10.993 | 128  | 2439     | 0.023 | ng/ul# | Qvalue<br>84 |
| -----                       |        |      |          |       |        |              |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082823\  
Data File : BM041538.D  
Acq On : 29 Aug 2023 01:11  
Operator : MA/JU  
Sample : 04113-11  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
EZYN8


Quant Time: Aug 29 02:50:36 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM082823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 28 15:20:06 2023  
Response via : Initial Calibration

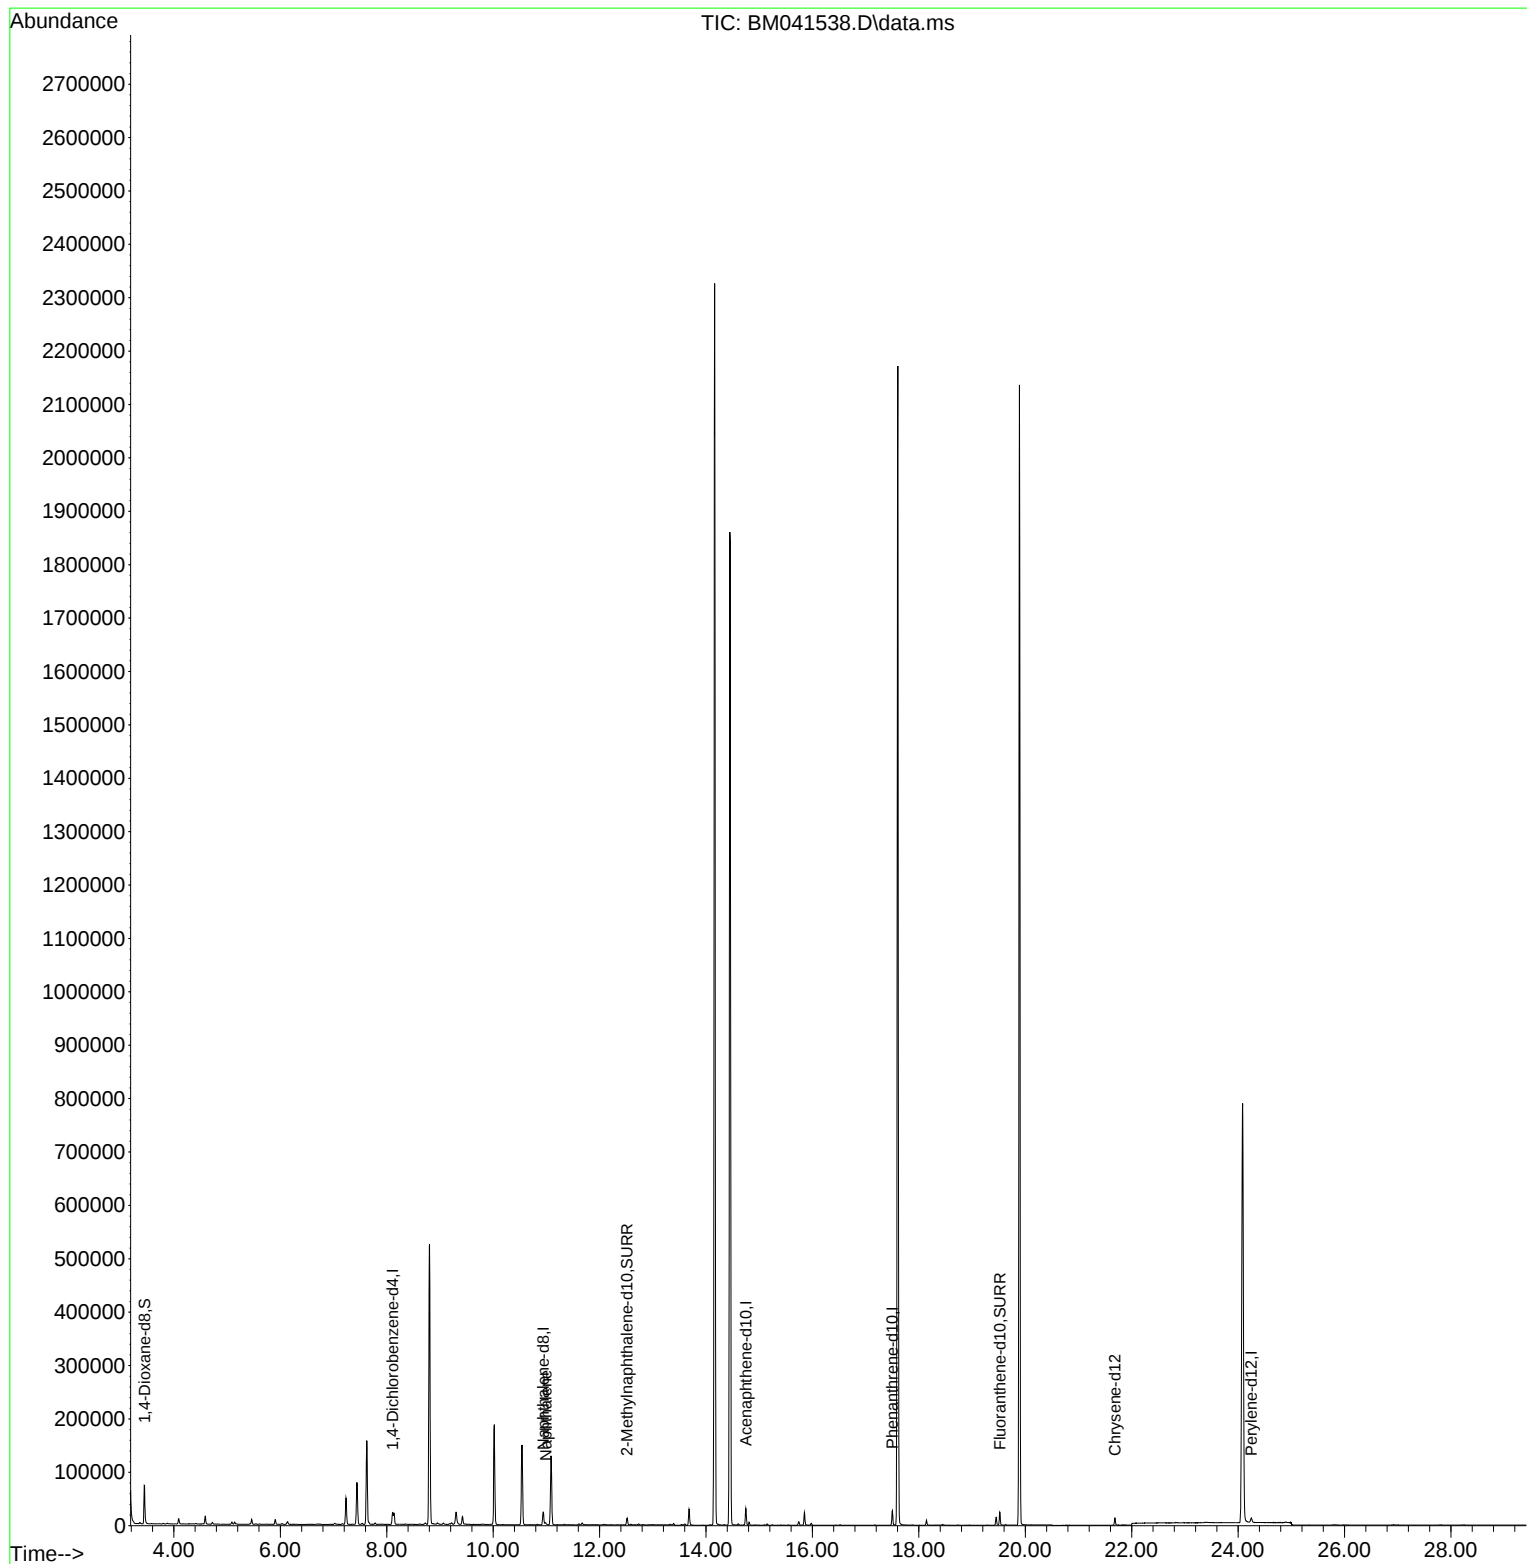

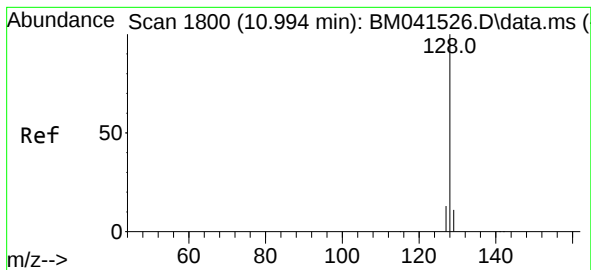

#5  
Naphthalene  
Concen: 0.023 ng/ul  
RT: 10.993 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: BM041538.D  
Acq: 29 Aug 2023 01:11

Instrument :  
BNA\_M  
ClientSampleId :  
EZYN8

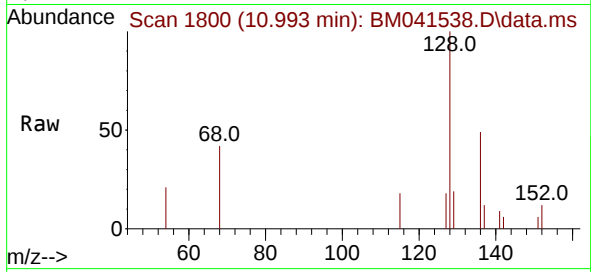

Tgt Ion:128 Resp: 2439  
Ion Ratio Lower Upper  
128 100  
129 19.0 8.9 13.3#  
127 17.8 10.6 15.8#

