

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041539.D
 Acq On : 29 Aug 2023 01:48
 Operator : MA/JU
 Sample : 04134-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHK6

Quant Time: Aug 29 02:50:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	12500	0.400	ng/ul	0.00
4) Naphthalene-d8	10.939	136	35175	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	17256	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	31505	0.400	ng/ul	0.00
17) Chrysene-d12	21.682	240	10853	0.400	ng/ul	-0.01
23) Perylene-d12	24.243	264	12918	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	70613	4.543	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	11725	0.252	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	17335	0.390	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	17.122	266	1681	0.130	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041539.D
Acq On : 29 Aug 2023 01:48
Operator : MA/JU
Sample : 04134-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHK6

Quant Time: Aug 29 02:50:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

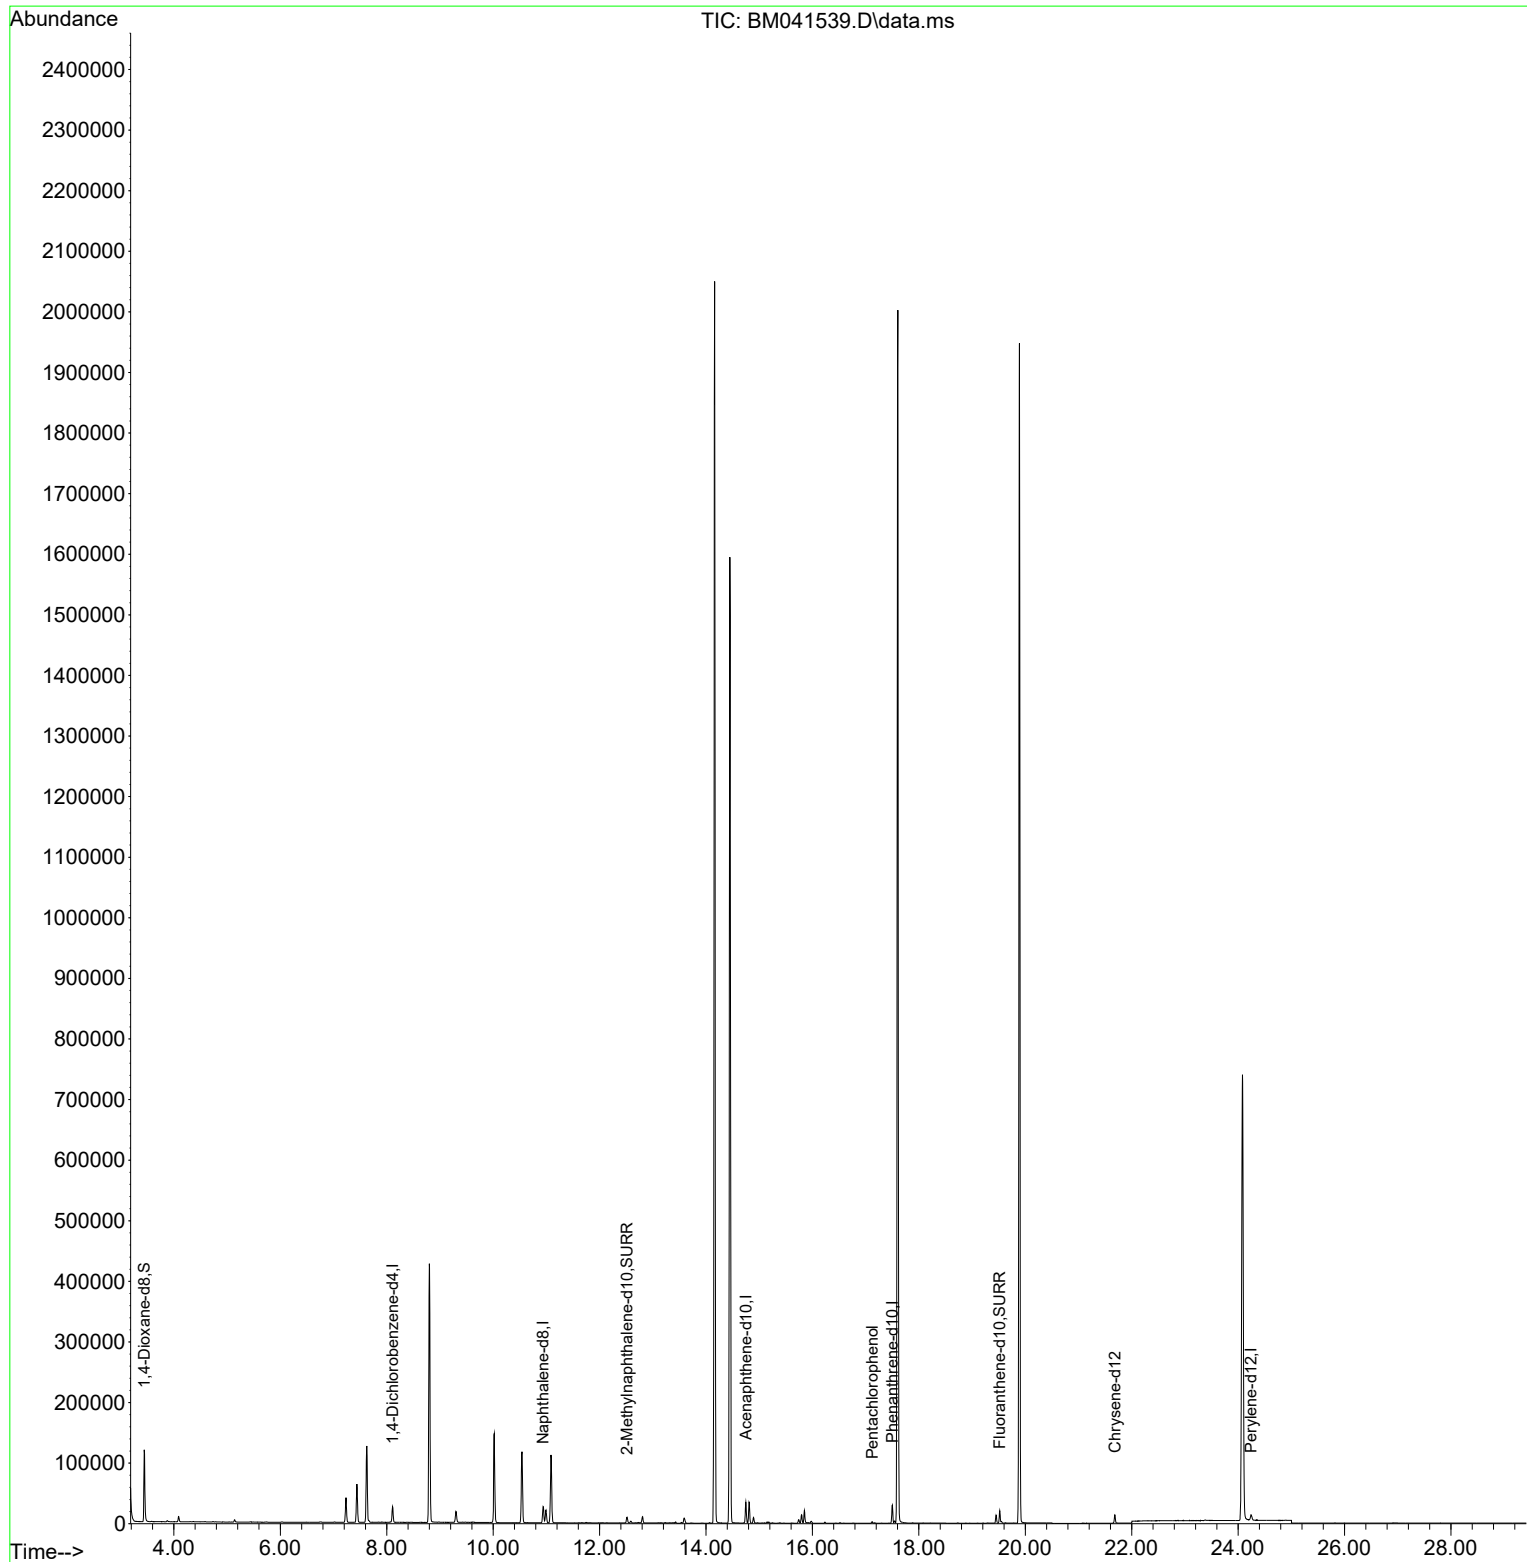

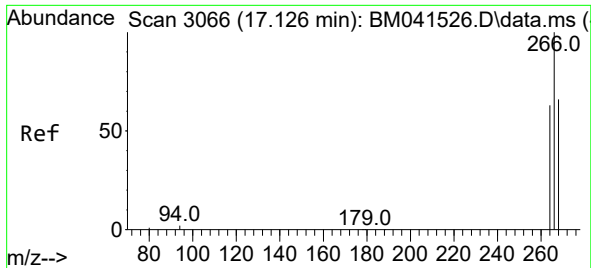

#14
 Pentachlorophenol
 Concen: 0.130 ng/ul
 RT: 17.122 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM041539.D
 Acq: 29 Aug 2023 01:48

Instrument :
 BNA_M
 ClientSampleId :
 DCHK6

Tgt Ion:266 Resp: 1681
 Ion Ratio Lower Upper
 266 100
 264 62.4 50.0 75.0
 268 64.5 51.4 77.0

