

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041540.D
 Acq On : 29 Aug 2023 02:25
 Operator : MA/JU
 Sample : 04134-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHK8

Quant Time: Aug 29 03:18:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	10656	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	30210	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	14995	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	28005	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	9693	0.400	ng/ul	0.00
23) Perylene-d12	24.246	264	11293	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	61790	4.664	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	10962	0.275	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	17237	0.435	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.117	266	258	0.022	ng/ul	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041540.D
Acq On : 29 Aug 2023 02:25
Operator : MA/JU
Sample : 04134-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHK8

Quant Time: Aug 29 03:18:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

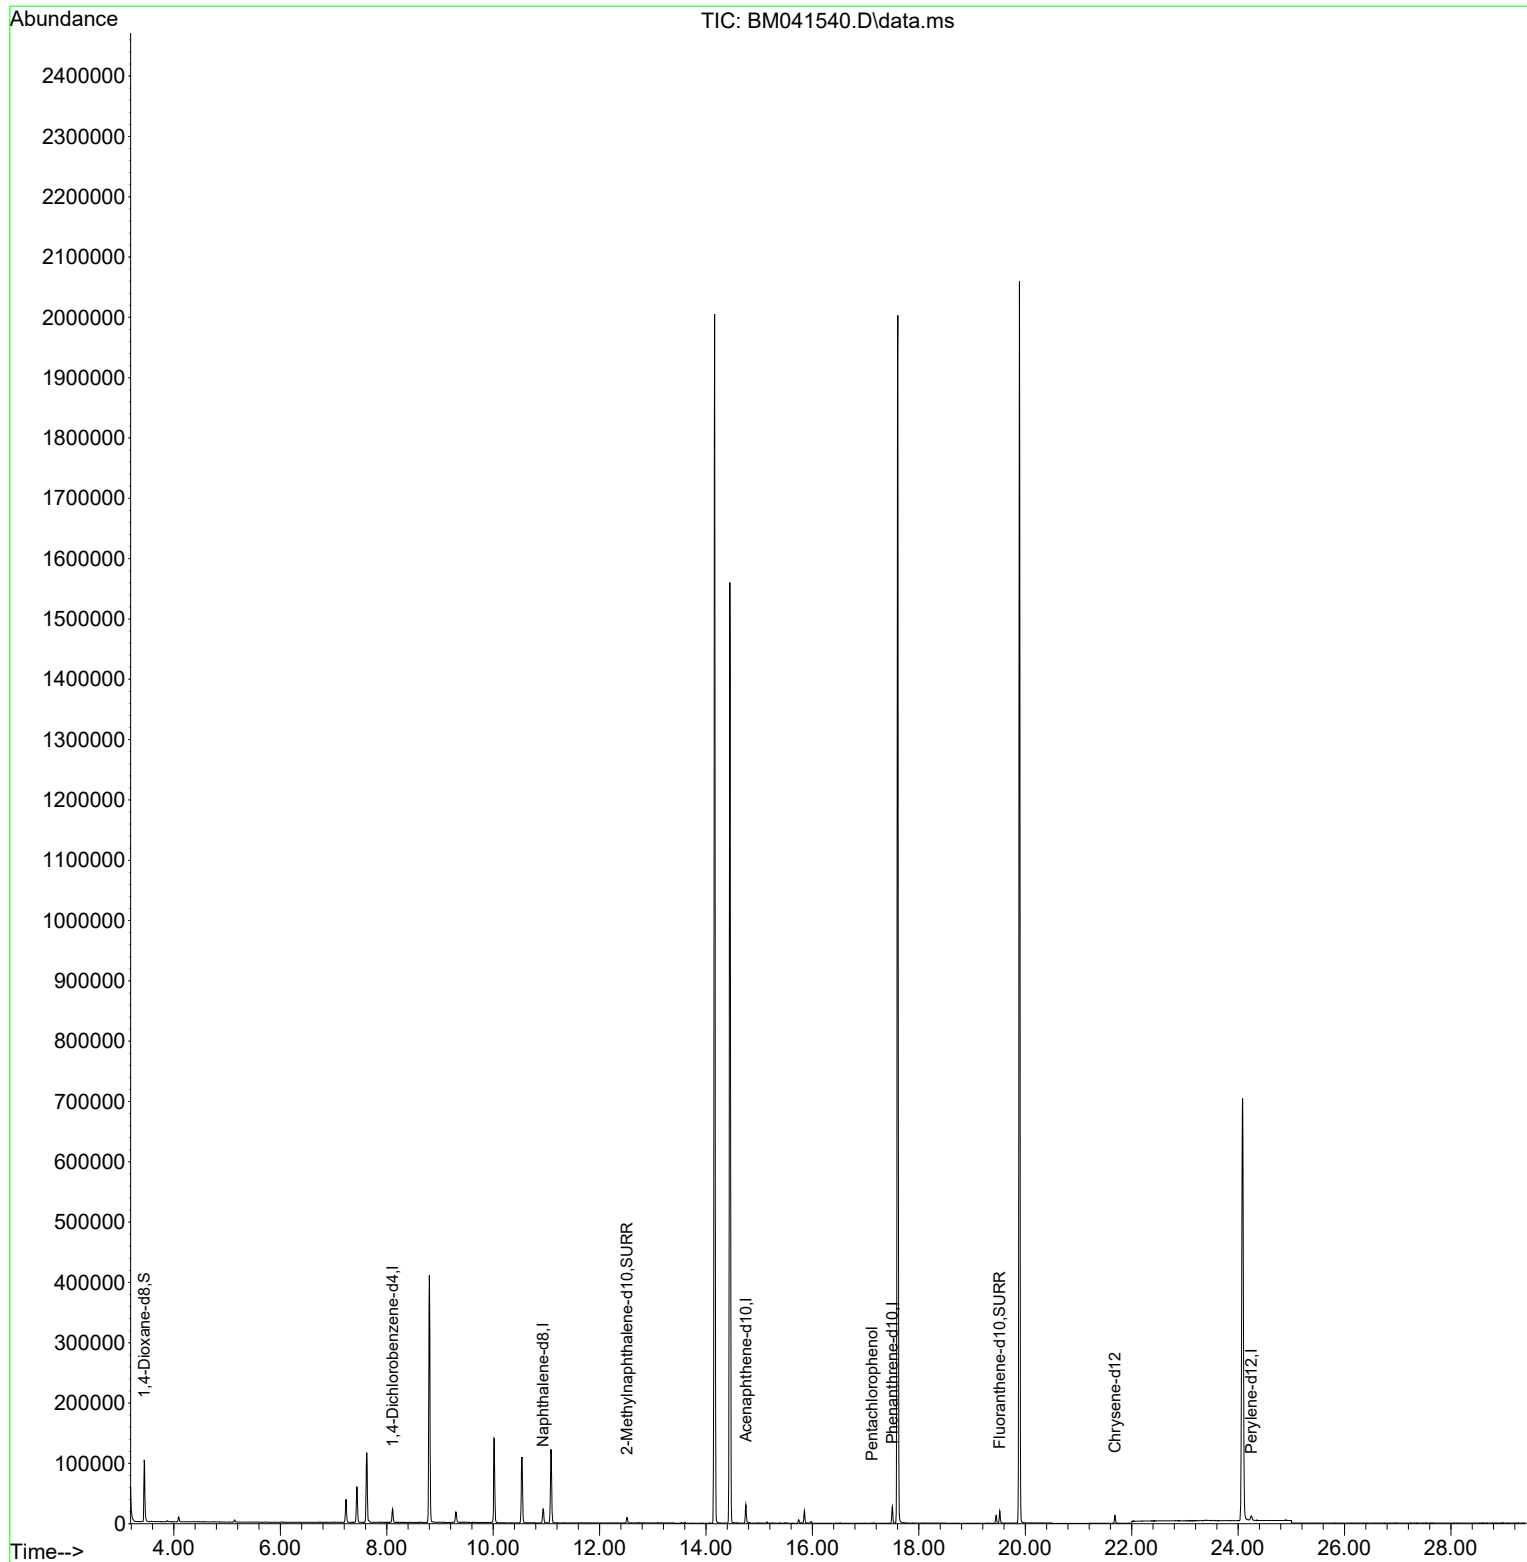

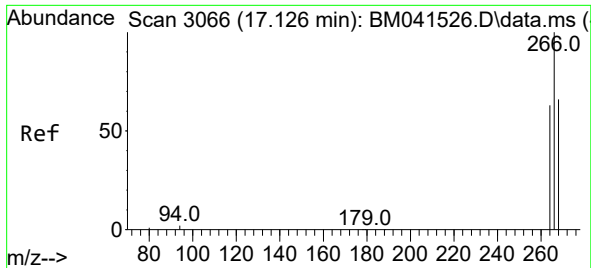

#14

Pentachlorophenol

Concen: 0.022 ng/ul

RT: 17.117 min Scan# 30

Delta R.T. -0.009 min

Lab File: BM041540.D


Acq: 29 Aug 2023 02:25

Instrument :

BNA_M

ClientSampleId :

DCHK8

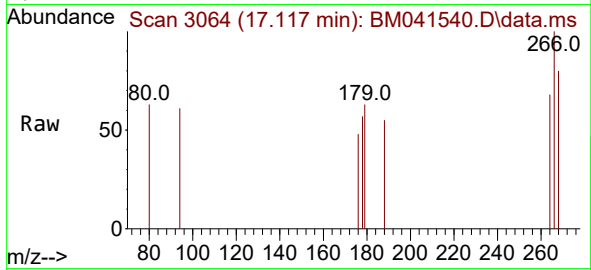

Tgt Ion:266 Resp: 258

Ion Ratio Lower Upper

266 100

264 57.8 50.0 75.0

268 70.2 51.4 77.0

