

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041546.D
 Acq On : 29 Aug 2023 06:40
 Operator : MA/JU
 Sample : 04134-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHL3

Quant Time: Aug 29 07:09:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	13562	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	37689	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	21815	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.502	188	34420	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	11320	0.400	ng/ul	0.00
23) Perylene-d12	24.245	264	12318	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	72476	4.298	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	13327	0.268	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	17632	0.381	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.126	266	466807	32.990	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041546.D
Acq On : 29 Aug 2023 06:40
Operator : MA/JU
Sample : 04134-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHL3


Quant Time: Aug 29 07:09:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

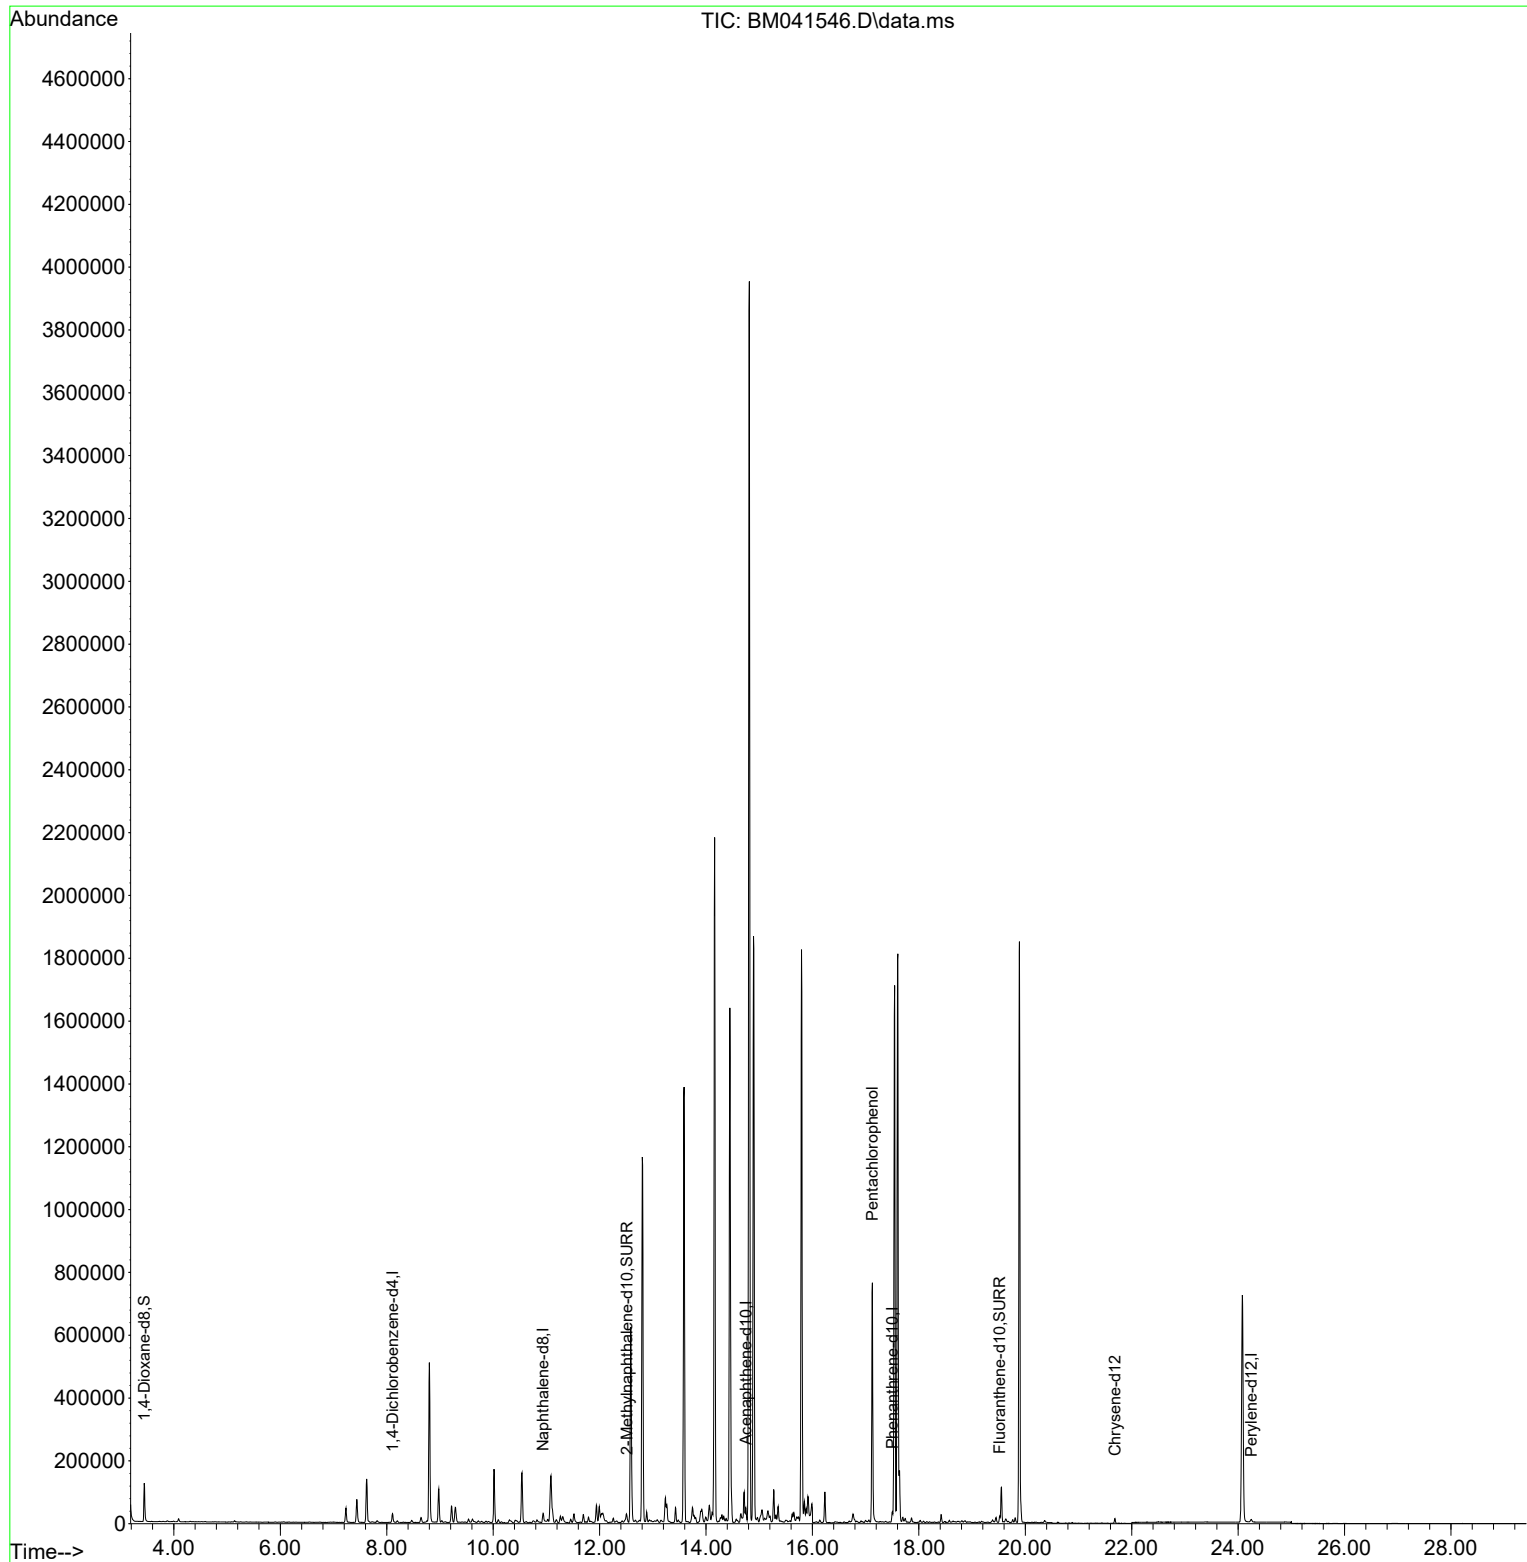

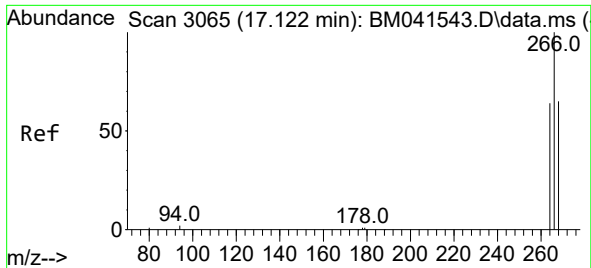

#14
Pentachlorophenol
Concen: 32.990 ng/ul
RT: 17.126 min Scan# 30
Delta R.T. -0.000 min
Lab File: BM041546.D
Acq: 29 Aug 2023 06:40

Instrument :
BNA_M
ClientSampleId :
DCHL3

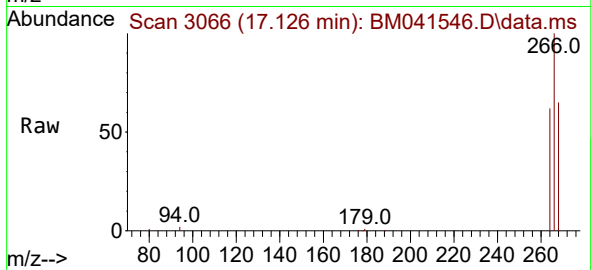

Tgt Ion:266 Resp: 466807
Ion Ratio Lower Upper
266 100
264 62.5 50.0 75.0
268 64.2 51.4 77.0

