

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041547.D
 Acq On : 29 Aug 2023 07:16
 Operator : MA/JU
 Sample : 04134-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHL8

Quant Time: Aug 29 08:09:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	11185	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	32110	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.745	164	15762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.497	188	30076	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.685	240	10175	0.400	ng/ul	# 0.00
23) Perylene-d12	24.246	264	10563	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.444	96	62050	4.462	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	9639	0.227	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	15761	0.378	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.122	266	664	0.054	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041547.D
Acq On : 29 Aug 2023 07:16
Operator : MA/JU
Sample : 04134-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHL8


Quant Time: Aug 29 08:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

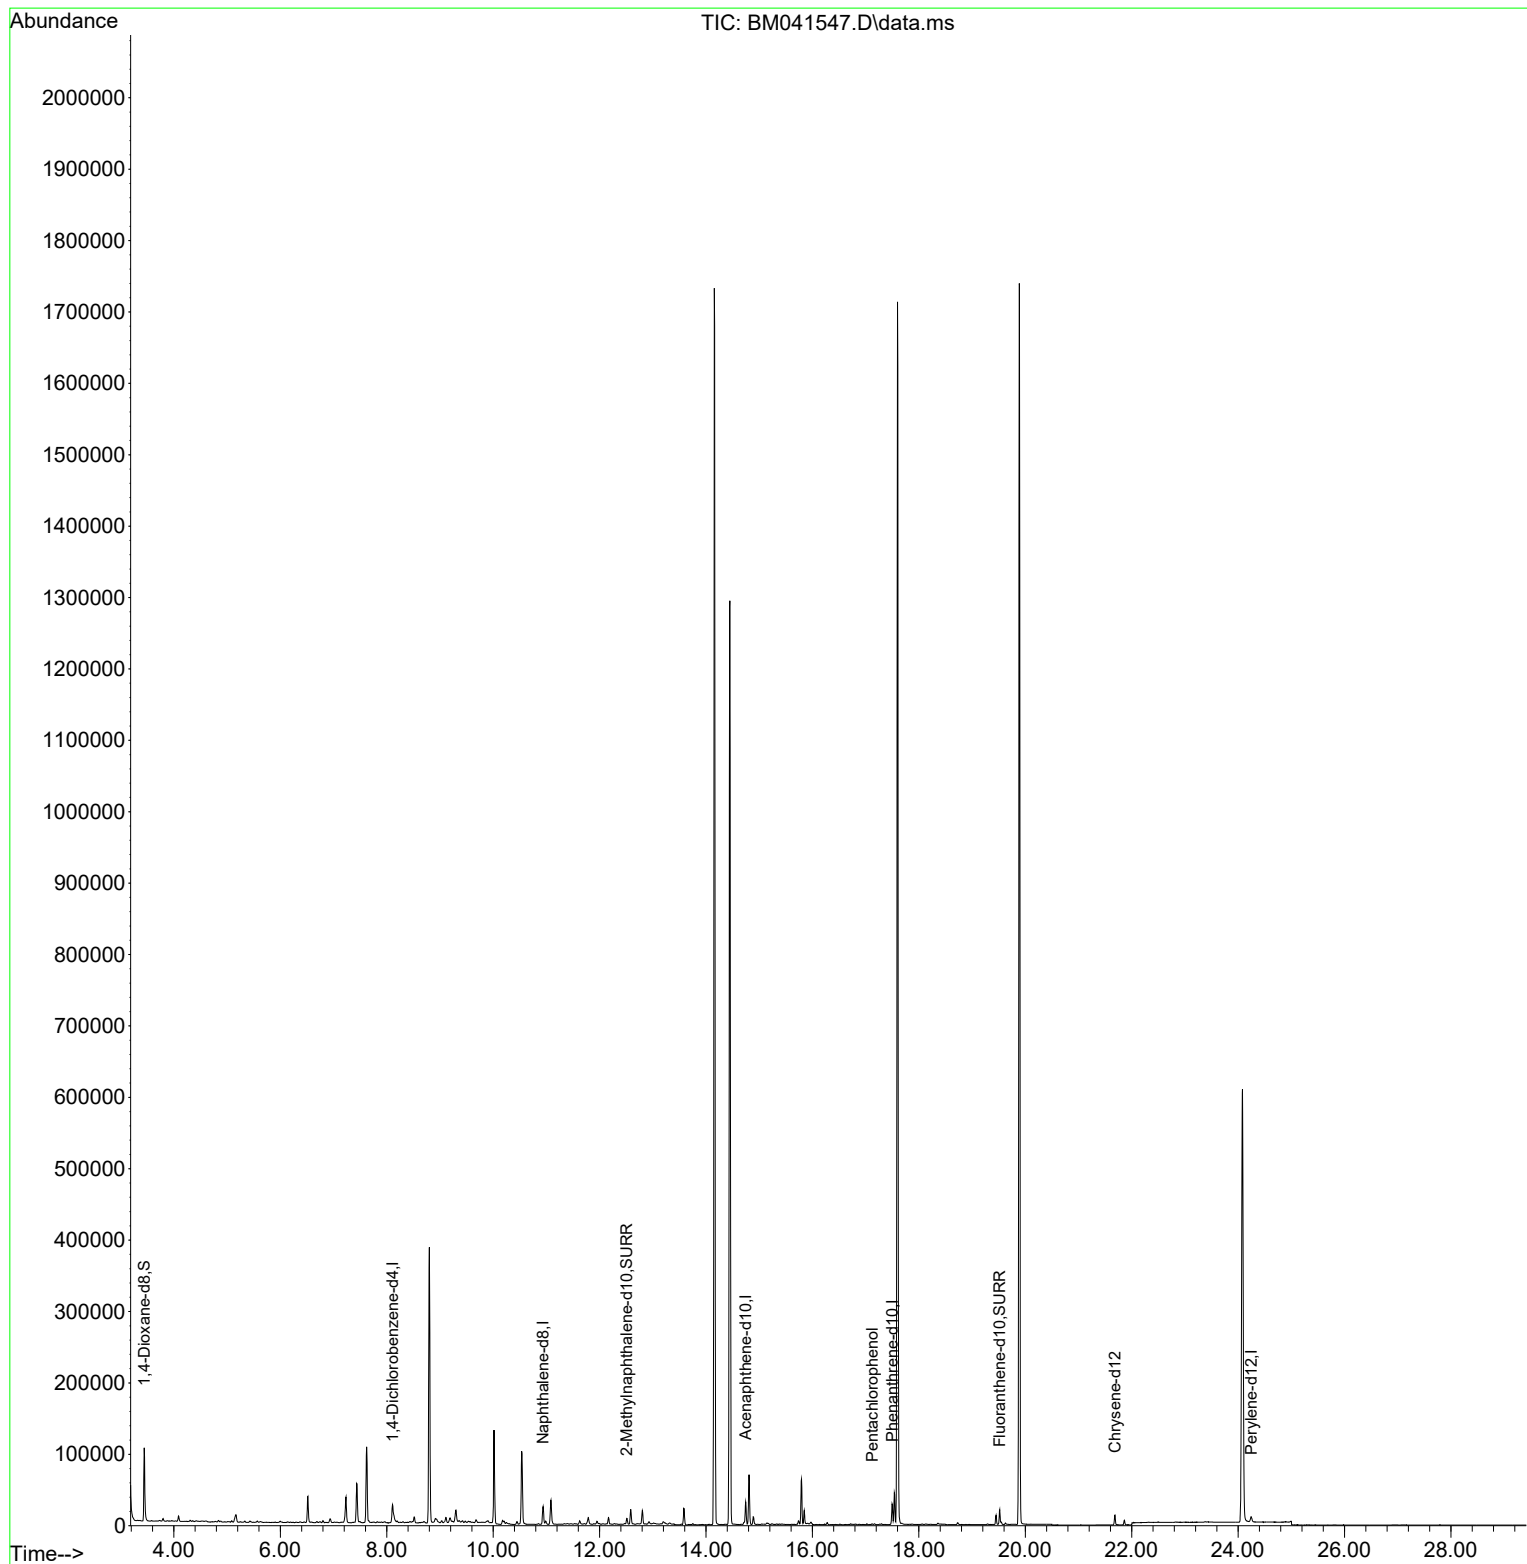

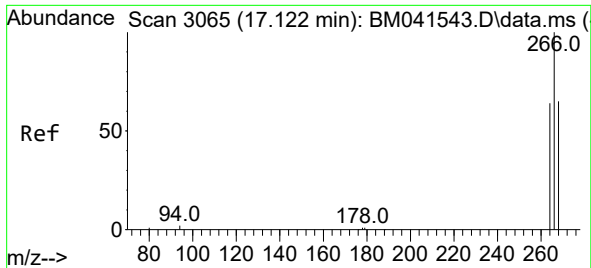

#14
 Pentachlorophenol
 Concen: 0.054 ng/ul
 RT: 17.122 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM041547.D
 Acq: 29 Aug 2023 07:16

Instrument :
 BNA_M
 ClientSampleId :
 DCHL8

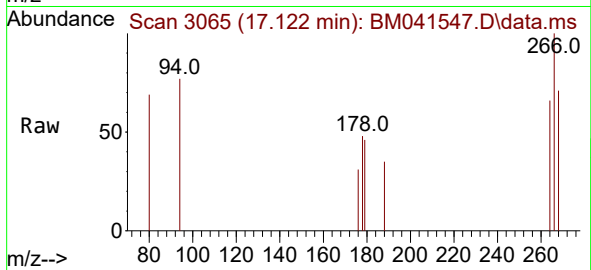

Tgt Ion:	266	Resp:	664
Ion	Ratio	Lower	Upper
266	100		
264	62.7	50.0	75.0
268	64.8	51.4	77.0

