

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041555.D
 Acq On : 29 Aug 2023 12:09
 Operator : MA/JU
 Sample : 04123-21
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHAU3

Quant Time: Aug 29 23:48:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	12800	0.400	ng/ul	0.00
4) Naphthalene-d8	10.939	136	32223	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.745	164	13899	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.498	188	24922	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.688	240	9767	0.400	ng/ul	# 0.00
23) Perylene-d12	24.251	264	12186	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	76251	4.791	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	13534	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	17385	0.435	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.482	88	26137	1.585	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041555.D
Acq On : 29 Aug 2023 12:09
Operator : MA/JU
Sample : 04123-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHAU3

Quant Time: Aug 29 23:48:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration

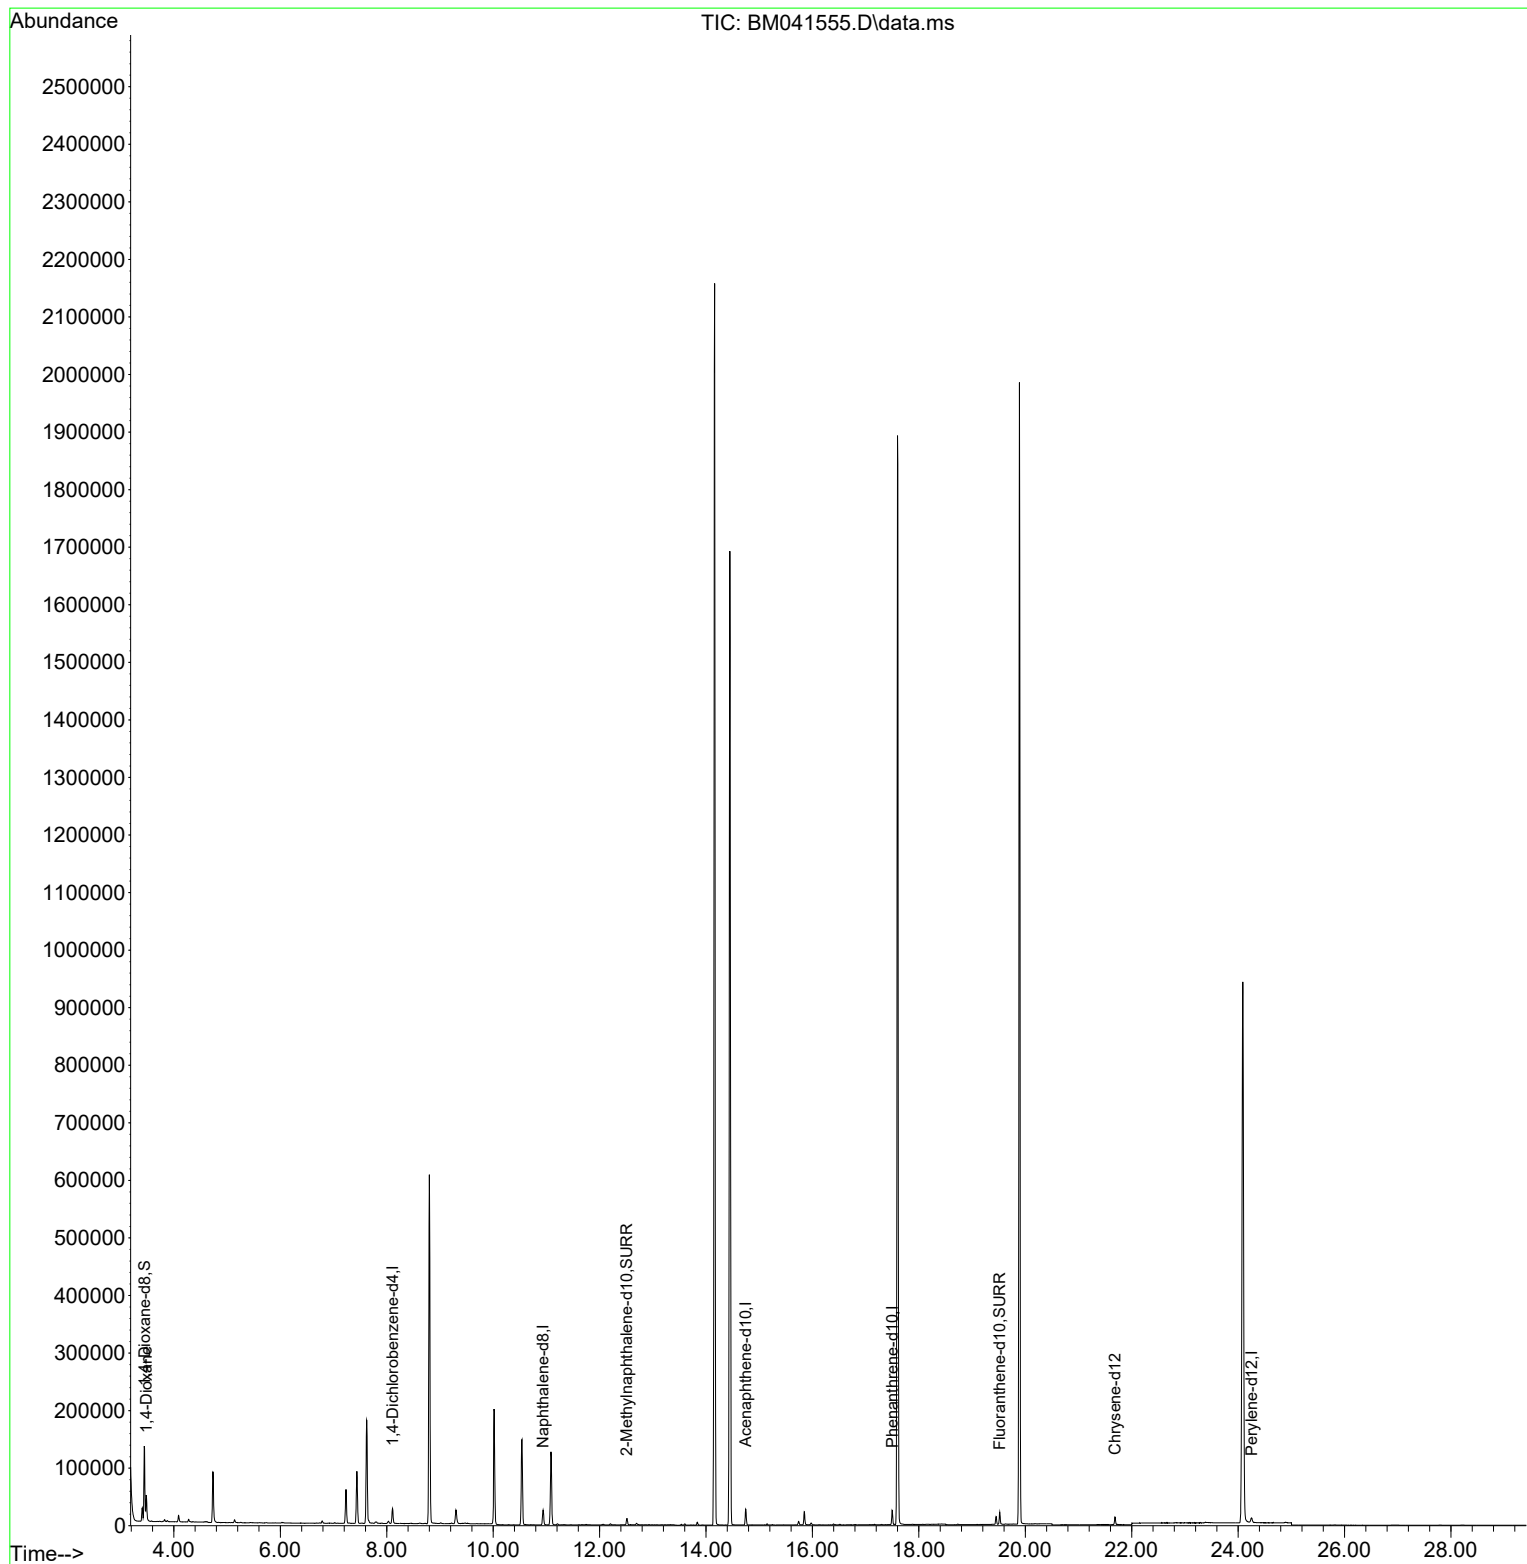

Abundance Scan 72 (3.486 min): BM041543.D\data.ms (-63)

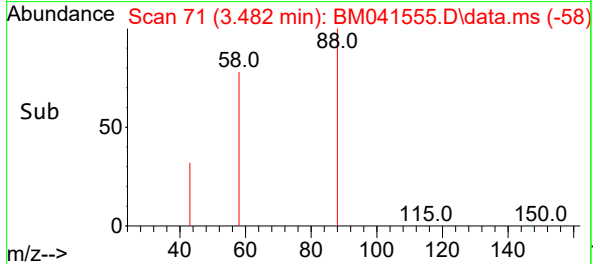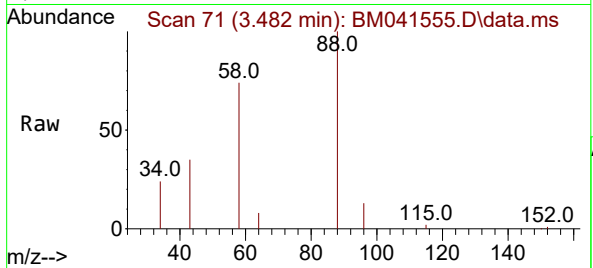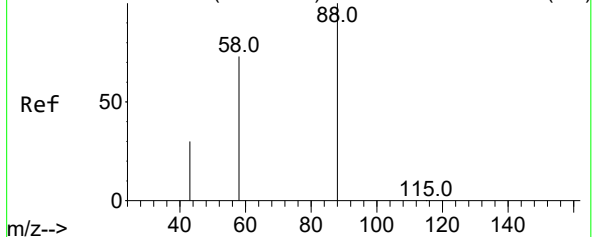

#2
1,4-Dioxane
Concen: 1.585 ng/ul
RT: 3.482 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM041555.D
Acq: 29 Aug 2023 12:09

Instrument :
BNA_M
ClientSampleId :
BHAU3

Tgt Ion:	88	Resp:	26137
Ion	Ratio	Lower	Upper
88	100		
43	34.8	30.6	46.0
58	74.4	49.3	73.9#

