

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
 Data File : BM041556.D
 Acq On : 29 Aug 2023 12:46
 Operator : MA/JU
 Sample : 04123-22
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9Q5

Quant Time: Aug 29 23:48:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 15:20:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	12289	0.400	ng/ul	0.00
4) Naphthalene-d8	10.939	136	31425	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.745	164	15510	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.498	188	25211	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.685	240	9212	0.400	ng/ul	# 0.00
23) Perylene-d12	24.251	264	11482	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	83702	5.478	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	12621	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	17190	0.456	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.482	88	5624	0.355	ng/ul	94
20) Pyrene	19.919	202	7581	0.088	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082823\
Data File : BM041556.D
Acq On : 29 Aug 2023 12:46
Operator : MA/JU
Sample : 04123-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9Q5

Quant Time: Aug 29 23:48:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 15:20:06 2023
Response via : Initial Calibration




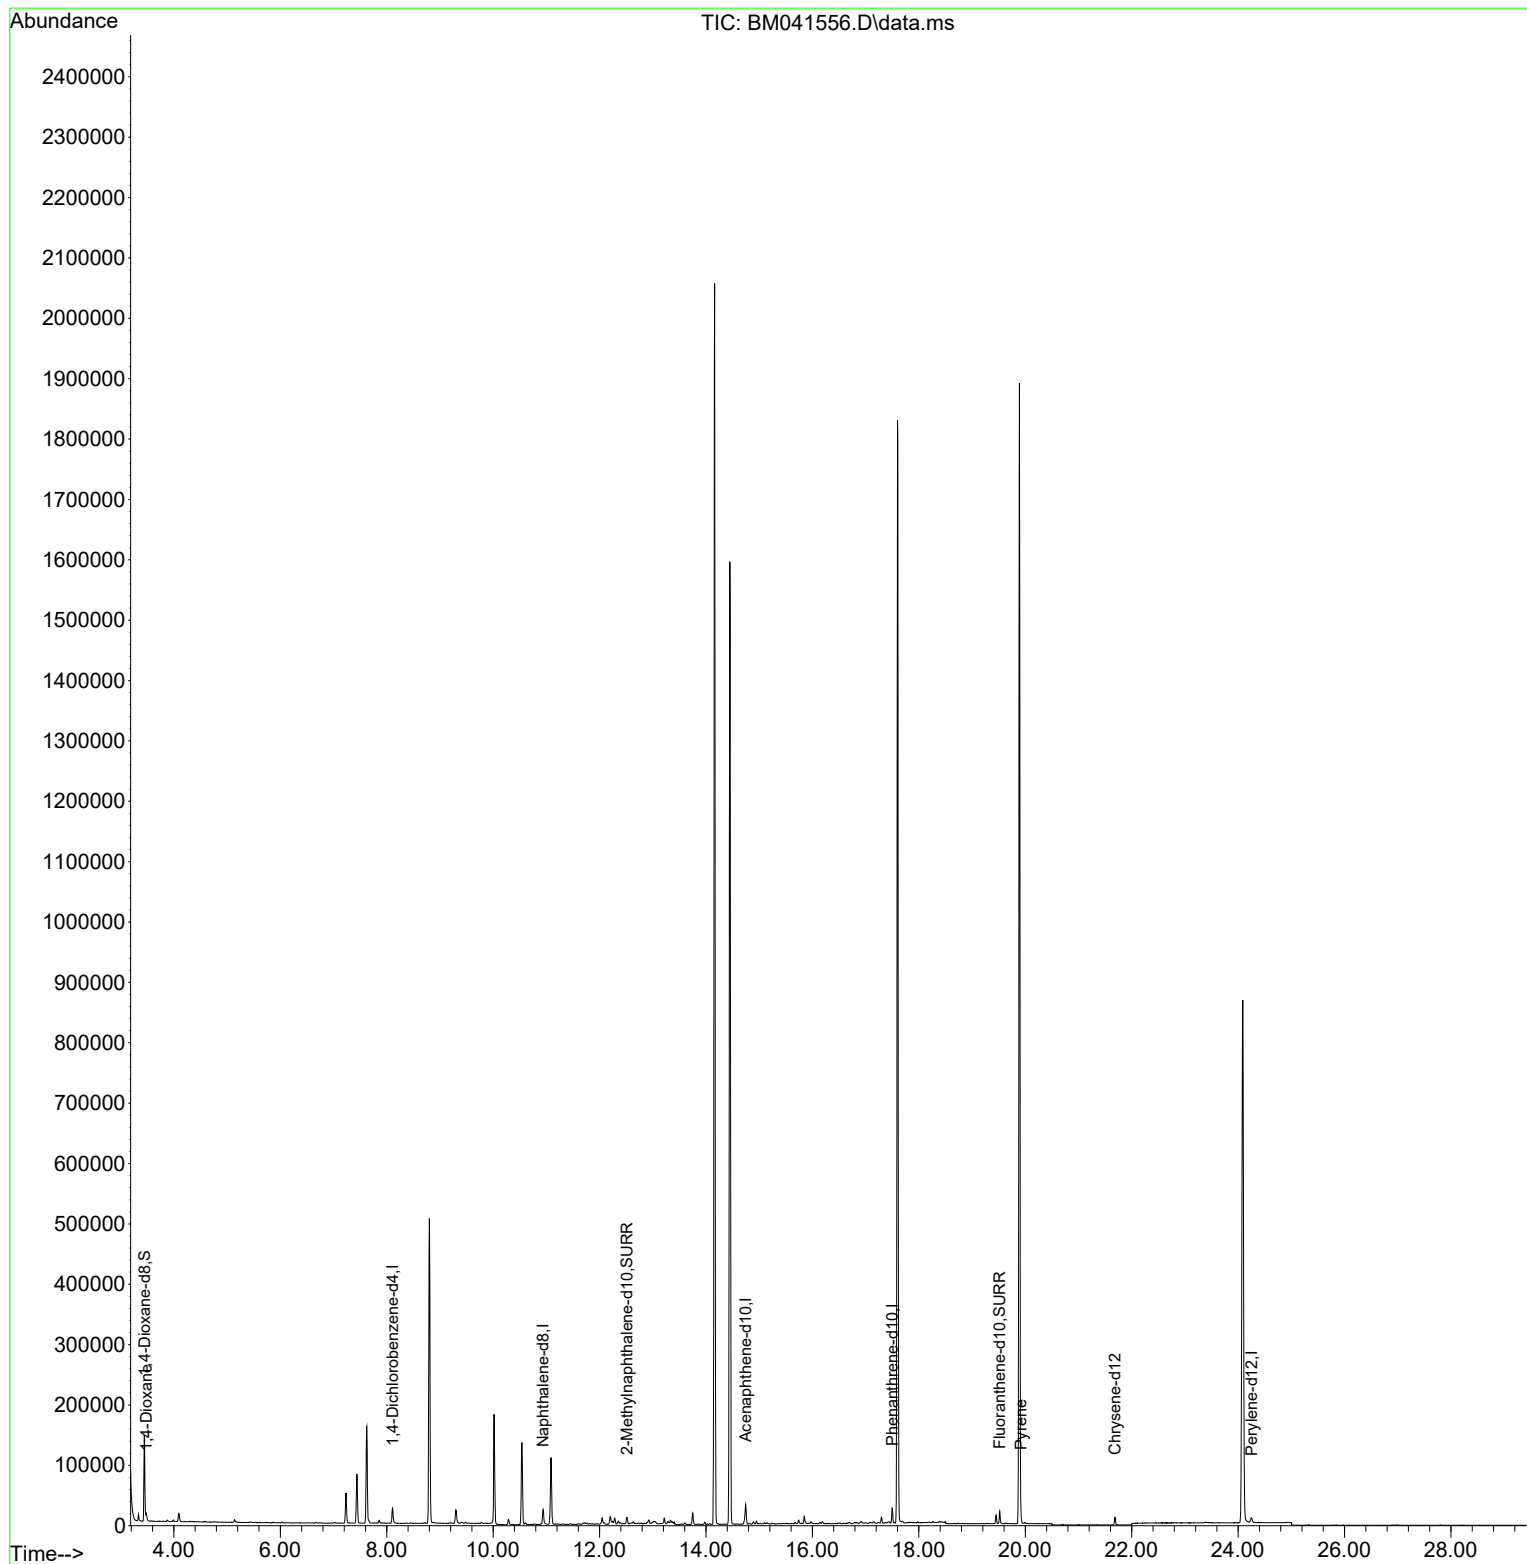


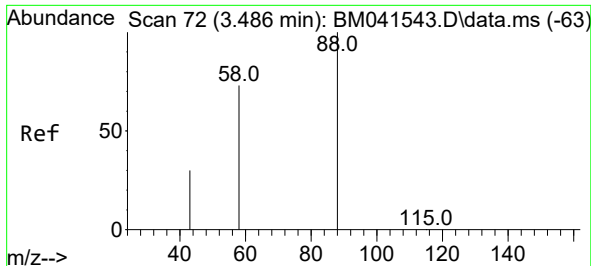

#2
1,4-Dioxane
Concen: 0.355 ng/ul
RT: 3.482 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM041556.D
Acq: 29 Aug 2023 12:46

Instrument :
BNA_M
ClientSampleId :
BH9Q5

Tgt Ion: 88 Resp: 5624
Ion Ratio Lower Upper
88 100
43 45.4 30.6 46.0
58 64.1 49.3 73.9

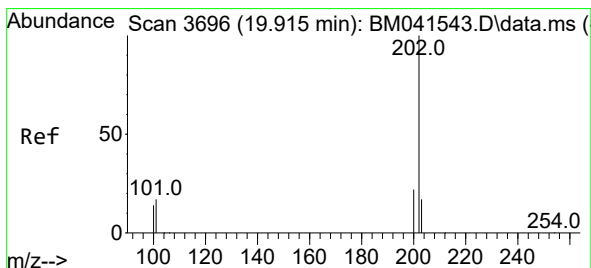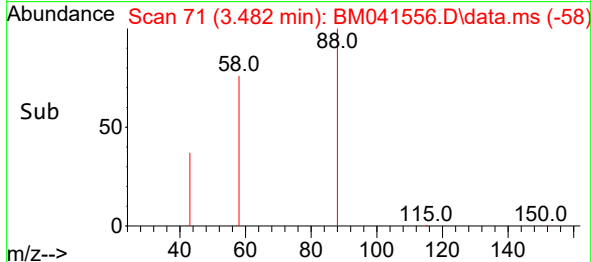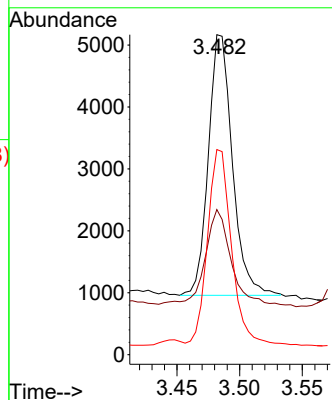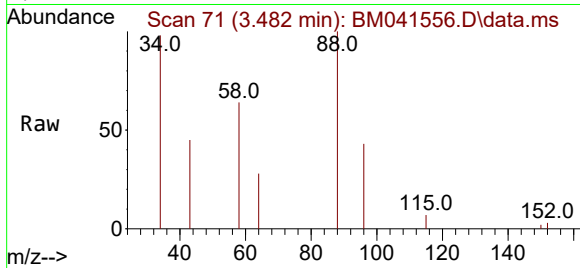

#20
Pyrene
Concen: 0.088 ng/ul
RT: 19.919 min Scan# 3697
Delta R.T. -0.005 min
Lab File: BM041556.D
Acq: 29 Aug 2023 12:46

Tgt Ion: 202 Resp: 7581
Ion Ratio Lower Upper
202 100
101 18.7 11.6 17.4#
100 16.2 9.1 13.7#

