

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082824\
 Data File : BM047380.D
 Acq On : 28 Aug 2024 14:24
 Operator : RC/JU
 Sample : P3735-01DL 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-11DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 28 15:01:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 26 18:11:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.345	152	360757	20.000	ng	0.00
21) Naphthalene-d8	10.104	136	1361596	20.000	ng	0.00
39) Acenaphthene-d10	14.010	164	895749	20.000	ng	0.00
64) Phenanthrene-d10	16.774	188	1683446	20.000	ng	0.00
76) Chrysene-d12	21.021	240	1280743	20.000	ng	0.00
86) Perylene-d12	23.727	264	1403597	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.004	112	705949	37.543	ng	0.00
7) Phenol-d6	6.569	99	964615	37.658	ng	0.00
23) Nitrobenzene-d5	8.498	82	624905	25.465	ng	0.00
42) 2,4,6-Tribromophenol	15.521	330	402707	37.263	ng	0.00
45) 2-Fluorobiphenyl	12.616	172	1444417	24.776	ng	0.00
79) Terphenyl-d14	19.444	244	1617095	22.474	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	10.151	128	308100	4.633	ng	100
37) 2-Methylnaphthalene	11.780	142	239903	4.948	ng	100
38) 1-Methylnaphthalene	12.004	142	256598	5.351	ng	97
49) Acenaphthylene	13.727	152	249871	3.508	ng	97
52) Acenaphthene	14.074	154	93869	2.076	ng	99
55) Dibenzofuran	14.415	168	183516	2.519	ng	# 95
58) Fluorene	15.074	166	482983	8.193	ng	100
71) Phenanthrene	16.821	178	3746968	45.831	ng	99
72) Anthracene	16.909	178	830765	10.424	ng	99
73) Carbazole	17.198	167	297123	3.885	ng	99
75) Fluoranthene	18.856	202	3013123	31.388	ng	100
78) Pyrene	19.227	202	2842796	28.940	ng	100
81) Benzo(a)anthracene	21.003	228	1439765	17.238	ng	98
83) Chrysene	21.062	228	1348178m	17.160	ng	
87) Indeno(1,2,3-cd)pyrene	26.720	276	635002	7.227	ng	97
88) Benzo(b)fluoranthene	22.885	252	1391423	16.992	ng	99
89) Benzo(k)fluoranthene	22.933	252	562243m	7.243	ng	
90) Benzo(a)pyrene	23.597	252	1101866	15.560	ng	98
91) Dibenzo(a,h)anthracene	26.762	278	229193	3.220	ng	# 88
92) Benzo(g,h,i)perylene	27.662	276	619822	8.376	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082824\
Data File : BM047380.D
Acq On : 28 Aug 2024 14:24
Operator : RC/JU
Sample : P3735-01DL 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-11DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

Quant Time: Aug 28 15:01:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

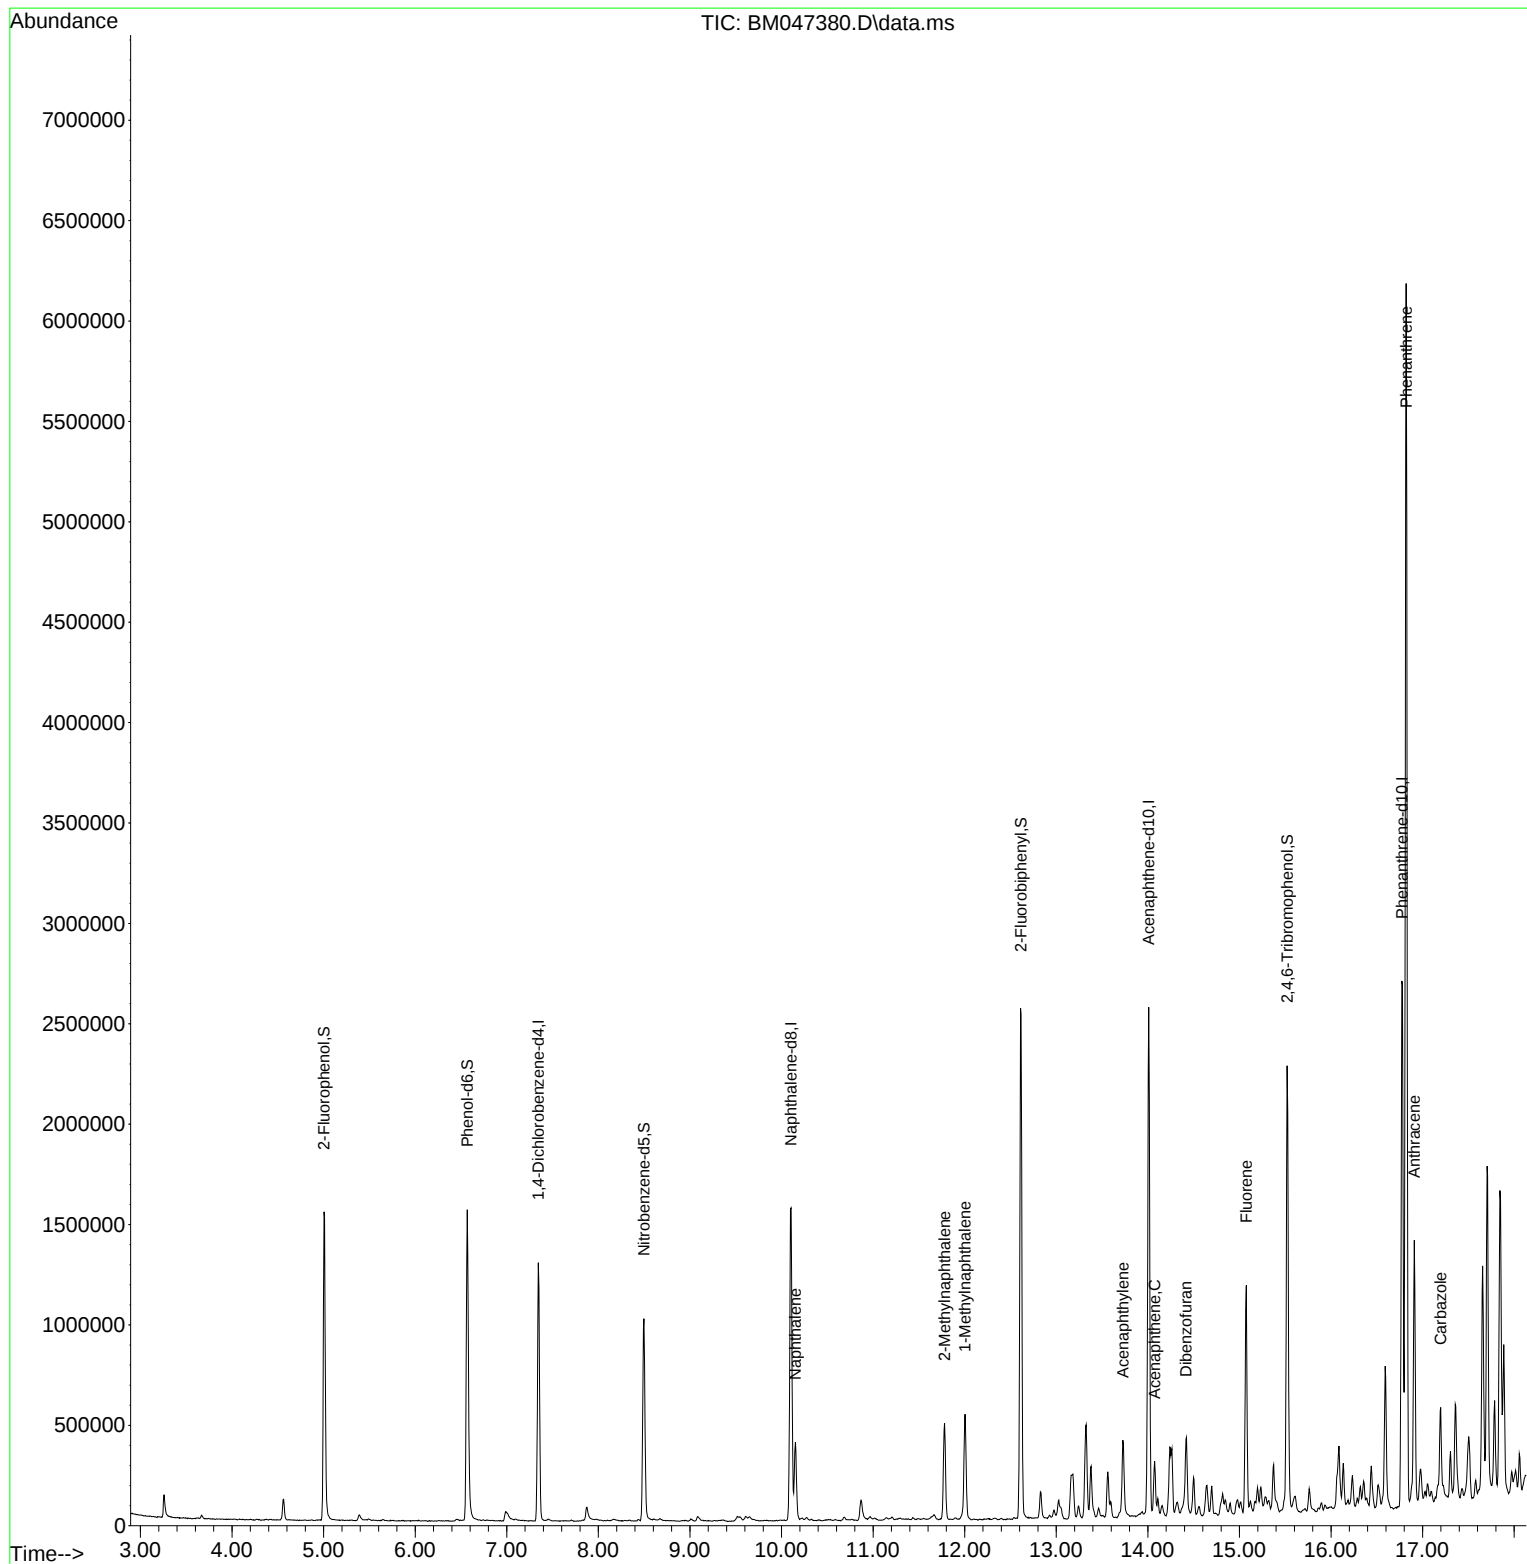


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082824\
Data File : BM047380.D
Acq On : 28 Aug 2024 14:24
Operator : RC/JU
Sample : P3735-01DL 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
WC-11DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024


Quant Time: Aug 28 15:01:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

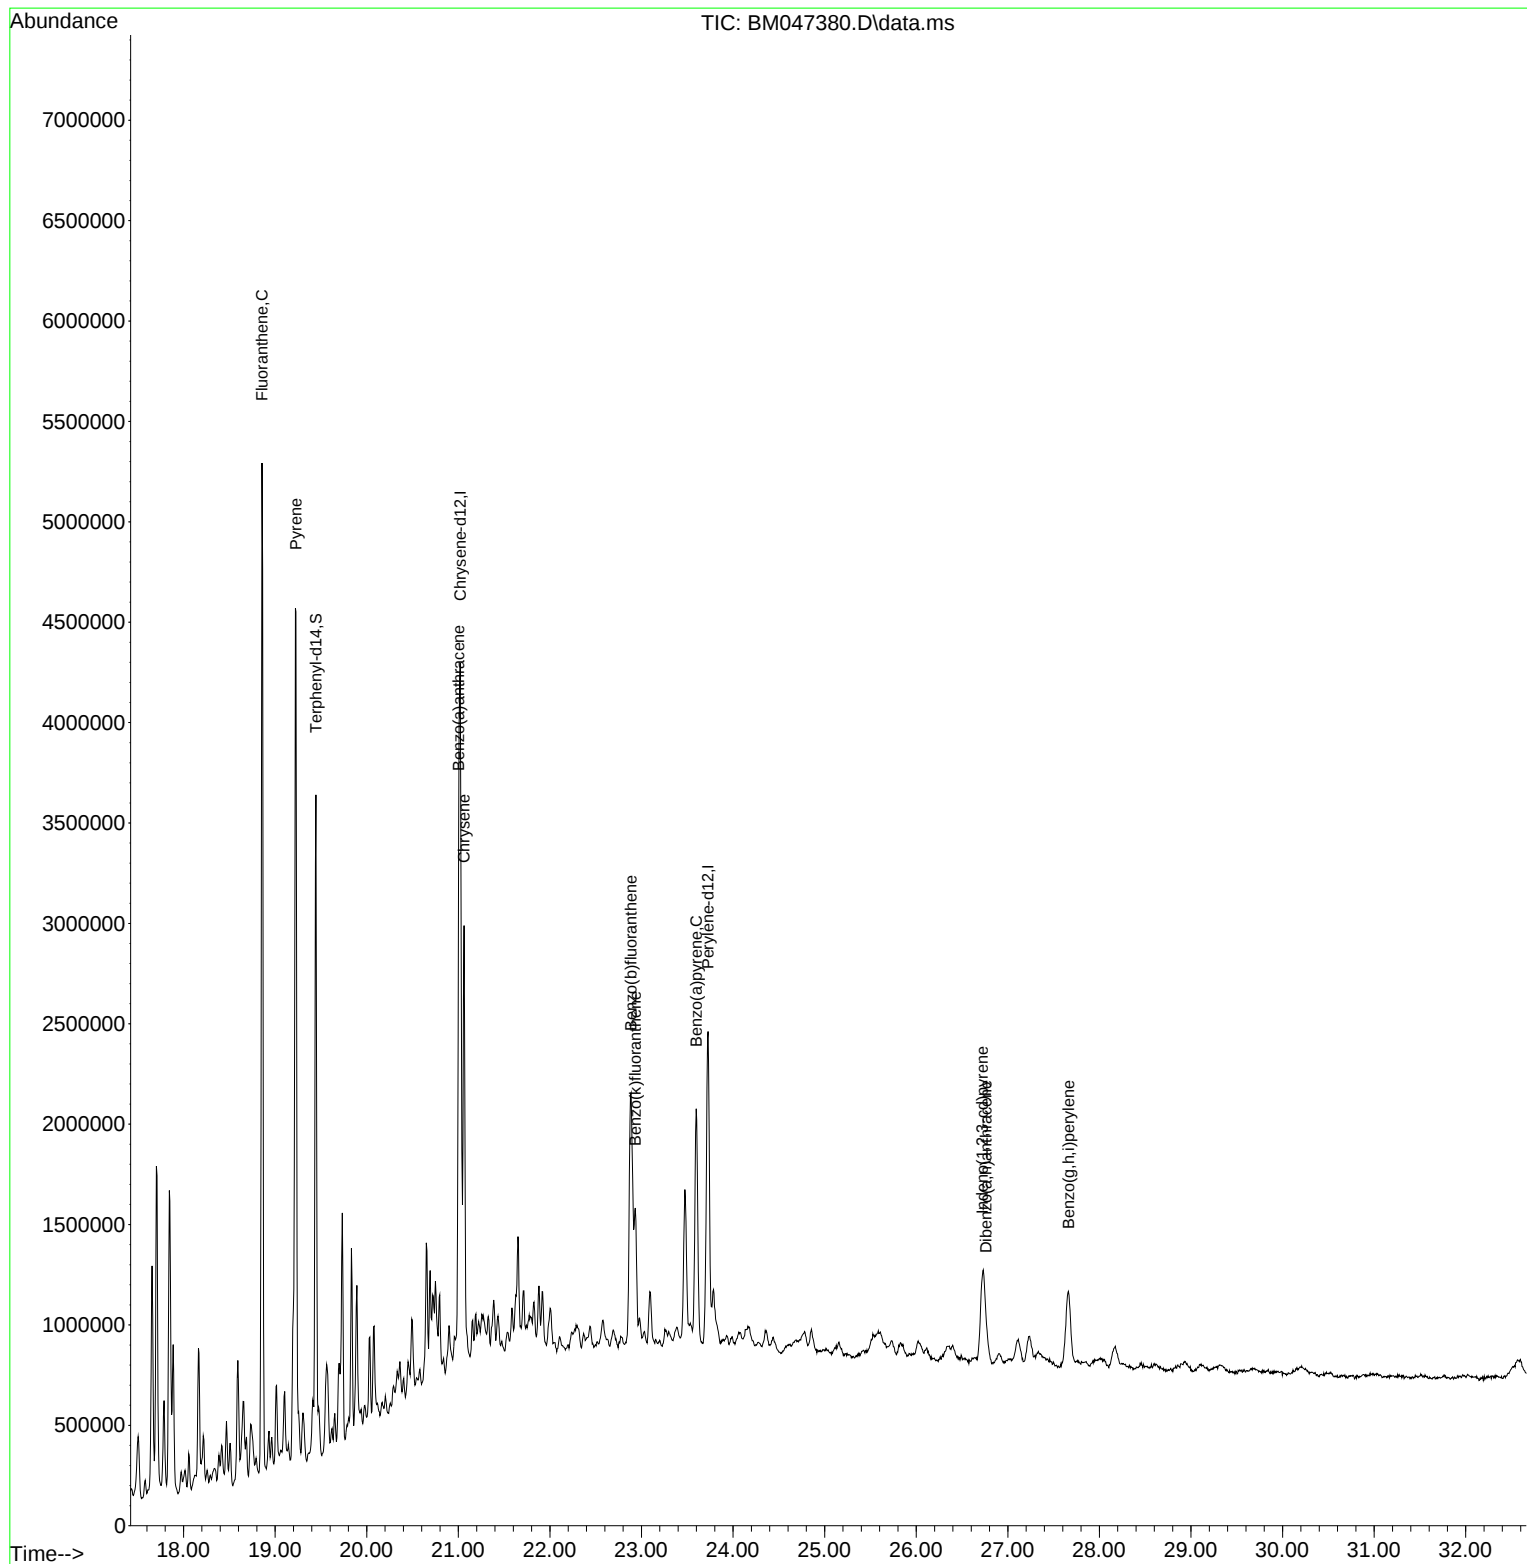



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.345 min Scan# 71
Delta R.T. -0.006 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL

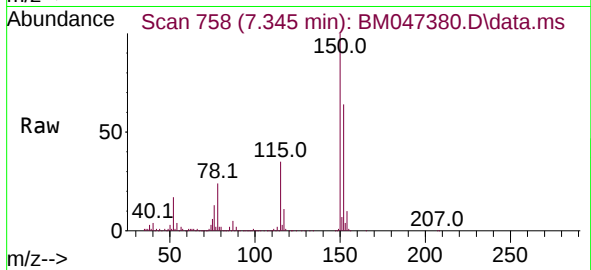

Tgt Ion:152 Resp: 36075
Ion Ratio Lower Upper
152 100
150 155.3 121.3 181.9
115 53.8 42.6 64.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024



#5
2-Fluorophenol
Concen: 37.543 ng
RT: 5.004 min Scan# 360
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24


Tgt Ion:112 Resp: 705949
Ion Ratio Lower Upper
112 100
64 56.0 45.7 68.5
63 29.2 23.8 35.8

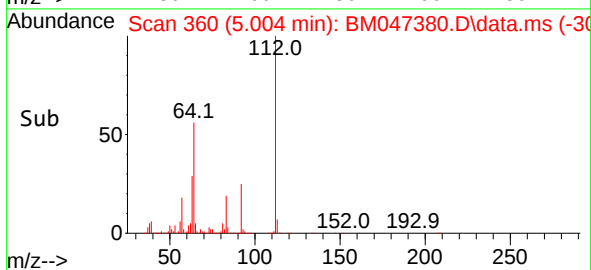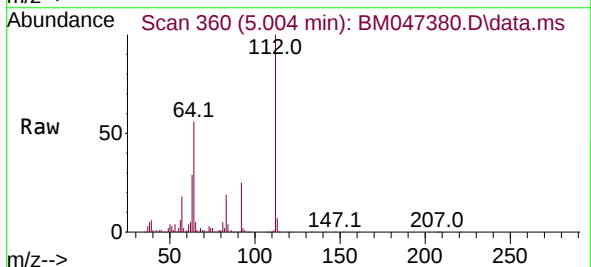



#7
Phenol-d6
Concen: 37.658 ng
RT: 6.569 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL




Tgt Ion: 99 Resp: 964615
Ion Ratio Lower Upper
99 100
42 16.1 13.0 19.4
71 34.5 27.5 41.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

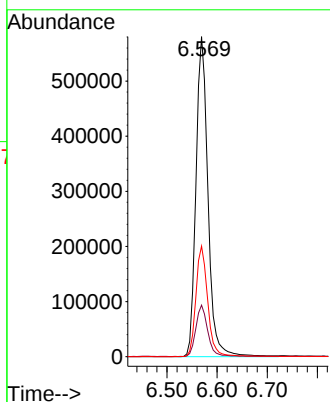


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.104 min Scan# 1227
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Tgt Ion:136 Resp: 1361596
Ion Ratio Lower Upper
136 100
137 10.9 8.8 13.2
54 6.7 5.2 7.8
68 5.8 4.6 6.8

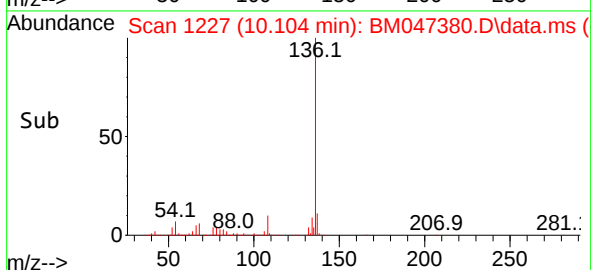



#23
Nitrobenzene-d5
Concen: 25.465 ng
RT: 8.498 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL




Tgt Ion: 82 Resp: 62490
Ion Ratio Lower Upper
82 100
128 43.0 34.6 51.8
54 43.7 35.5 53.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024




#31
Naphthalene
Concen: 4.633 ng
RT: 10.151 min Scan# 1235
Delta R.T. -0.006 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24

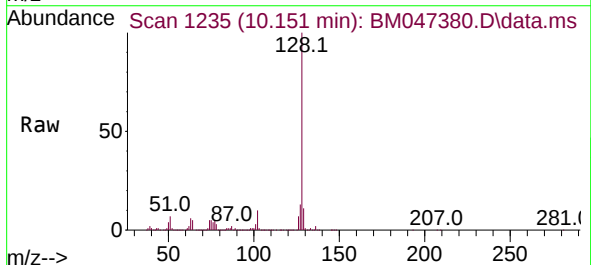

Tgt Ion:128 Resp: 308100
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.6
127 13.0 10.4 15.6

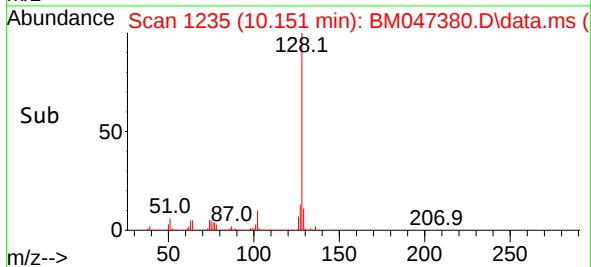







#37
2-Methylnaphthalene
Concen: 4.948 ng
RT: 11.780 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24

Instrument :
BNA_M
ClientSampleId :
WC-11DL

Tgt Ion:142 Resp: 23990
Ion Ratio Lower Upper
142 100
141 88.3 70.8 106.2
115 34.6 27.5 41.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

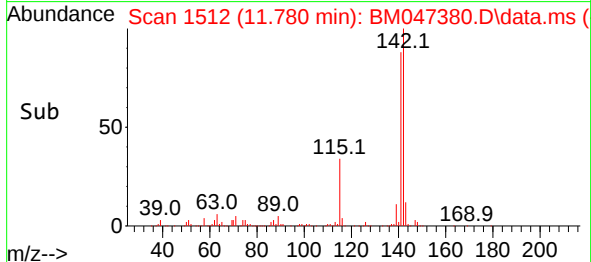

#38
1-Methylnaphthalene
Concen: 5.351 ng
RT: 12.004 min Scan# 1550
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24


Tgt Ion:142 Resp: 256598
Ion Ratio Lower Upper
142 100
141 93.8 72.9 109.3
116 3.6 3.0 4.6

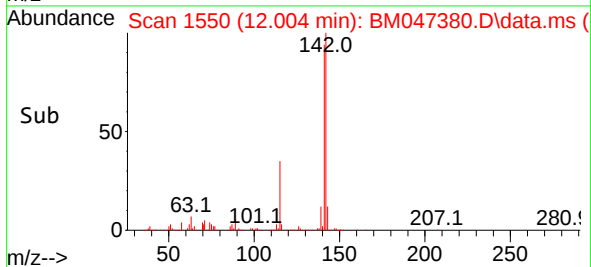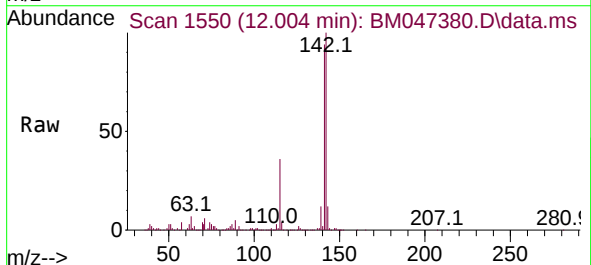



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.010 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL




Tgt Ion:164 Resp: 895749
Ion Ratio Lower Upper
164 100
162 99.8 79.7 119.5
160 43.9 34.9 52.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024




#42
2,4,6-Tribromophenol
Concen: 37.263 ng
RT: 15.521 min Scan# 2148
Delta R.T. -0.006 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24

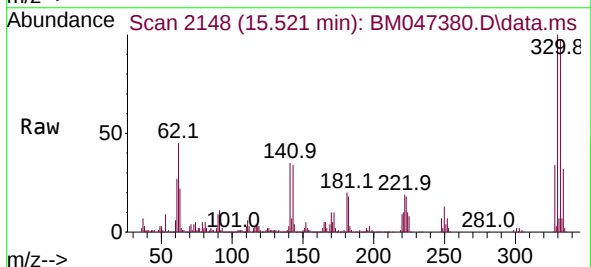


Tgt Ion:330 Resp: 402707
Ion Ratio Lower Upper
330 100
332 95.9 77.2 115.8
141 33.8 27.6 41.4

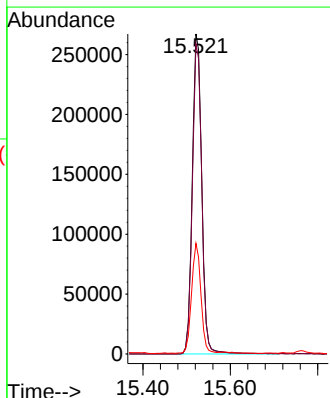



#45
2-Fluorobiphenyl
Concen: 24.776 ng
RT: 12.616 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL




Tgt Ion:172 Resp: 144441
Ion Ratio Lower Upper
172 100
171 34.7 27.8 41.6
170 23.3 18.5 27.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

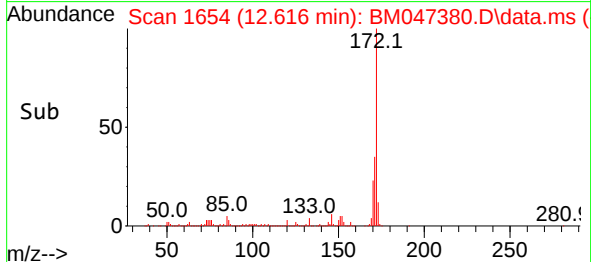


#49
Acenaphthylene
Concen: 3.508 ng
RT: 13.727 min Scan# 1843
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24



Tgt Ion:152 Resp: 249871
Ion Ratio Lower Upper
152 100
151 19.1 15.4 23.0
153 15.8 10.6 15.8

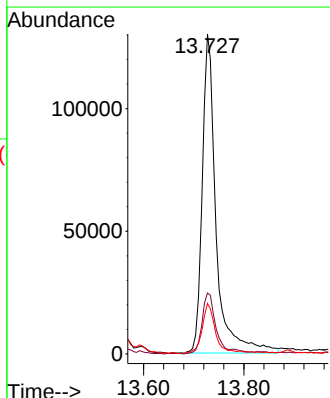







#52
Acenaphthene
Concen: 2.076 ng
RT: 14.074 min Scan# 1903
Delta R.T. -0.006 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24

Instrument :
BNA_M
ClientSampleId :
WC-11DL

Tgt Ion:154 Resp: 93869
Ion Ratio Lower Upper
154 100
153 110.3 89.5 134.3
152 53.9 43.0 64.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

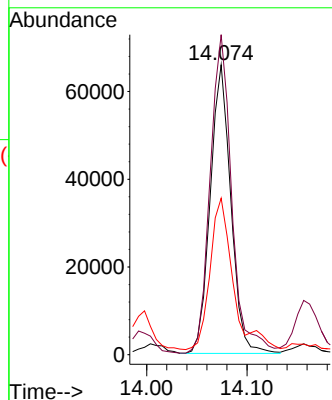

#55
Dibenzofuran
Concen: 2.519 ng
RT: 14.415 min Scan# 1960
Delta R.T. -0.006 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24

Tgt Ion:168 Resp: 183516
Ion Ratio Lower Upper
168 100
139 35.8 27.5 41.3
169 17.5 10.5 15.7#

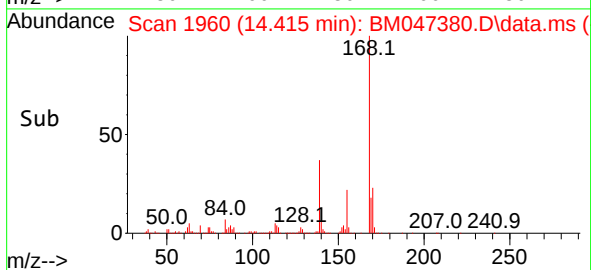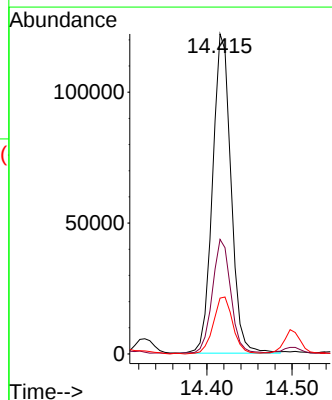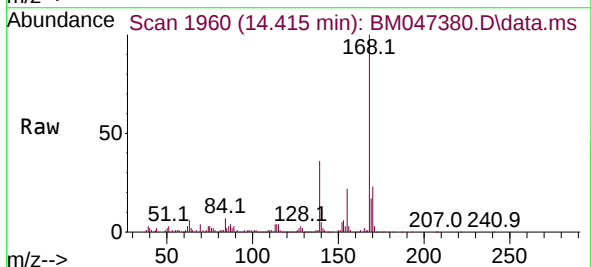



#58

Fluorene

Concen: 8.193 ng

RT: 15.074 min Scan# 2072

Delta R.T. -0.000 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Instrument :

BNA_M

ClientSampleId :





WC-11DL

Tgt Ion:166 Resp: 482983
 Ion Ratio Lower Upper
 166 100
 165 97.1 77.8 116.6
 167 15.1 11.1 16.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

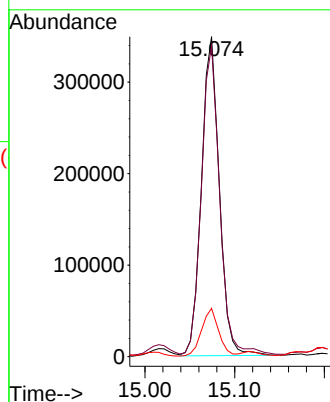

#64

Phenanthrene-d10

Concen: 20.000 ng




RT: 16.774 min Scan# 2361


Delta R.T. -0.000 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24


Tgt Ion:188 Resp: 1683446
 Ion Ratio Lower Upper
 188 100
 94 8.2 6.4 9.6
 80 9.3 7.4 11.2

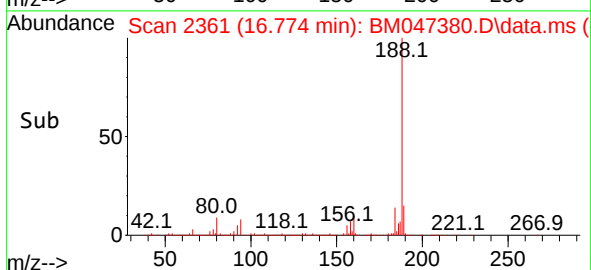



#71
Phenanthrene
Concen: 45.831 ng
RT: 16.821 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL




Tgt Ion:178 Resp: 3746968
Ion Ratio Lower Upper
178 100
176 19.3 15.2 22.8
179 15.6 12.2 18.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

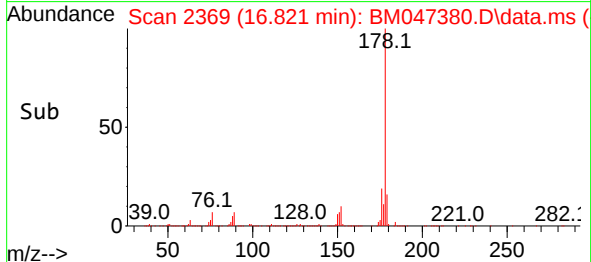


#72
Anthracene
Concen: 10.424 ng
RT: 16.909 min Scan# 2384
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Tgt Ion:178 Resp: 830765
Ion Ratio Lower Upper
178 100
176 18.2 14.7 22.1
179 15.2 12.6 18.8

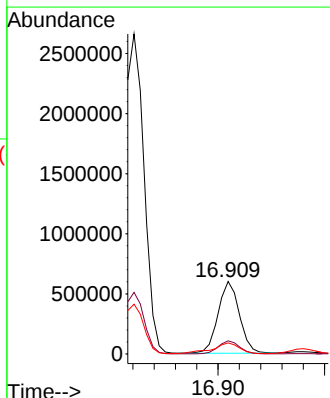



#73
 Carbazole
 Concen: 3.885 ng
 RT: 17.198 min Scan# 2433
 Delta R.T. -0.000 min
 Lab File: BM047380.D
 Acq: 28 Aug 2024 14:24




Instrument :
 BNA_M
 ClientSampleId :
 WC-11DL



Tgt Ion:167 Resp: 297123
 Ion Ratio Lower Upper
 167 100
 166 21.7 16.9 25.3
 139 11.6 9.5 14.3




Manual Integrations
 APPROVED


Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

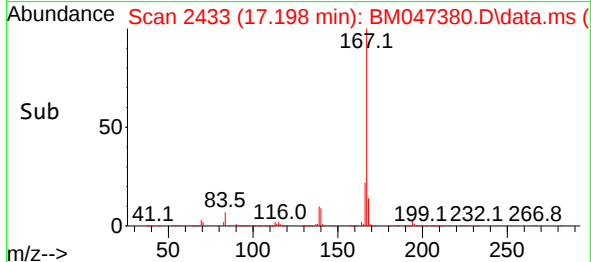

#75
 Fluoranthene
 Concen: 31.388 ng
 RT: 18.856 min Scan# 2715
 Delta R.T. -0.000 min
 Lab File: BM047380.D
 Acq: 28 Aug 2024 14:24

Tgt Ion:202 Resp: 3013123
 Ion Ratio Lower Upper
 202 100
 101 9.2 0.0 29.0
 203 17.6 0.0 37.5

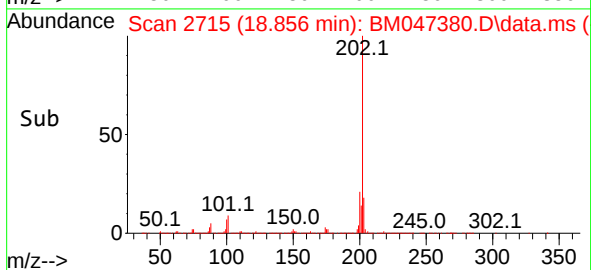



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.021 min Scan# 3083

Delta R.T. -0.000 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Instrument :

BNA_M

ClientSampleId :

WC-11DL

Tgt Ion:240 Resp: 128074

Ion Ratio Lower Upper

240 100

120 9.3 7.4 11.0





236 25.7 20.8 31.2

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024

Supervised By :mohammad ahmed 08/30/2024



#78

Pyrene

Concen: 28.940 ng

RT: 19.227 min Scan# 2778

Delta R.T. 0.006 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24




Tgt Ion:202 Resp: 2842796


Ion Ratio Lower Upper

202 100

200 20.8 16.7 25.1


203 17.5 14.2 21.4

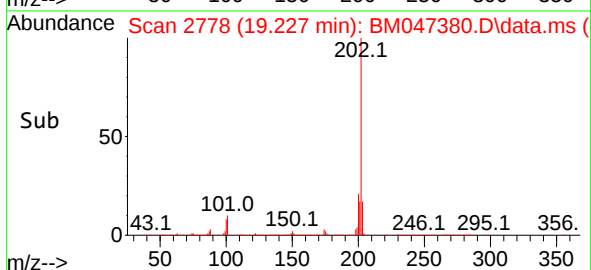



#79
 Terphenyl-d14
 Concen: 22.474 ng
 RT: 19.444 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM047380.D
 Acq: 28 Aug 2024 14:24




Instrument :
 BNA_M
 ClientSampleId :
 WC-11DL




Tgt Ion:244 Resp: 1617095
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 8.7 7.0 10.4

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024




#81
 Benzo(a)anthracene
 Concen: 17.238 ng
 RT: 21.003 min Scan# 3080
 Delta R.T. -0.000 min
 Lab File: BM047380.D
 Acq: 28 Aug 2024 14:24




Tgt Ion:228 Resp: 1439765
 Ion Ratio Lower Upper
 228 100
 226 27.7 21.4 32.0
 229 20.6 15.8 23.8

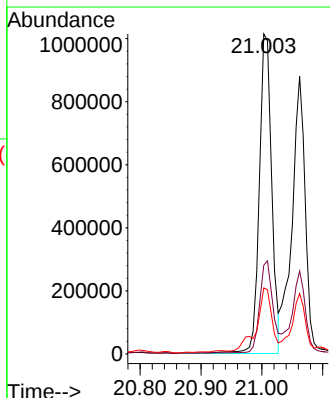



#83
Chrysene
Concen: 17.160 ng m
RT: 21.062 min Scan# 3090
Delta R.T. -0.000 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24




Instrument :
BNA_M
ClientSampleId :
WC-11DL




Tgt Ion:228 Resp: 1348178
Ion Ratio Lower Upper
228 100
226 29.8 24.0 36.0
229 21.7 15.9 23.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

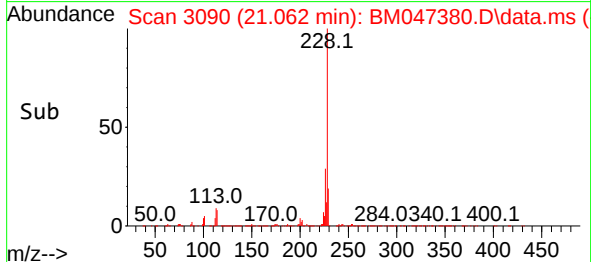


#86
Perylene-d12
Concen: 20.000 ng
RT: 23.727 min Scan# 3543
Delta R.T. 0.012 min
Lab File: BM047380.D
Acq: 28 Aug 2024 14:24



Tgt Ion:264 Resp: 1403597
Ion Ratio Lower Upper
264 100
260 23.7 19.0 28.4
265 22.5 17.8 26.6

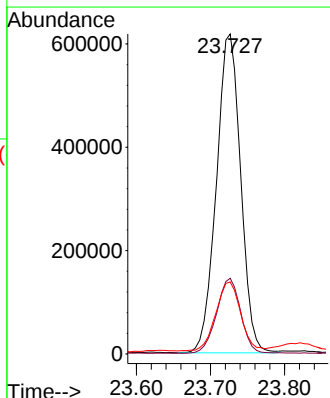



#87

Indeno(1,2,3-cd)pyrene

Concen: 7.227 ng

RT: 26.720 min Scan# 4050

Delta R.T. 0.012 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Instrument :

BNA_M

ClientSampleId :





WC-11DL

Tgt Ion:276 Resp: 635002
Ion Ratio Lower Upper
276 100
138 19.4 17.7 26.5
277 25.1 20.0 30.0

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
Supervised By :mohammad ahmed 08/30/2024

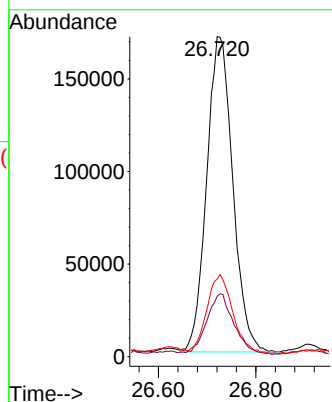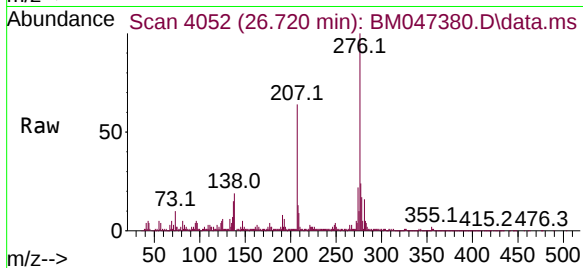

#88

Benzo(b)fluoranthene

Concen: 16.992 ng




RT: 22.885 min Scan# 3400


Delta R.T. 0.012 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Tgt Ion:252 Resp: 1391423
Ion Ratio Lower Upper
252 100
253 22.5 17.8 26.6
125 9.4 6.6 10.0

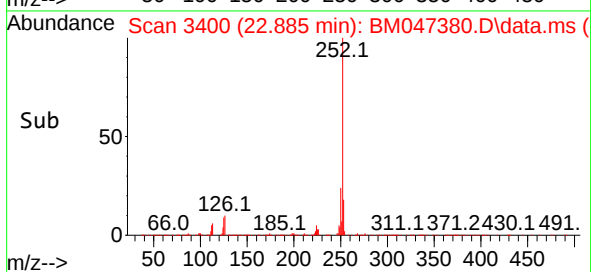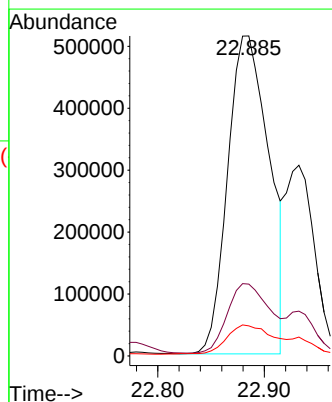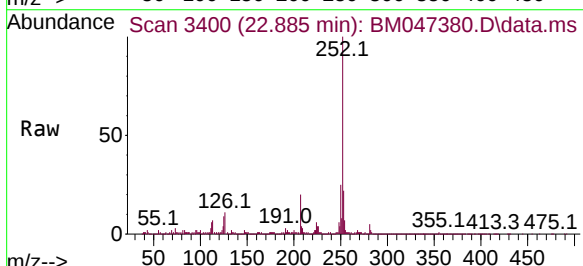



#89

Benzo(k)fluoranthene

Concen: 7.243 ng m

RT: 22.933 min Scan# 3408

Delta R.T. -0.000 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Instrument :

BNA_M

ClientSampleId :





WC-11DL

Tgt Ion:252 Resp: 56224
 Ion Ratio Lower Upper
 252 100
 253 23.5 17.5 26.3
 125 9.9 6.6 9.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/29/2024
 Supervised By :mohammad ahmed 08/30/2024

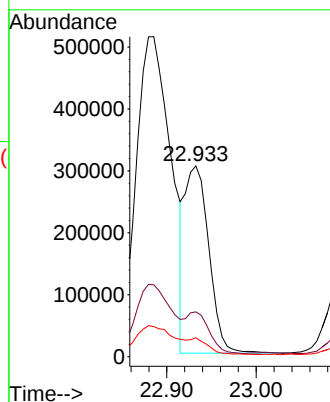

#90

Benzo(a)pyrene

Concen: 15.560 ng




RT: 23.597 min Scan# 3521


Delta R.T. 0.006 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Tgt Ion:252 Resp: 1101866
 Ion Ratio Lower Upper
 252 100
 253 23.0 17.7 26.5
 125 9.7 7.4 11.2

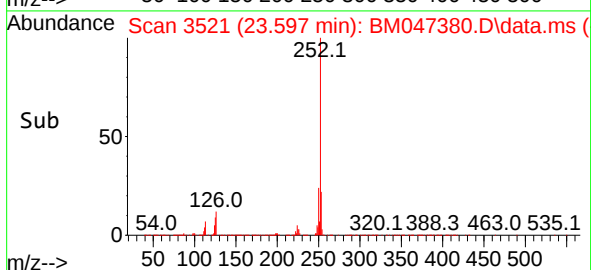



#91

Dibenzo(a,h)anthracene

Concen: 3.220 ng

RT: 26.762 min Scan# 4058

Delta R.T. 0.006 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Instrument :

BNA_M

ClientSampleId :

WC-11DL





Tgt Ion: 278 Resp: 22919

Ion	Ratio	Lower	Upper
278	100		
139	16.9	11.1	16.7
279	31.0	19.2	28.8

Manual Integrations

APPROVED

Reviewed By : Jagrut Upadhyay 08/29/2024
Supervised By : mohammad ahmed 08/30/2024

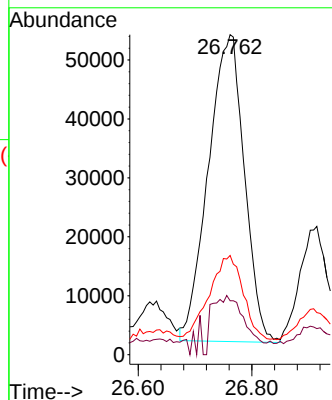

#92

Benzo(g,h,i)perylene

Concen: 8.376 ng

RT: 27.662 min Scan# 4212

Delta R.T. 0.023 min

Lab File: BM047380.D

Acq: 28 Aug 2024 14:24

Tgt Ion: 276 Resp: 619822

Ion	Ratio	Lower	Upper
276	100		
277	25.4	19.4	29.0
138	20.1	15.0	22.6

