


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082824\
Data File : BM047372.D
Acq On : 28 Aug 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

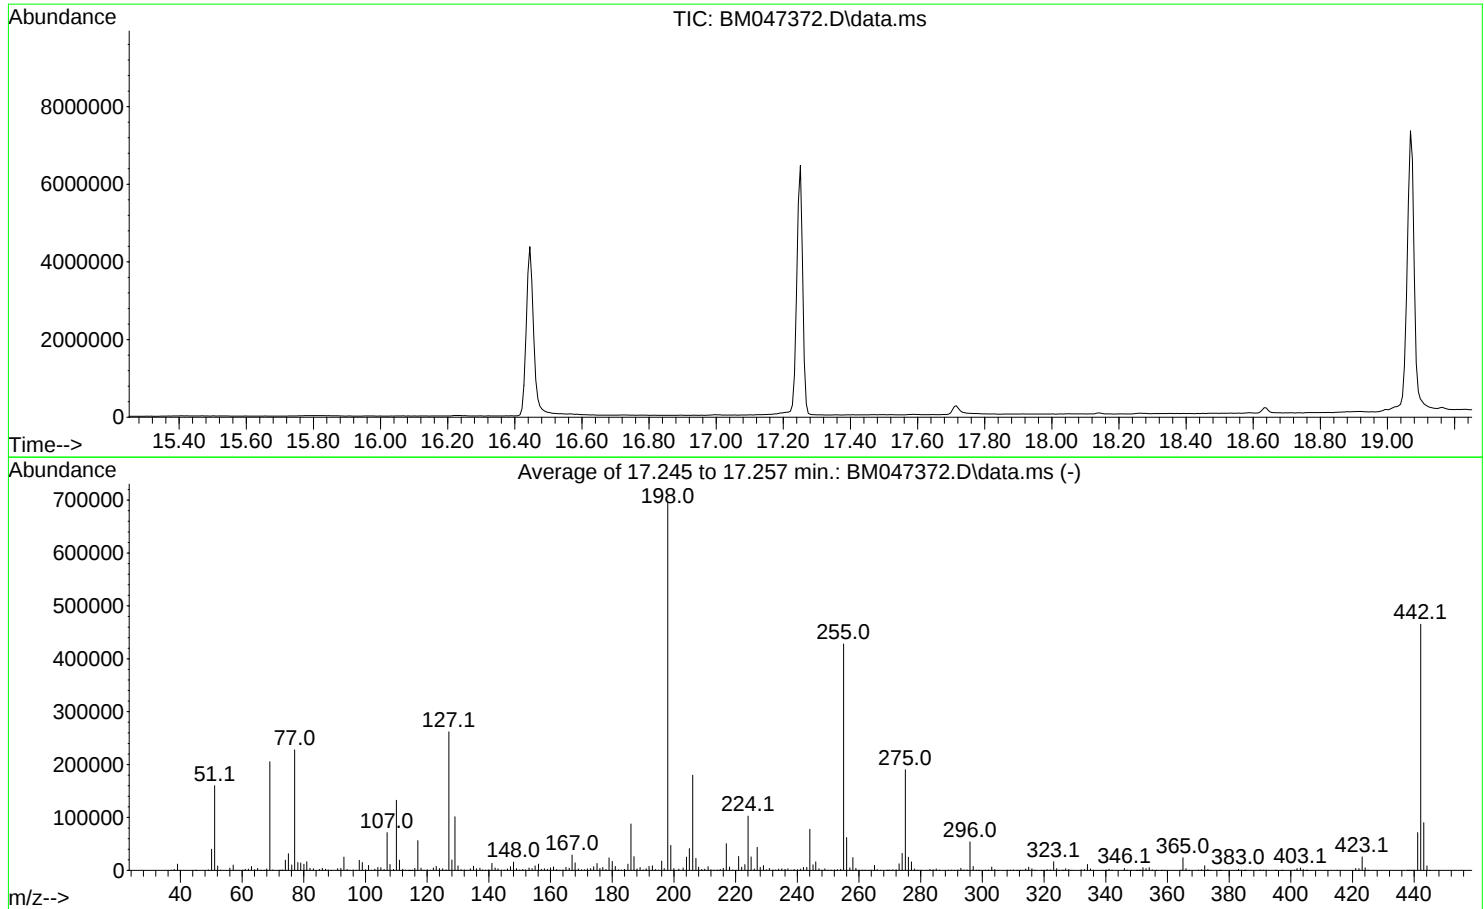

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	160121	PASS
68	69	0.00	2	1.3	2684	PASS
69	198	0.00	100	29.5	205483	PASS
70	69	0.00	2	0.4	906	PASS
127	198	10	80	37.7	262025	PASS
197	198	0.00	2	0.5	3245	PASS
198	198	100	100	100.0	695531	PASS
199	198	5	9	6.8	47208	PASS
275	198	10	60	27.3	190187	PASS
365	198	1	100	3.5	24019	PASS
441	198	0.01	100	10.3	71483	PASS
442	442	50	100	100.0	465429	PASS
443	442	15	24	19.4	90285	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/28/2024	BNA_M	<u>BM047372.D</u>
Compound Name	Response	Retention Time
DDT	2400168	20.309
DDD	49661	19.915
DDE	3877	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53538	2453706	2.18

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082824\
Data File : BM047372.D
Acq On : 28 Aug 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 28 11:53:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

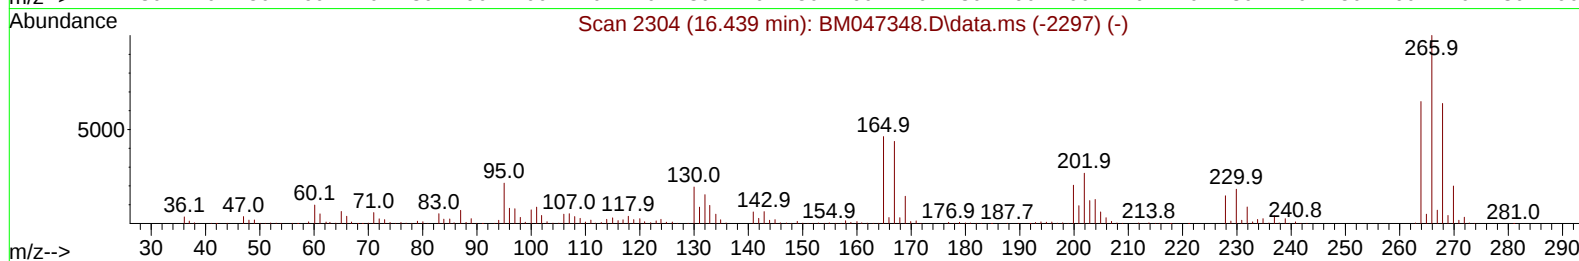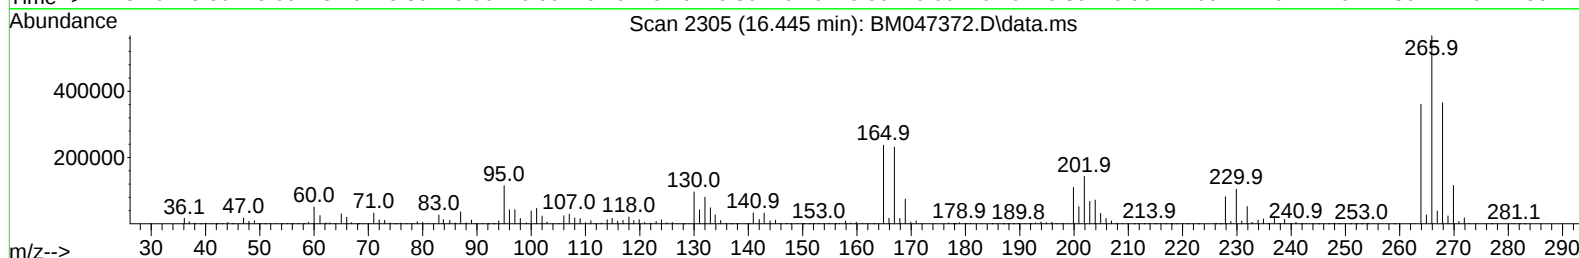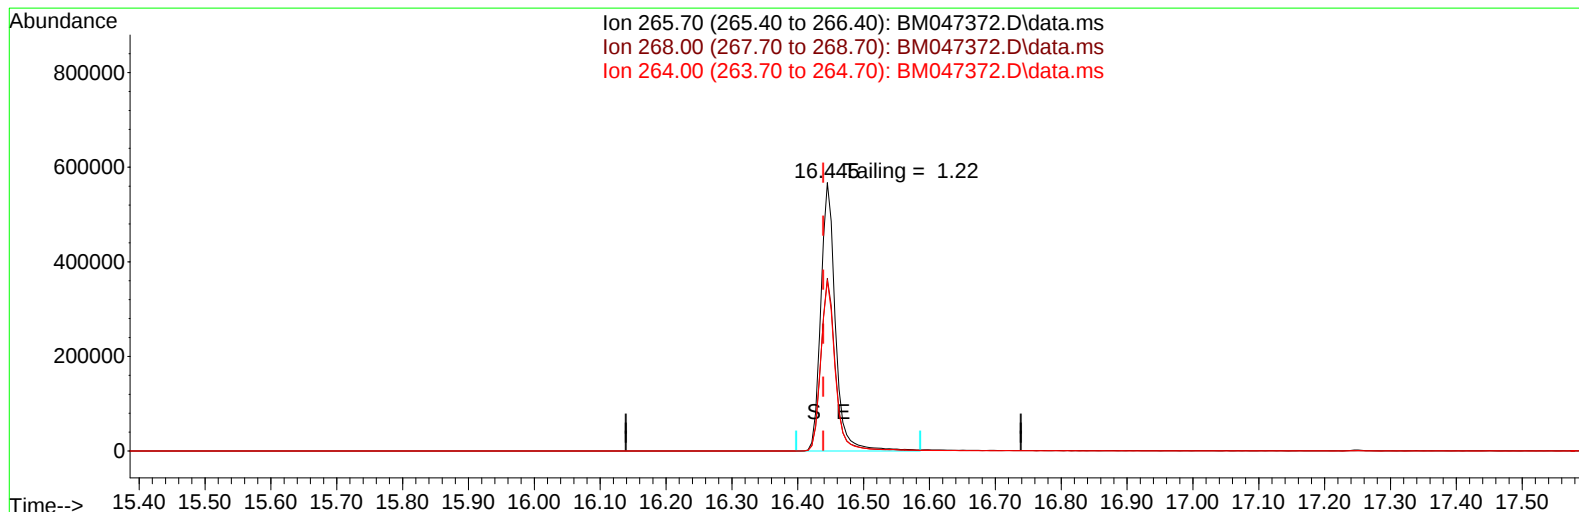

TIC: BM047372.D\data.ms

(70) Pentachlorophenol (C)

16.445min (+ 0.006) 243645.20 ng




response 877151

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.35
264.00	64.90	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082824\
Data File : BM047372.D
Acq On : 28 Aug 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 28 11:53:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

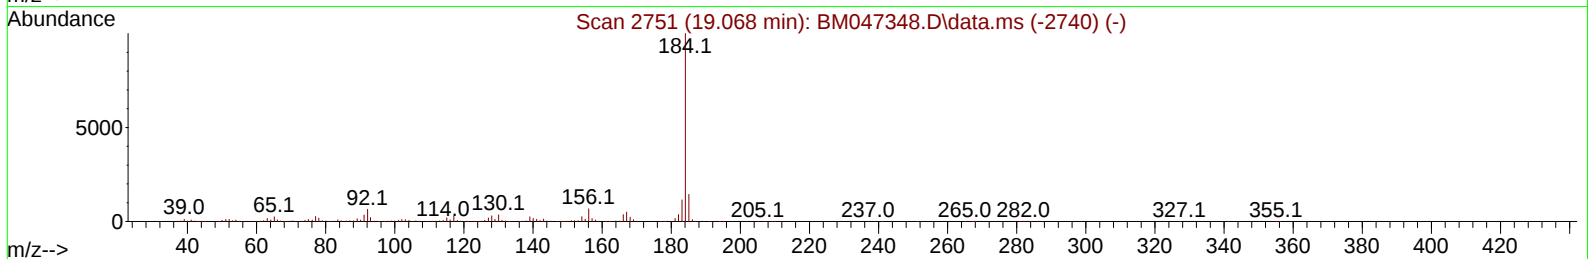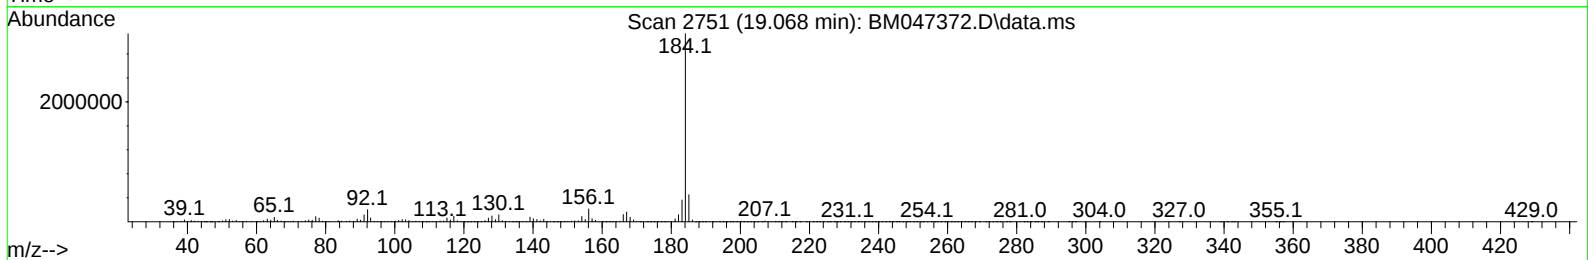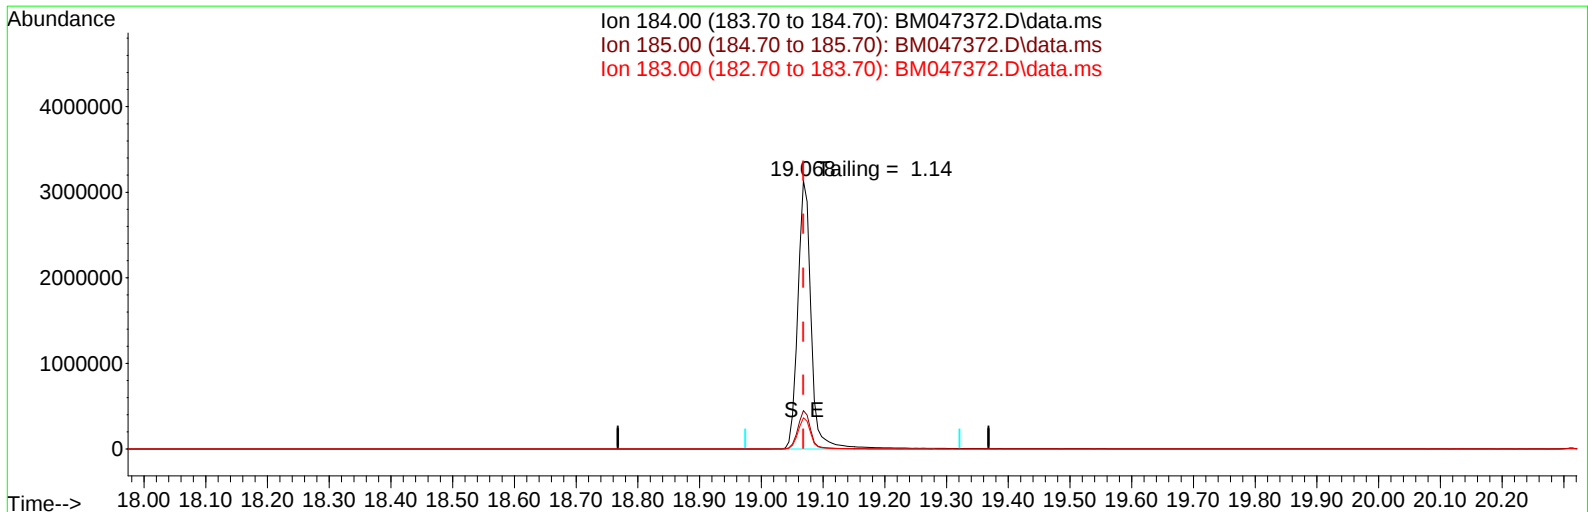

TIC: BM047372.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 161027.30 ng

response 4719982

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.35
183.00	11.50	11.62
0.00	0.00	0.00