


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082919\
 Data File : BM022402.D
 Acq On : 29 Aug 2019 11:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 16:51:32 2019

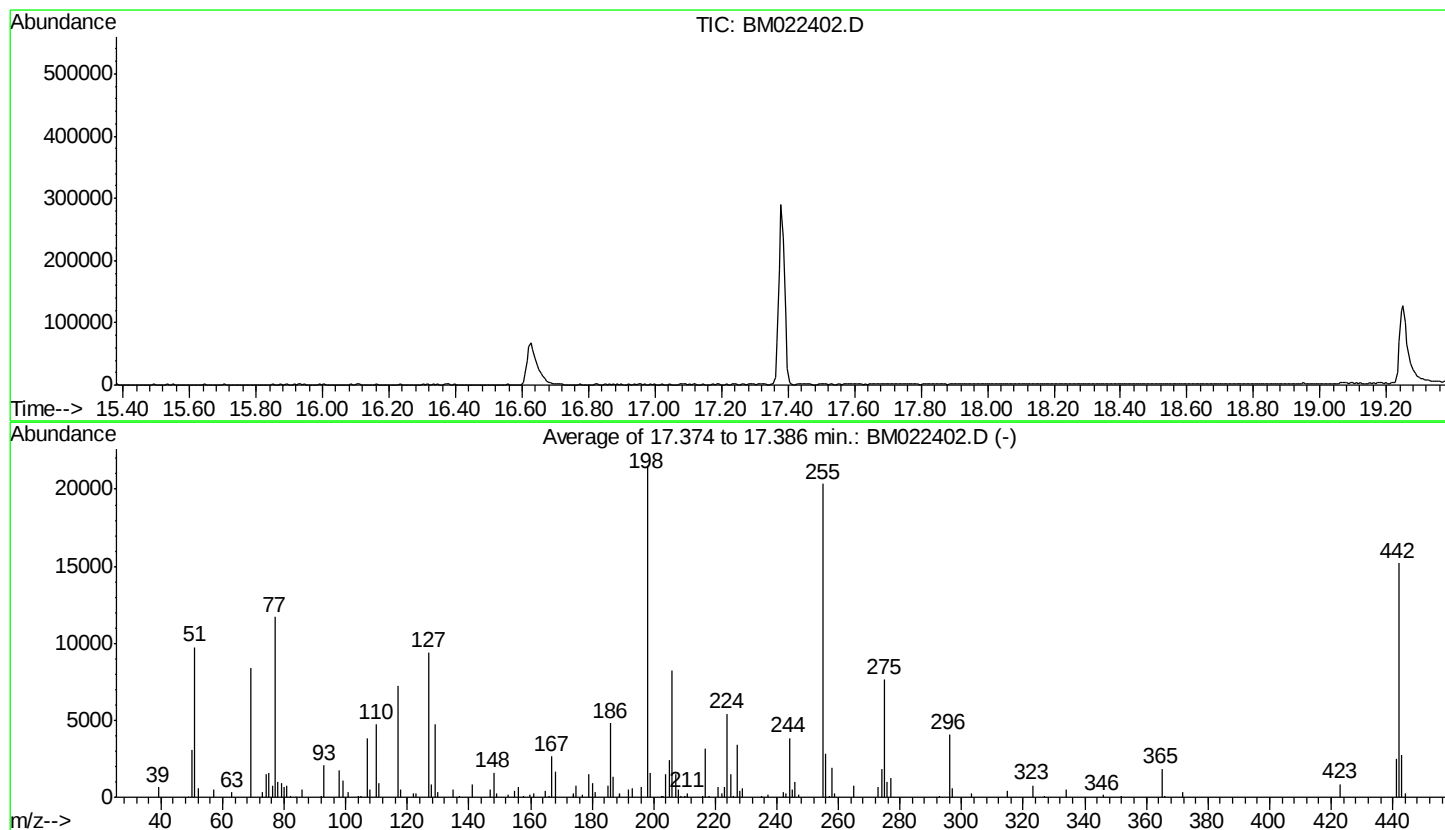

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	9745	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.9	8370	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	9381	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21538	PASS
199	198	5	9	7.3	1581	PASS
275	198	10	60	35.4	7631	PASS
365	198	1	100	8.5	1831	PASS
441	198	0.01	100	11.5	2474	PASS
442	198	50	100	70.6	15215	PASS
443	442	15	24	18.1	2747	PASS