

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041616.D
 Acq On : 31 Aug 2023 15:01
 Operator : MA/JU
 Sample : 04159-15
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHL5

Quant Time: Sep 01 02:09:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	5600	0.400	ng/ul	0.00
4) Naphthalene-d8	10.939	136	12638	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	5414	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.498	188	10087	0.400	ng/ul	0.00
17) Chrysene-d12	21.682	240	3703	0.400	ng/ul	0.00
23) Perylene-d12	24.240	264	4870	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	38002	4.598	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	4830	0.317	ng/ul	-0.01
18) Fluoranthene-d10	19.515	212	6806	0.373	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.887	202	2659	0.054	ng/ul#	1
26) Benzo(a)pyrene	24.073	252	5122	0.127	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041616.D
Acq On : 31 Aug 2023 15:01
Operator : MA/JU
Sample : 04159-15
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHL5

Quant Time: Sep 01 02:09:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration




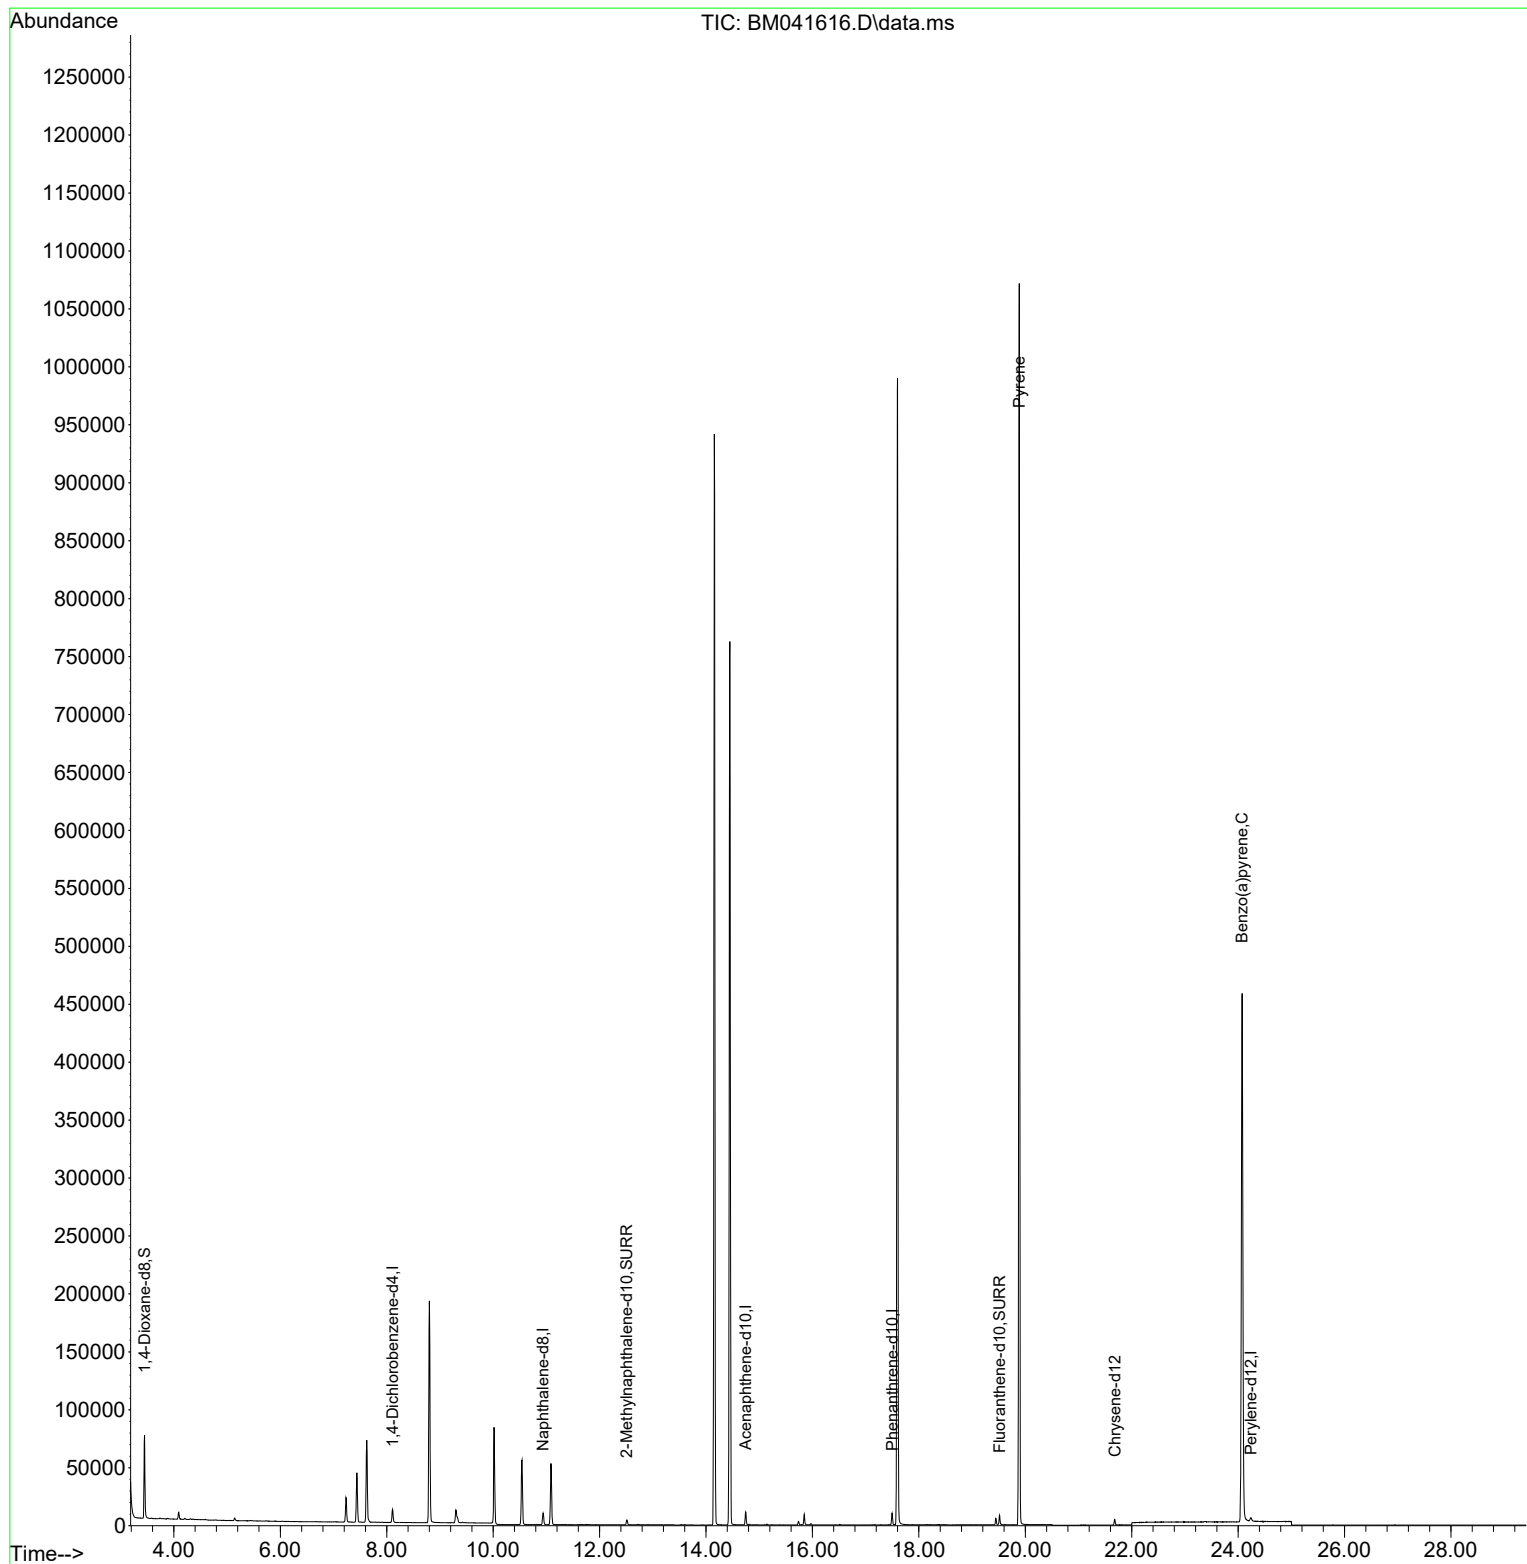


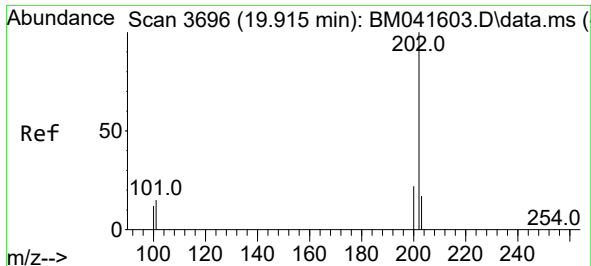

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.887 min Scan# 3690
Delta R.T. -0.037 min
Lab File: BM041616.D
Acq: 31 Aug 2023 15:01

Instrument :
BNA_M
ClientSampleId :
DCHL5

Tgt Ion:202 Resp: 2659
Ion Ratio Lower Upper
202 100
101 177.4 12.2 18.4#
100 1305.4 9.8 14.8#

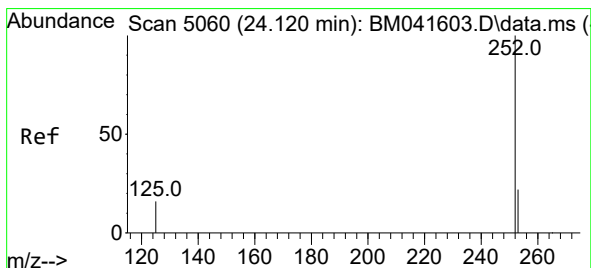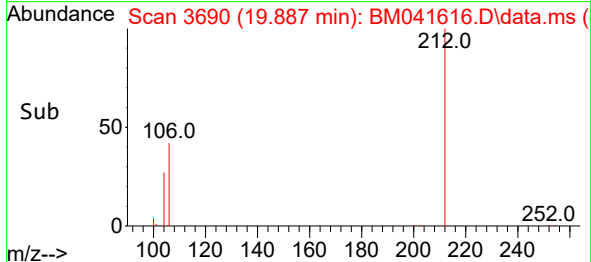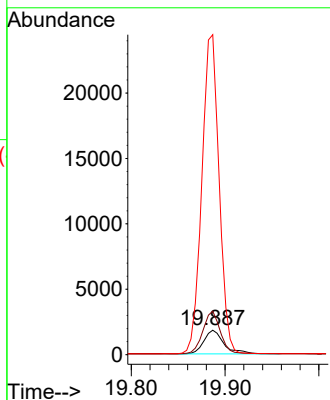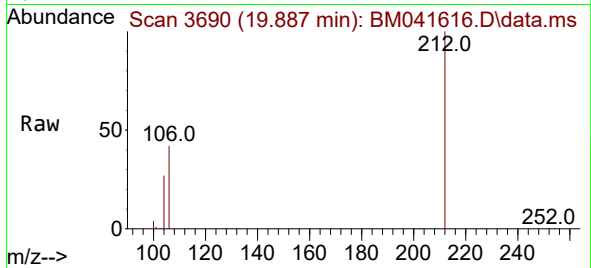

#26
Benzo(a)pyrene
Concen: 0.127 ng/ul
RT: 24.073 min Scan# 5044
Delta R.T. -0.064 min
Lab File: BM041616.D
Acq: 31 Aug 2023 15:01

Tgt Ion:252 Resp: 5122
Ion Ratio Lower Upper
252 100
253 40.5 20.9 31.3#
125 51.2 21.1 31.7#

