

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041622.D
 Acq On : 31 Aug 2023 19:20
 Operator : MA/JU
 Sample : PB155161BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK161

Quant Time: Sep 01 02:09:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	5698	0.400	ng/ul	0.00
4) Naphthalene-d8	10.939	136	13106	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	5590	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.497	188	9545	0.400	ng/ul	0.00
17) Chrysene-d12	21.679	240	2816	0.400	ng/ul	-0.01
23) Perylene-d12	24.237	264	3485	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	58294	6.932	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	5097	0.322	ng/ul	-0.01
18) Fluoranthene-d10	19.515	212	5291	0.381	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.739	166	2636	0.090	ng/ul#	12
20) Pyrene	19.887	202	2186	0.059	ng/ul#	1
26) Benzo(a)pyrene	24.070	252	3750	0.130	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041622.D
Acq On : 31 Aug 2023 19:20
Operator : MA/JU
Sample : PB155161BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK161

Quant Time: Sep 01 02:09:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration




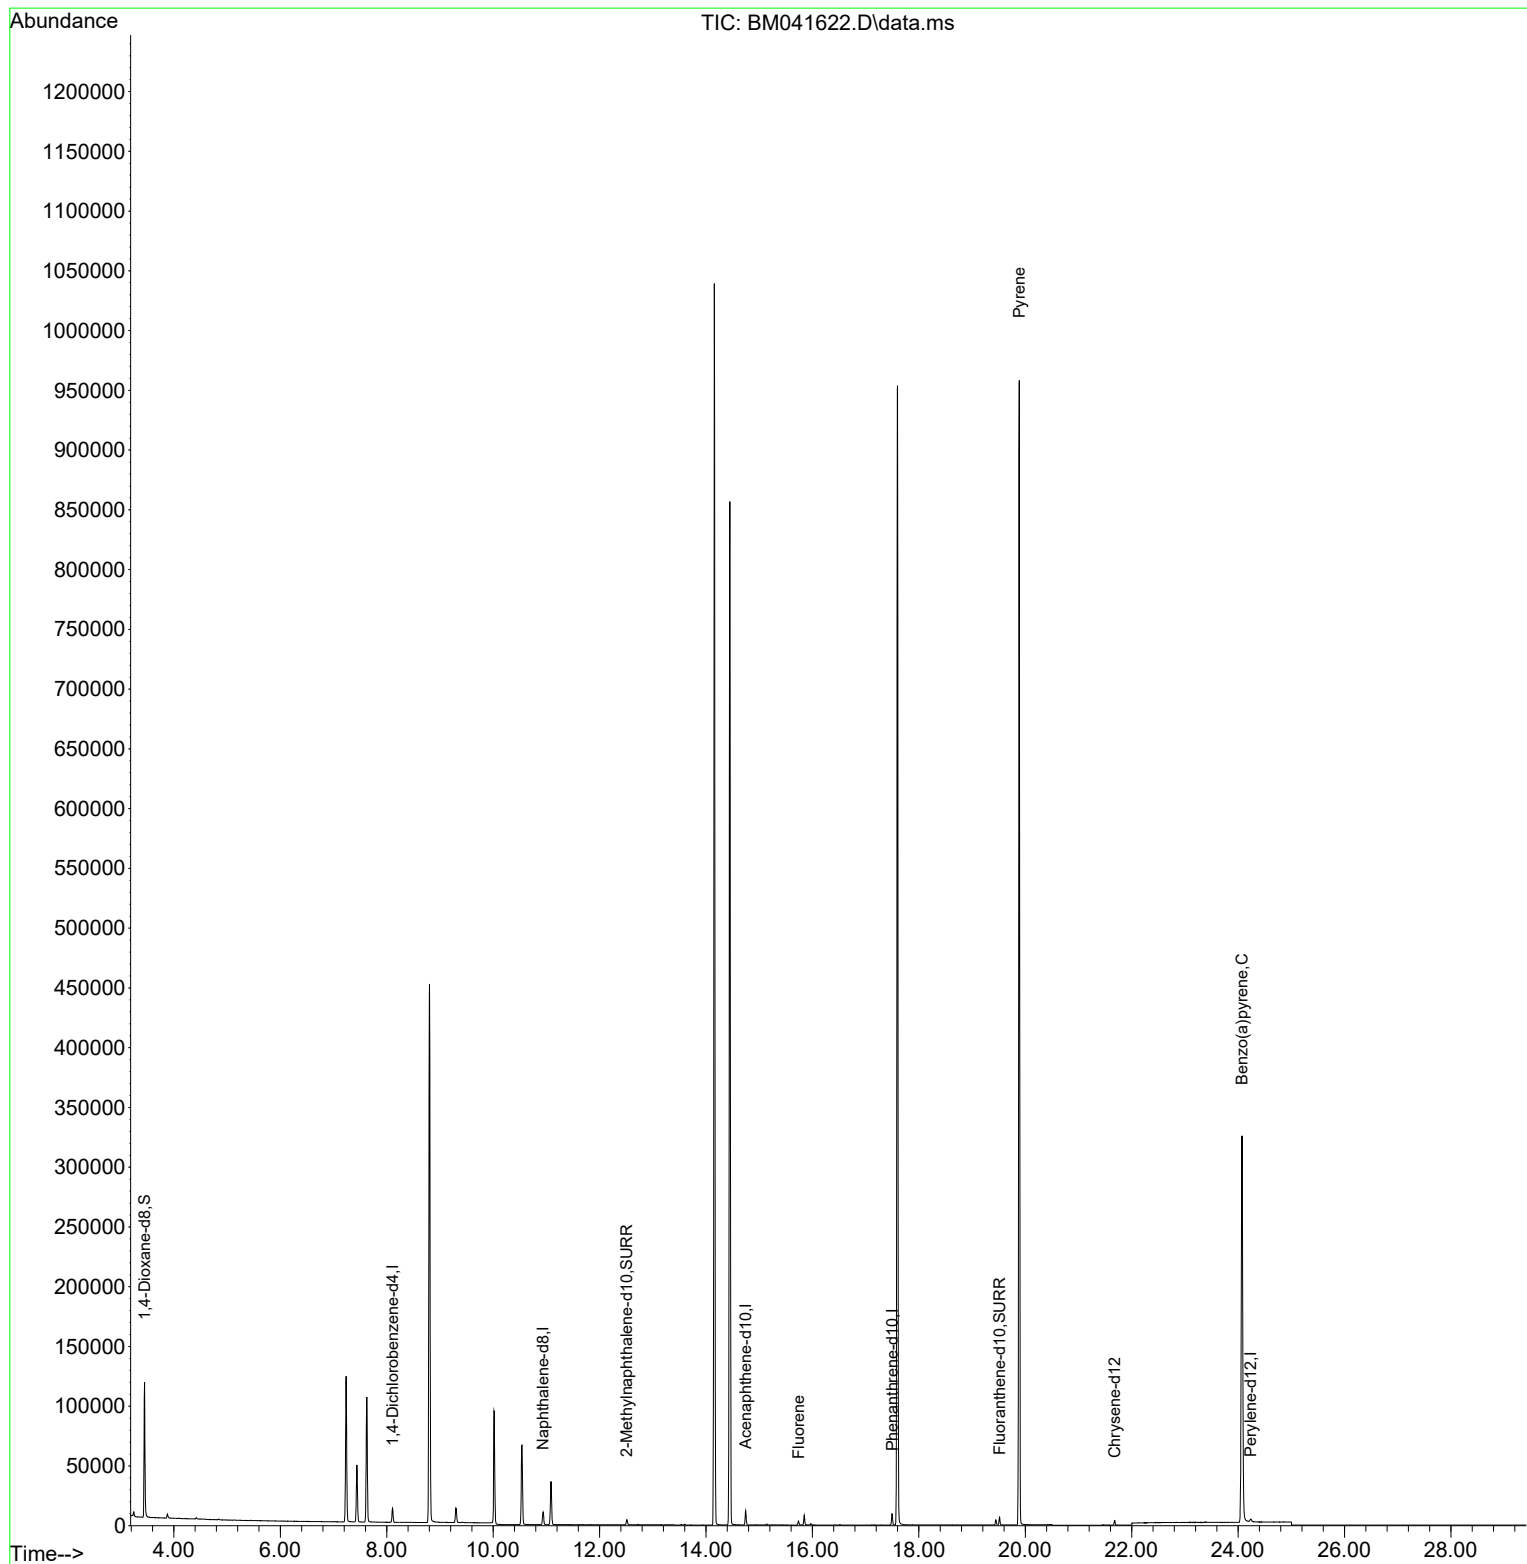


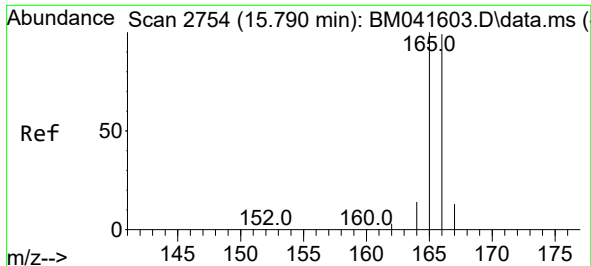

#12
 Fluorene
 Concen: 0.090 ng/ul
 RT: 15.739 min Scan# 21
 Delta R.T. -0.060 min
 Lab File: BM041622.D
 Acq: 31 Aug 2023 19:20




Instrument :
 BNA_M
 ClientSampleId :
 SBLK161


Tgt Ion:166 Resp: 2636
 Ion Ratio Lower Upper
 166 100
 165 8.5 82.2 123.2#
 167 35.5 11.5 17.3#

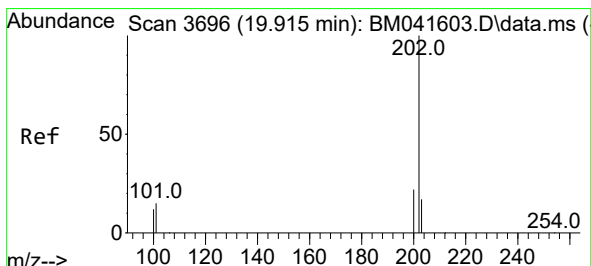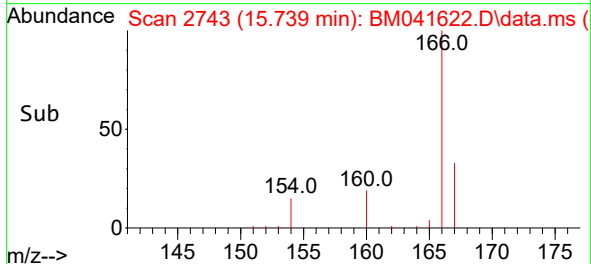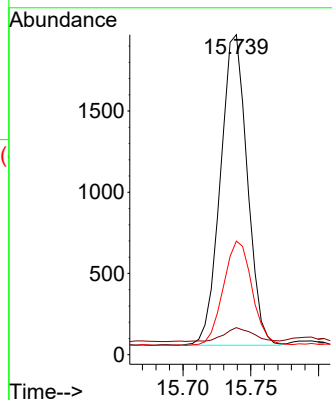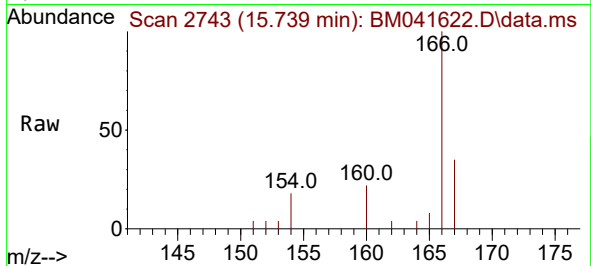

#20
 Pyrene
 Concen: 0.059 ng/ul
 RT: 19.887 min Scan# 3690
 Delta R.T. -0.037 min
 Lab File: BM041622.D
 Acq: 31 Aug 2023 19:20


Tgt Ion:202 Resp: 2186
 Ion Ratio Lower Upper
 202 100
 101 163.1 12.2 18.4#
 100 1205.0 9.8 14.8#

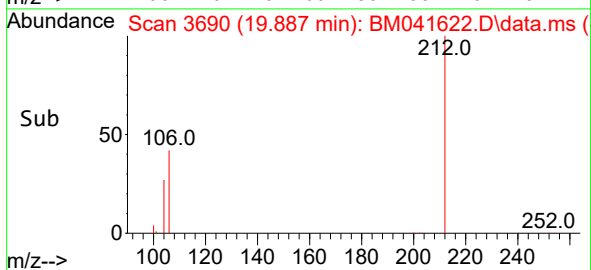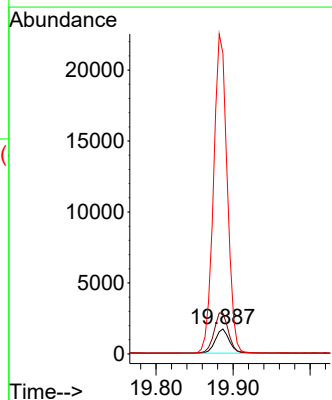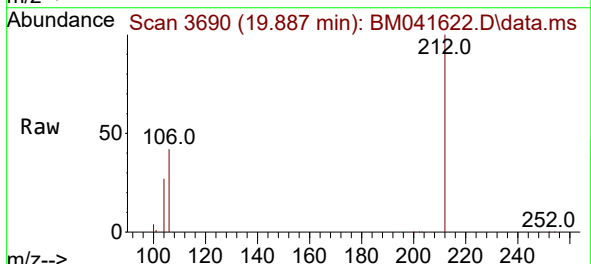

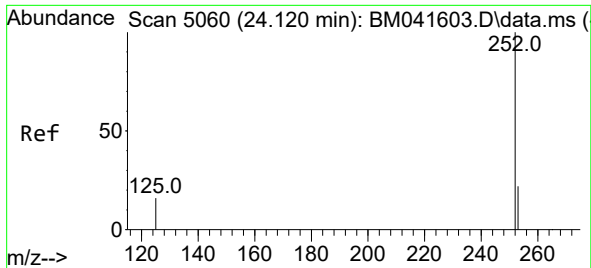

#26
Benzo(a)pyrene
Concen: 0.130 ng/ul
RT: 24.070 min Scan# 50
Delta R.T. -0.067 min
Lab File: BM041622.D
Acq: 31 Aug 2023 19:20

Instrument :
BNA_M
ClientSampleId :
SBLK161

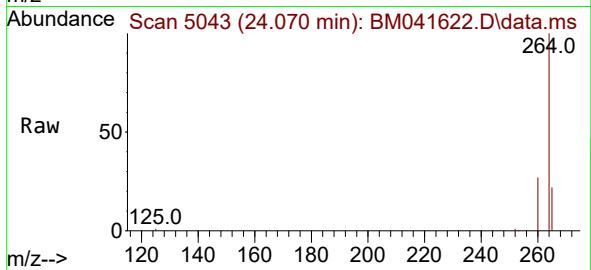

Tgt Ion:252 Resp: 3750
Ion Ratio Lower Upper
252 100
253 40.4 20.9 31.3#
125 51.3 21.1 31.7#

