

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041573.D
 Acq On : 30 Aug 2023 10:43
 Operator : MA/JU
 Sample : 04123-20
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHAU0

Quant Time: Aug 31 02:16:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	7179	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	16681	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	7335	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	13806	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	5223	0.400	ng/ul	0.00
23) Perylene-d12	24.251	264	6753	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	75413	7.118	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	7956	0.395	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	11115	0.431	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.490	88	16125	1.427	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041573.D
Acq On : 30 Aug 2023 10:43
Operator : MA/JU
Sample : 04123-20
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHAU0

Quant Time: Aug 31 02:16:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

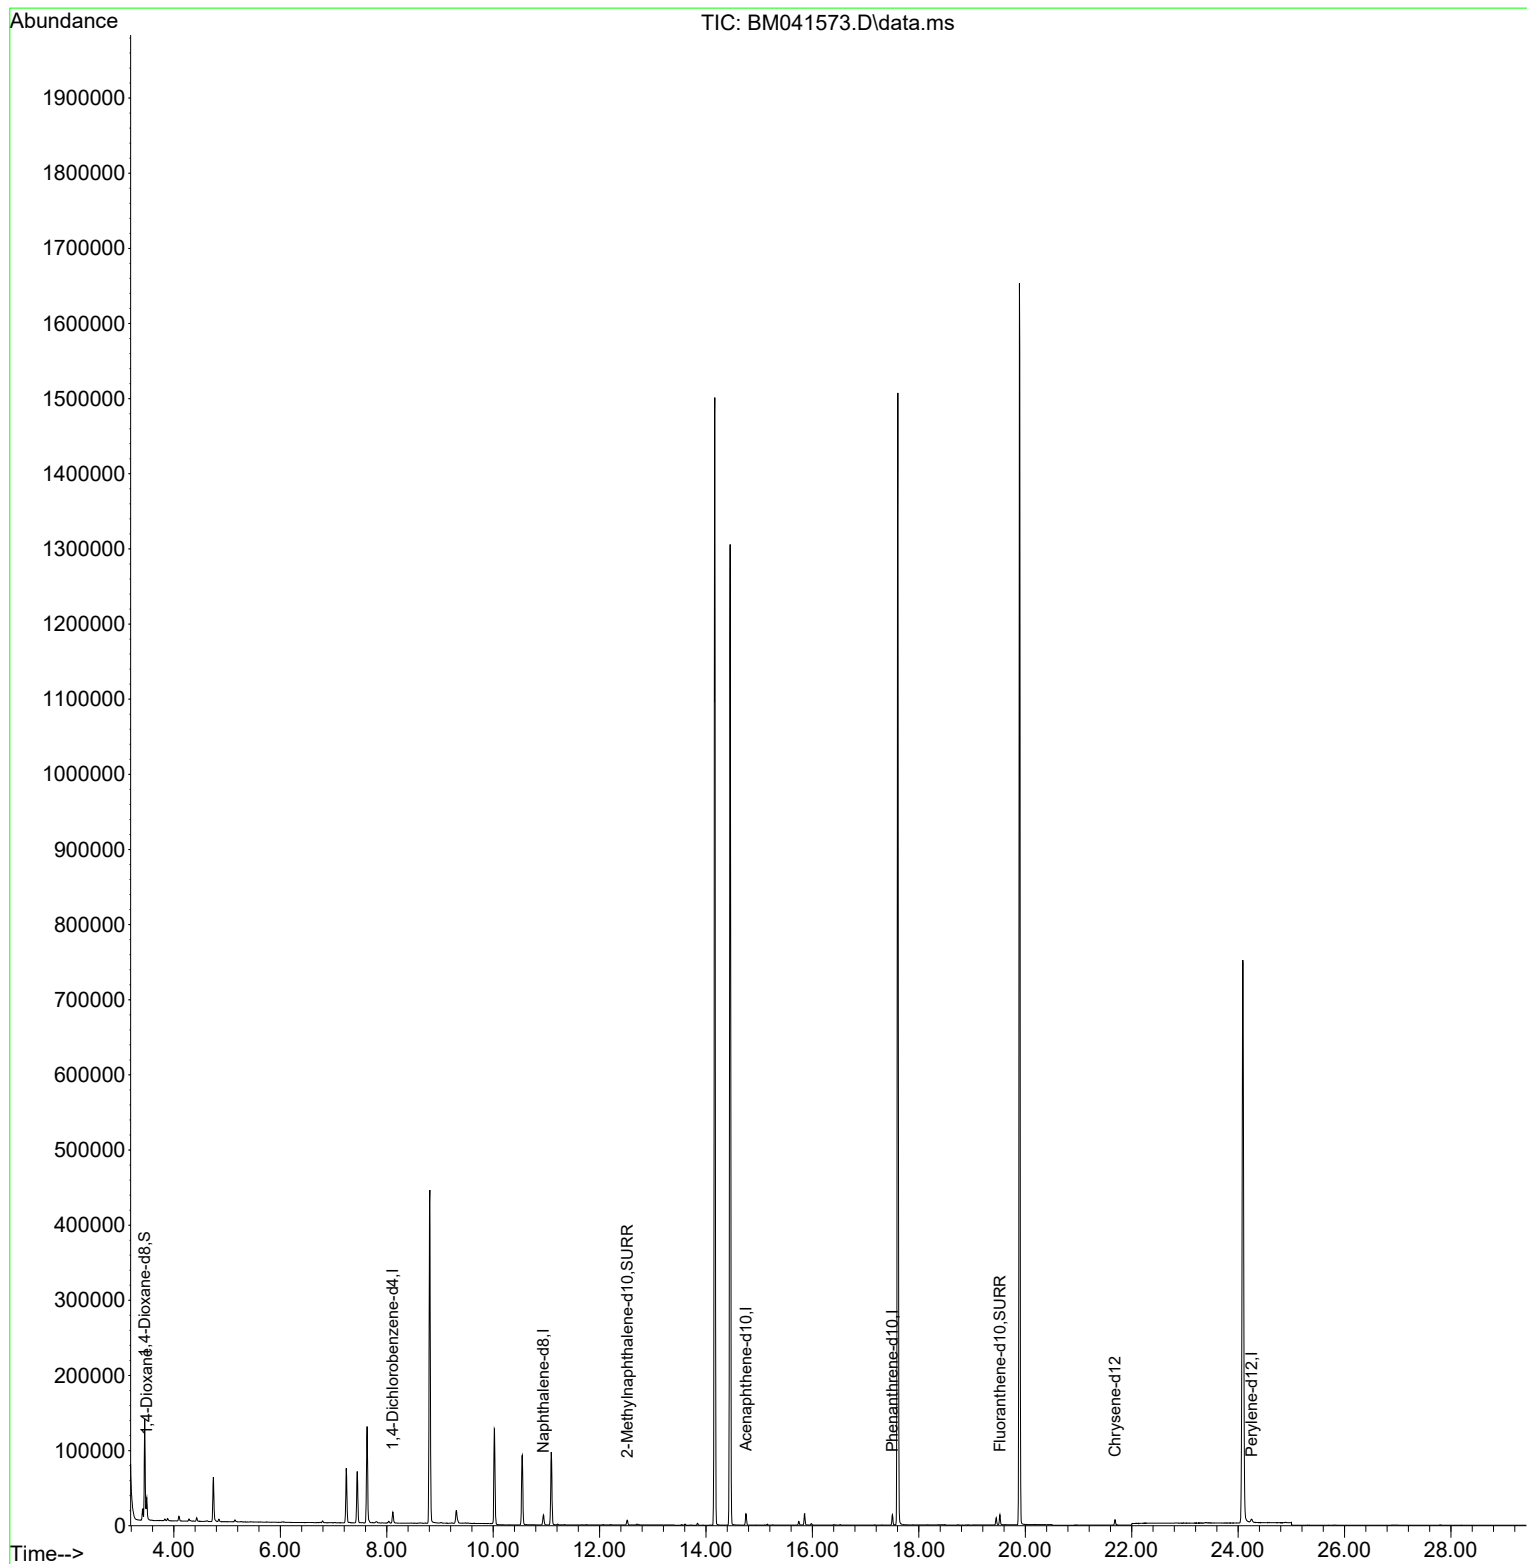

Abundance Scan 73 (3.490 min): BM041571.D\data.ms (-66)

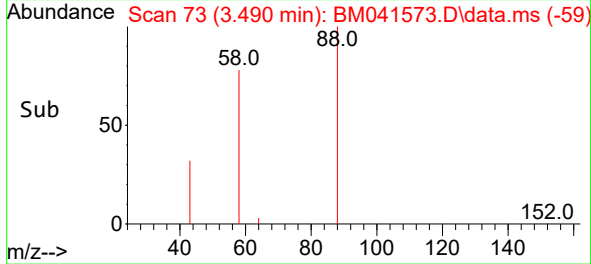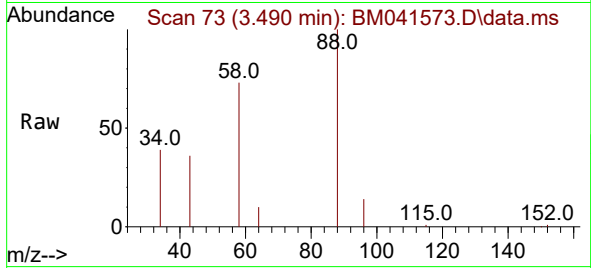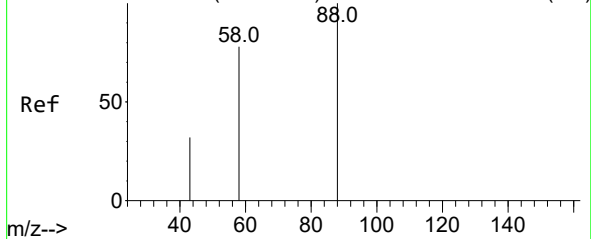

#2
1,4-Dioxane
Concen: 1.427 ng/ul
RT: 3.490 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM041573.D
Acq: 30 Aug 2023 10:43

Instrument :
BNA_M
ClientSampleId :
BHAU0

Tgt Ion:	88	Resp:	16125
Ion	Ratio	Lower	Upper
88	100		
43	36.2	46.2	69.2#
58	73.5	58.1	87.1

